


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
 Data File : BF103440.D
 Acq On : 6 Mar 2018 5:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 05 13:40:47 2018

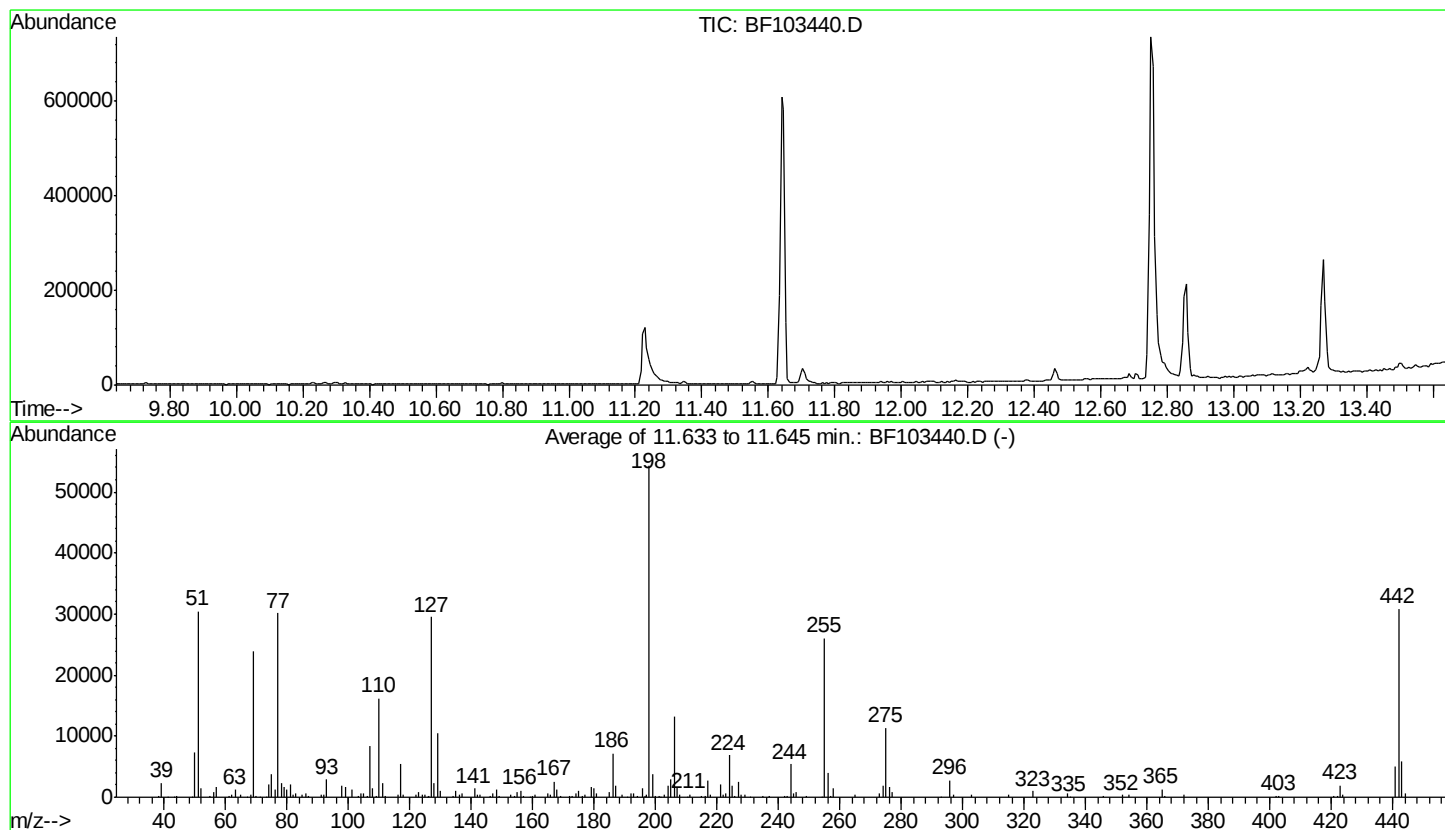

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.1	30445	PASS
68	69	0.00	2	1.4	334	PASS
69	198	0.00	100	44.0	23877	PASS
70	69	0.00	2	0.5	119	PASS
127	198	10	80	54.3	29466	PASS
197	198	0.00	2	0.8	413	PASS
198	198	100	100	100.0	54304	PASS
199	198	5	9	6.9	3754	PASS
275	198	10	60	20.9	11323	PASS
365	198	1	100	2.4	1319	PASS
441	443	0.01	100	83.1	4938	PASS
442	198	50	100	56.8	30867	PASS
443	442	15	24	19.2	5941	PASS