


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030519\
Data File : BF112847.D
Acq On : 5 Mar 2019 11:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 01 15:40:43 2019

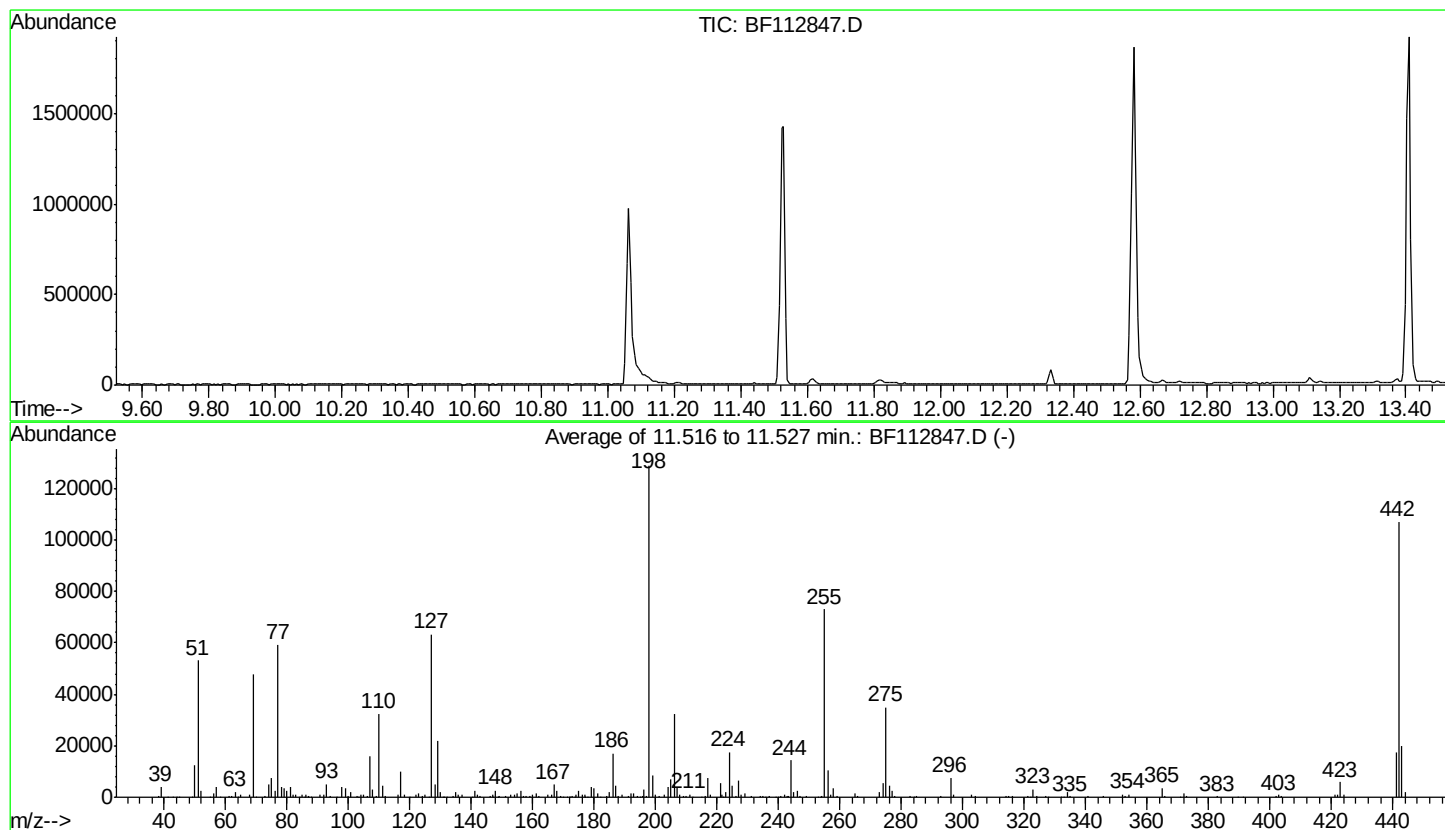

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	53162	PASS
68	69	0.00	2	1.7	790	PASS
69	198	0.00	100	37.0	47664	PASS
70	69	0.00	2	0.5	258	PASS
127	198	10	80	49.2	63325	PASS
197	198	0.00	2	0.4	565	PASS
198	198	100	100	100.0	128824	PASS
199	198	5	9	6.7	8600	PASS
275	198	10	60	27.2	35022	PASS
365	198	1	100	2.8	3561	PASS
441	198	0.01	100	13.6	17581	PASS
442	198	50	100	83.1	107082	PASS
443	442	15	24	18.4	19752	PASS