
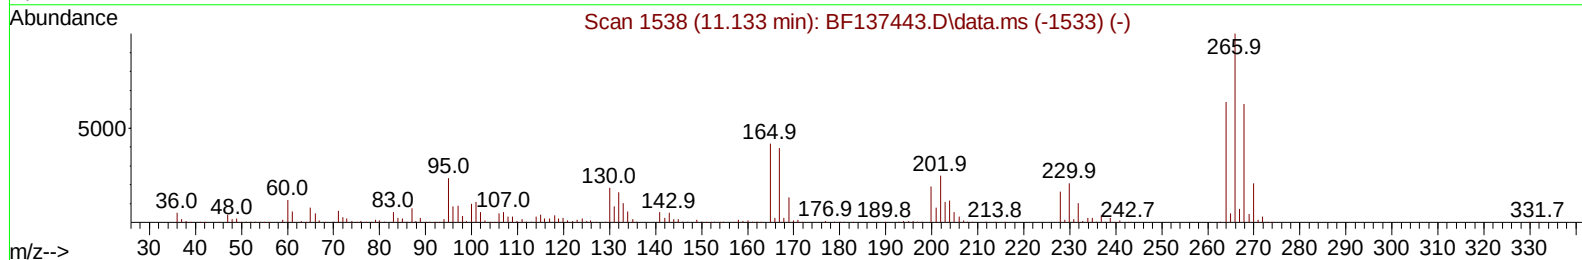
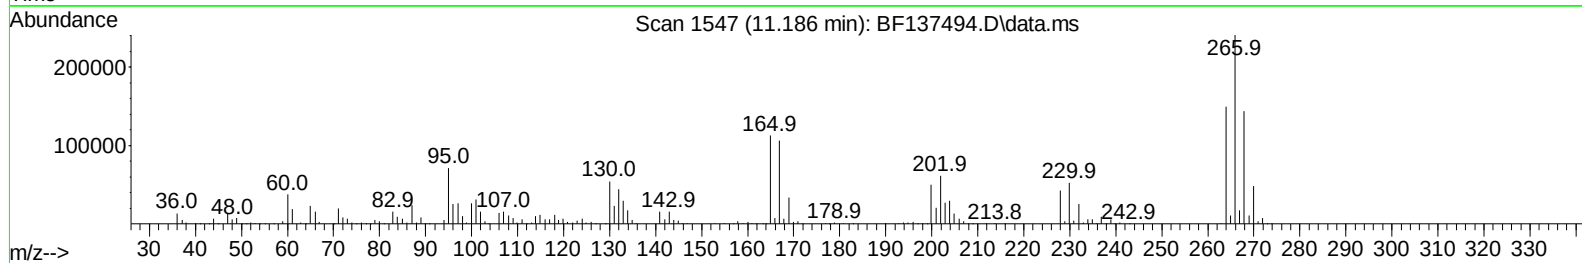


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF030524\  
Data File : BF137494.D  
Acq On : 05 Mar 2024 11:52  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 13:16:48 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF022924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 04 00:26:53 2024  
Response via : Initial Calibration

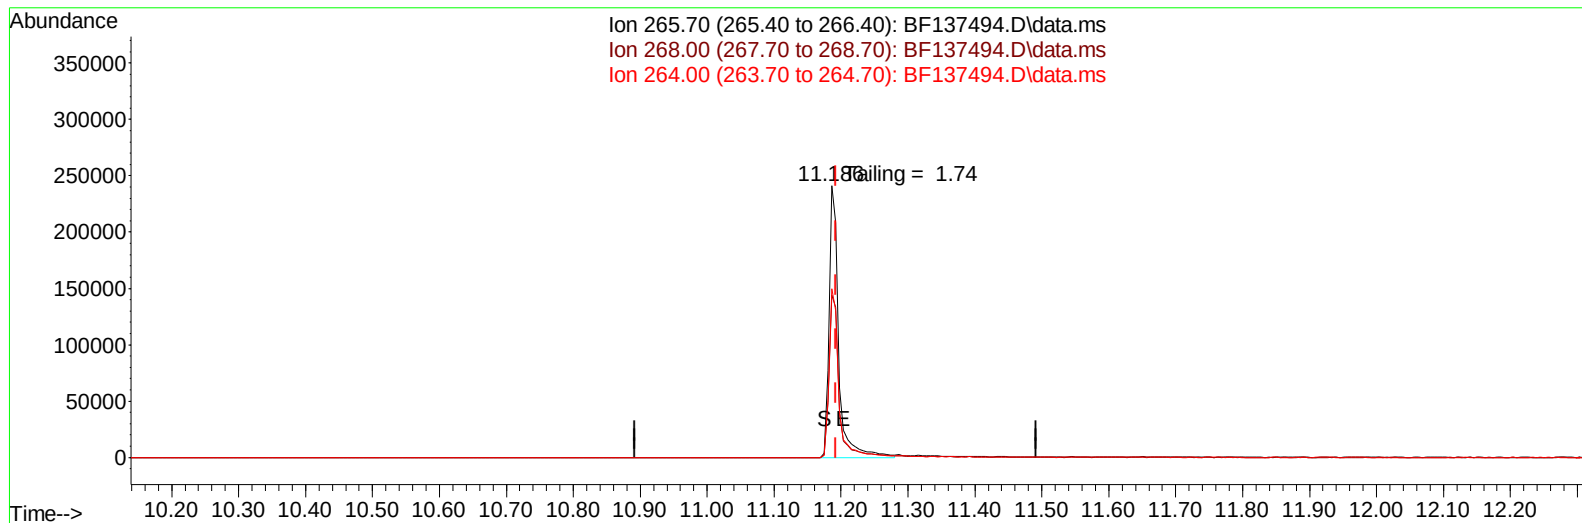




TIC: BF137494.D\data.ms

**(70) Pentachlorophenol (C)****11.186min (-0.006) 32717.20 ng****response 247385**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.70  | 59.81  |
| 264.00 | 63.60  | 62.07  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF030524\  
 Data File : BF137494.D  
 Acq On : 05 Mar 2024 11:52  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 13:16:48 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF022924.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Mar 04 00:26:53 2024  
 Response via : Initial Calibration

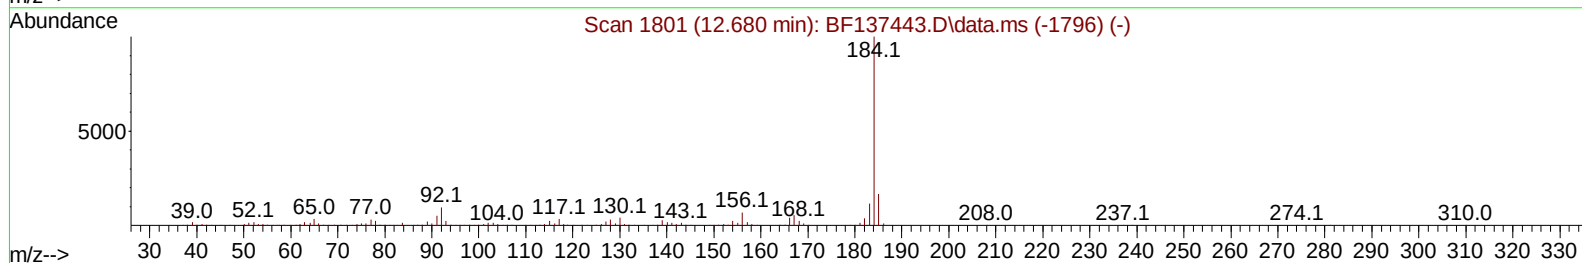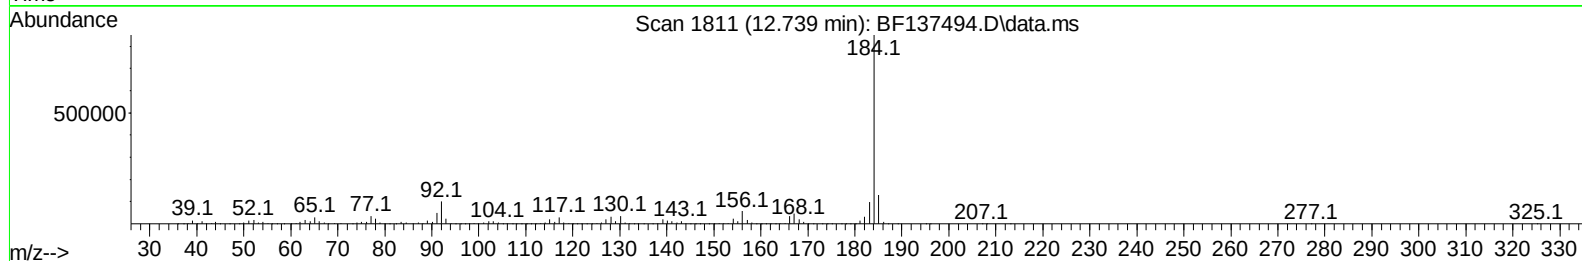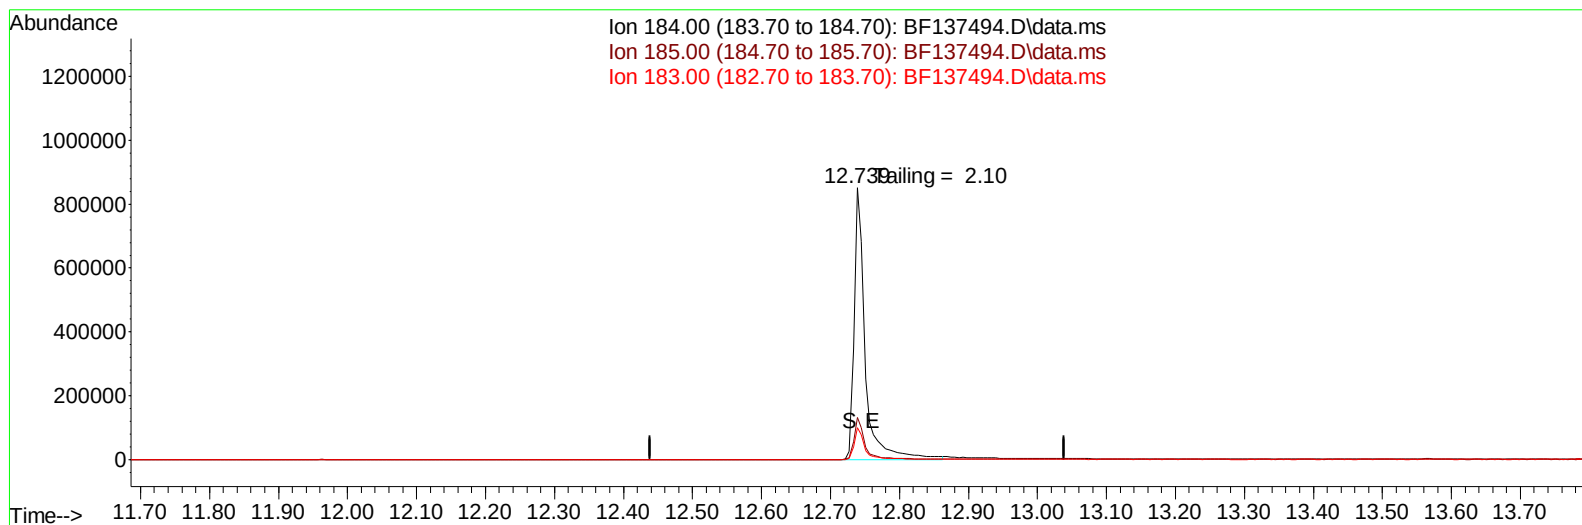

TIC: BF137494.D\data.ms

**(77) Benzidine**

12.739min (-12.739) 0.00 ng

response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 184.00 | 100.00 | 0.00  |
| 185.00 | 16.50  | 0.00# |
| 183.00 | 11.60  | 0.00# |
| 0.00   | 0.00   | 0.00  |