

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030524\
 Data File : BF137496.D
 Acq On : 05 Mar 2024 12:53
 Operator : CG\JU
 Sample : PB159421BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB159421BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.222	19	23	29	rVB	67219	93477	1.01%	0.171%
2	5.151	517	521	530	rBV	82965	131344	1.42%	0.240%
3	5.522	579	584	587	rBV	6247010	7093194	76.48%	12.940%
4	6.504	745	751	754	rBV	6230273	7379141	79.56%	13.461%
5	6.857	808	811	825	rBV	1822589	1557502	16.79%	2.841%
6	7.422	901	907	910	rBV	4563088	4918003	53.03%	8.972%
7	8.133	1023	1028	1050	rBV	2058618	2209033	23.82%	4.030%
8	9.216	1205	1212	1215	rBV	7807581	8272308	89.19%	15.091%
9	9.886	1321	1326	1343	rBV	2793081	2557190	27.57%	4.665%
10	10.686	1457	1462	1465	rBV	4957719	4606106	49.66%	8.403%
11	11.380	1577	1580	1604	rBV	2686329	2612472	28.17%	4.766%
12	12.992	1848	1854	1857	rBV	8516090	9274872	100.00%	16.920%
13	14.045	2029	2033	2046	rBV	2130698	2046170	22.06%	3.733%
14	15.574	2287	2293	2301	rBV	1148765	1543897	16.65%	2.816%
15	15.639	2301	2304	2313	rVB	89589	140648	1.52%	0.257%
16	16.121	2382	2386	2397	rVB2	79857	149981	1.62%	0.274%
17	16.692	2477	2483	2494	rVB2	66785	133922	1.44%	0.244%
18	17.362	2591	2597	2606	rVB3	40001	98168	1.06%	0.179%




Sum of corrected areas: 54817428

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030524\
Data File : BF137496.D
Acq On : 05 Mar 2024 12:53
Operator : CG\JU
Sample : PB159421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159421BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

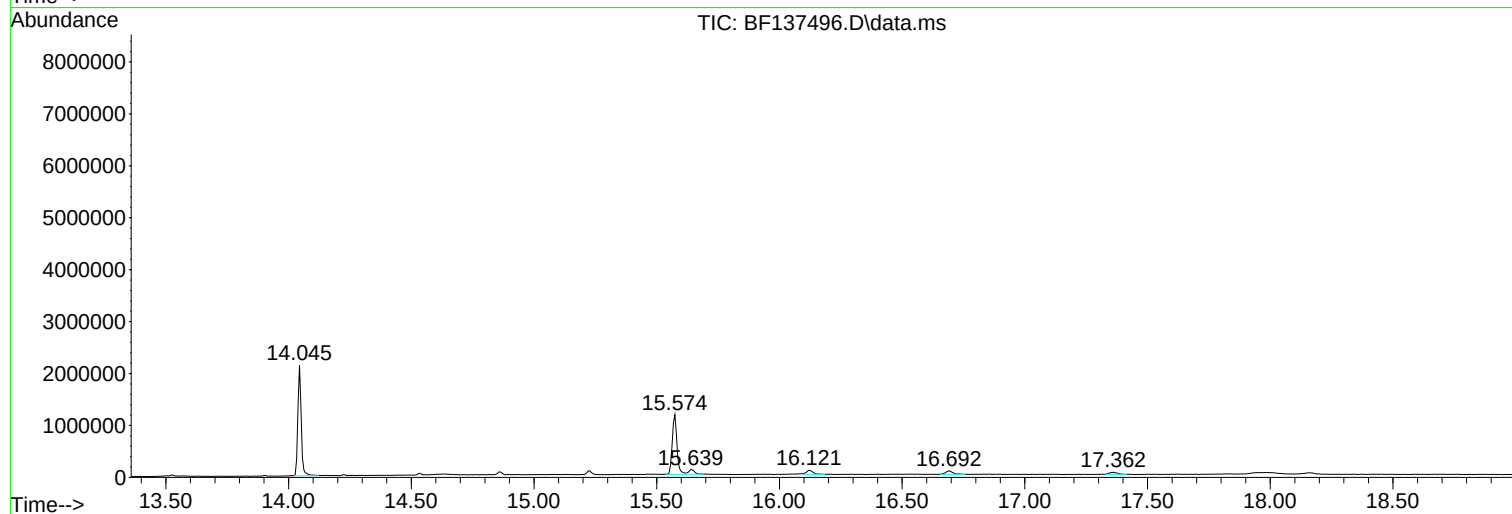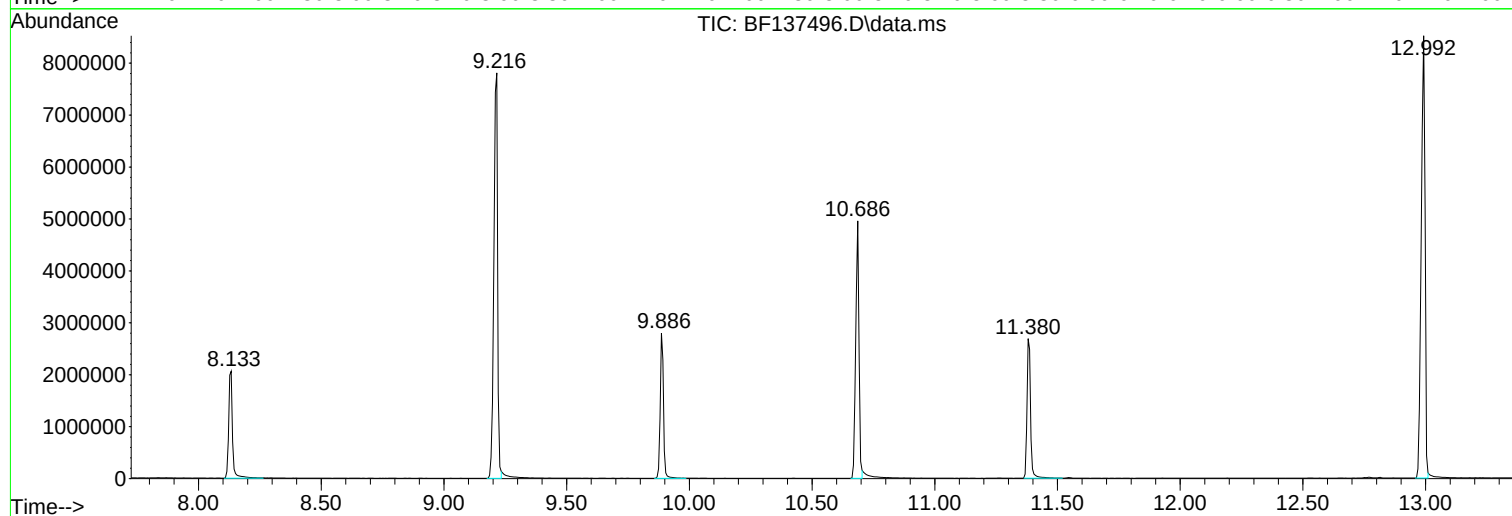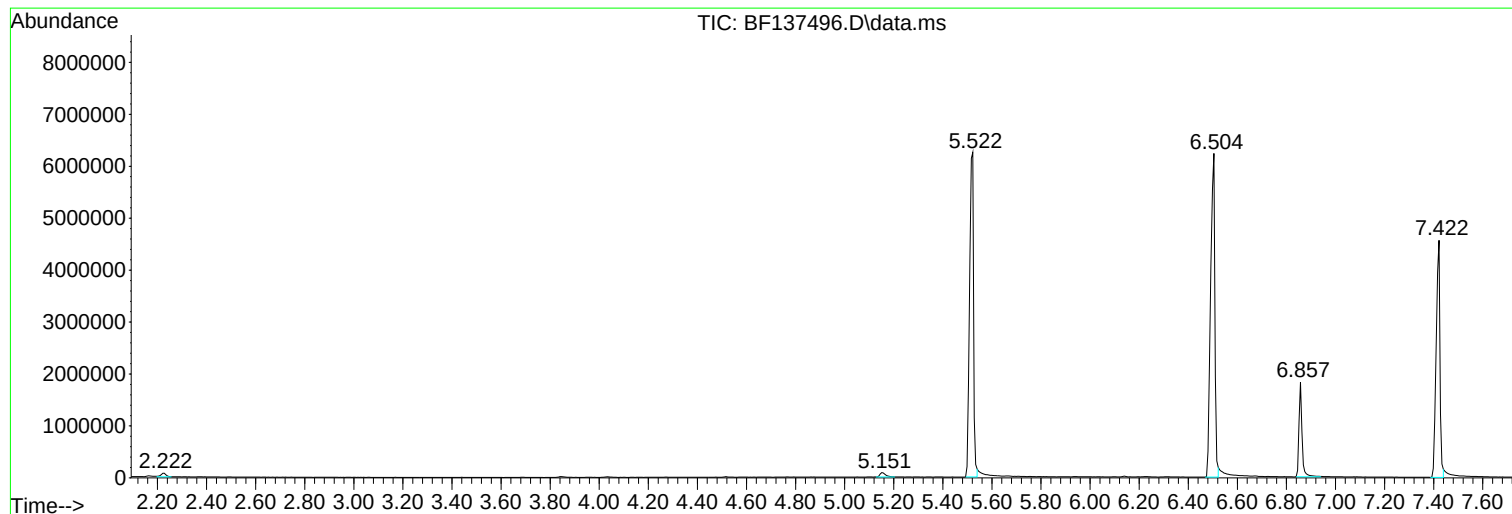

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030524\
Data File : BF137496.D
Acq On : 05 Mar 2024 12:53
Operator : CG\JU
Sample : PB159421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159421BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030524\
Data File : BF137496.D
Acq On : 05 Mar 2024 12:53
Operator : CG\JU
Sample : PB159421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159421BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------