


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030524\
Data File : BF137494.D
Acq On : 05 Mar 2024 11:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 06 00:07:28 2024

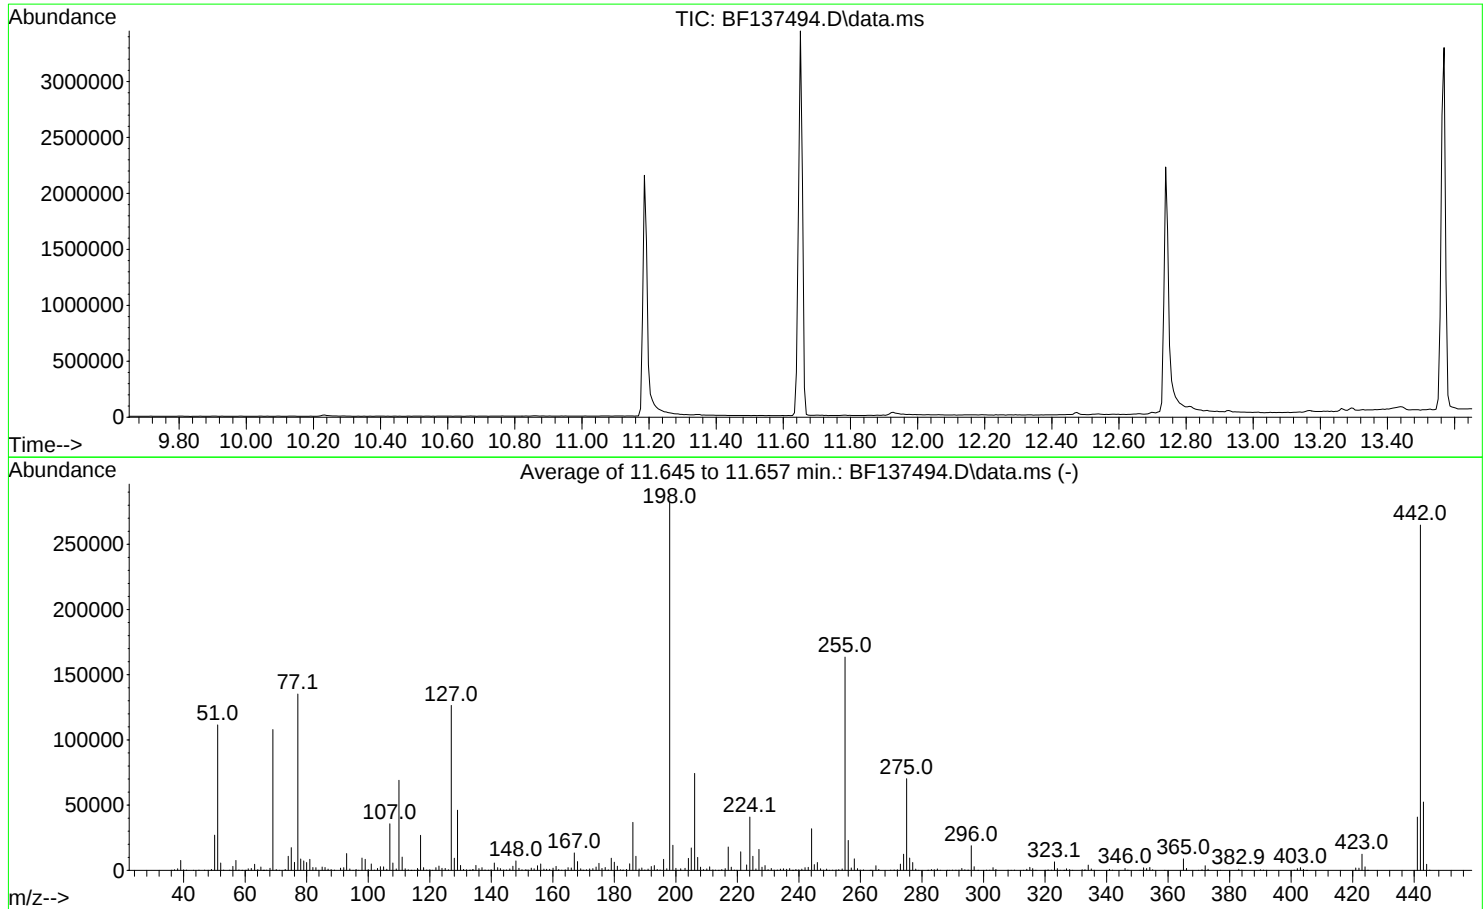




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	111537	PASS
68	69	0.00	2	1.4	1564	PASS
69	198	0.00	100	38.3	107957	PASS
70	69	0.00	2	0.6	673	PASS
127	198	10	80	44.8	126445	PASS
197	198	0.00	2	0.5	1287	PASS
198	198	100	100	100.0	282027	PASS
199	198	5	9	6.8	19248	PASS
275	198	10	60	24.9	70347	PASS
365	198	1	100	3.1	8816	PASS
441	198	0.01	100	14.5	40896	PASS
442	442	50	100	100.0	264779	PASS
443	442	15	24	19.8	52424	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030524\
Data File : BF137494.D
Acq On : 05 Mar 2024 11:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 05 13:16:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 00:26:53 2024
Response via : Initial Calibration

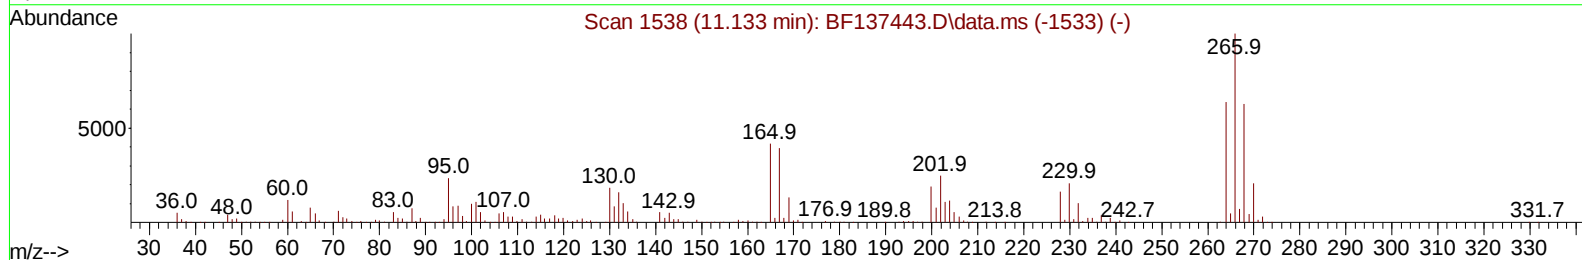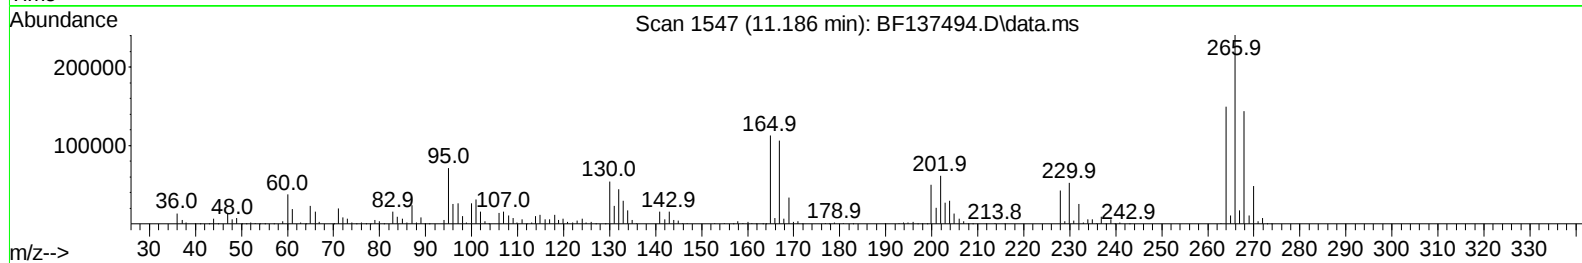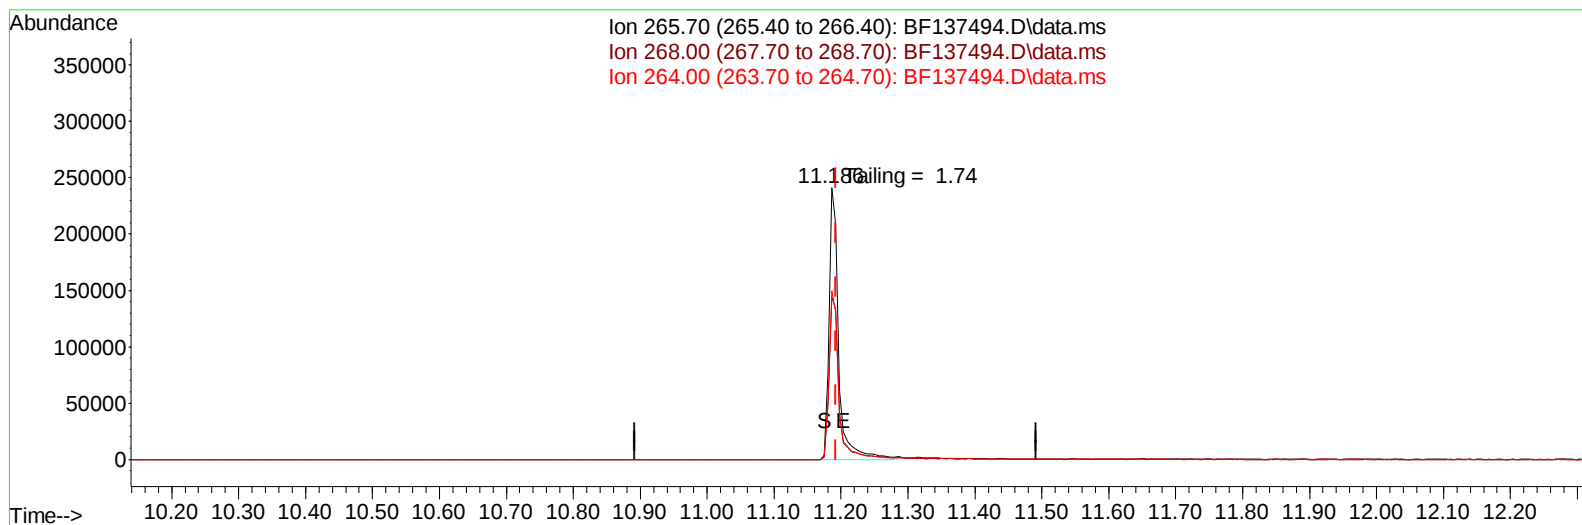

TIC: BF137494.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 32717.20 ng




response 247385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	59.81
264.00	63.60	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030524\
Data File : BF137494.D
Acq On : 05 Mar 2024 11:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 05 13:16:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 00:26:53 2024
Response via : Initial Calibration

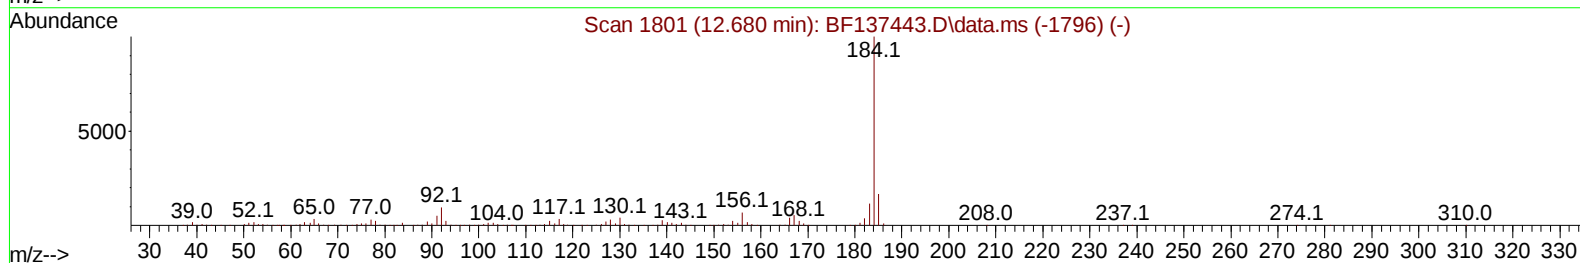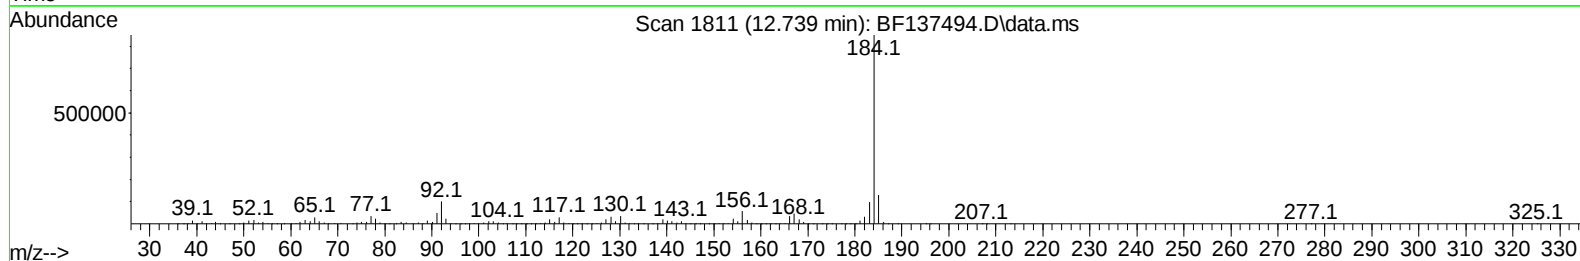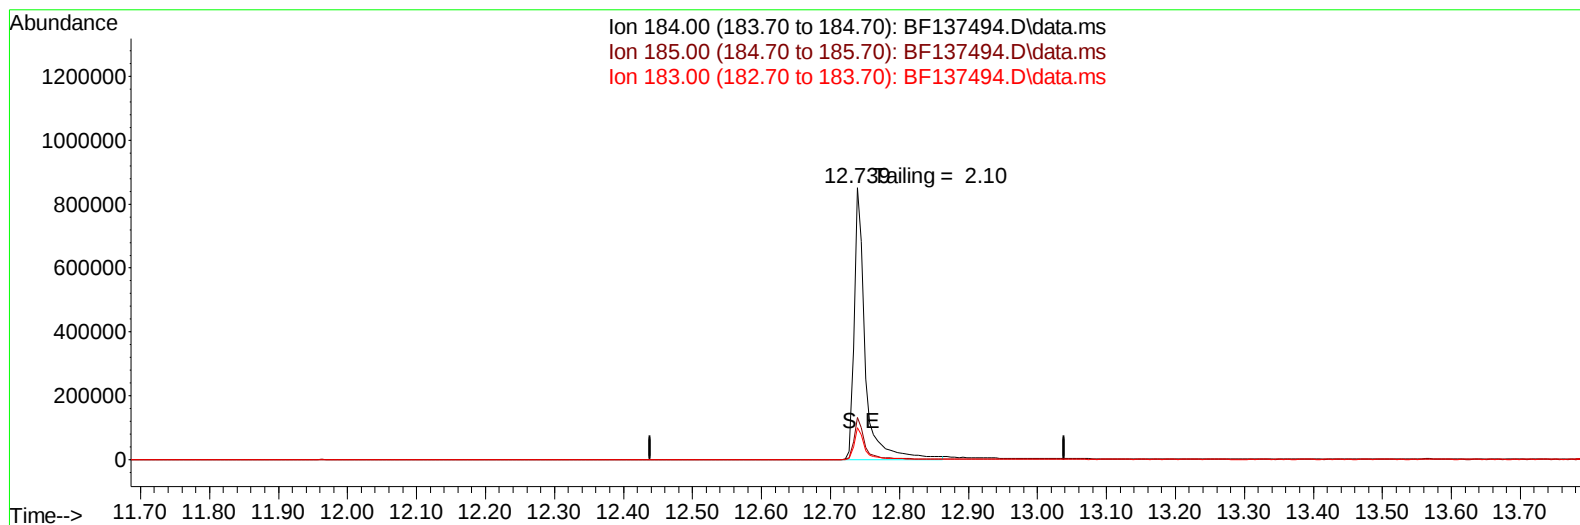

TIC: BF137494.D\data.ms

(77) Benzidine

12.739min (-12.739) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.50	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/5/2024	BNA_F	<u>BF137494.D</u>
Compound Name	Response	Retention Time
DDT	546166	13.568
DDD	10351	13.263
DDE	2483	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12834	559000	2.30

Instrument :
BNA_F
ClientSampleId :
DFTPP