


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030615\
Data File : BF077618.D
Acq On : 6 Mar 2015 11:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 04 13:27:09 2015

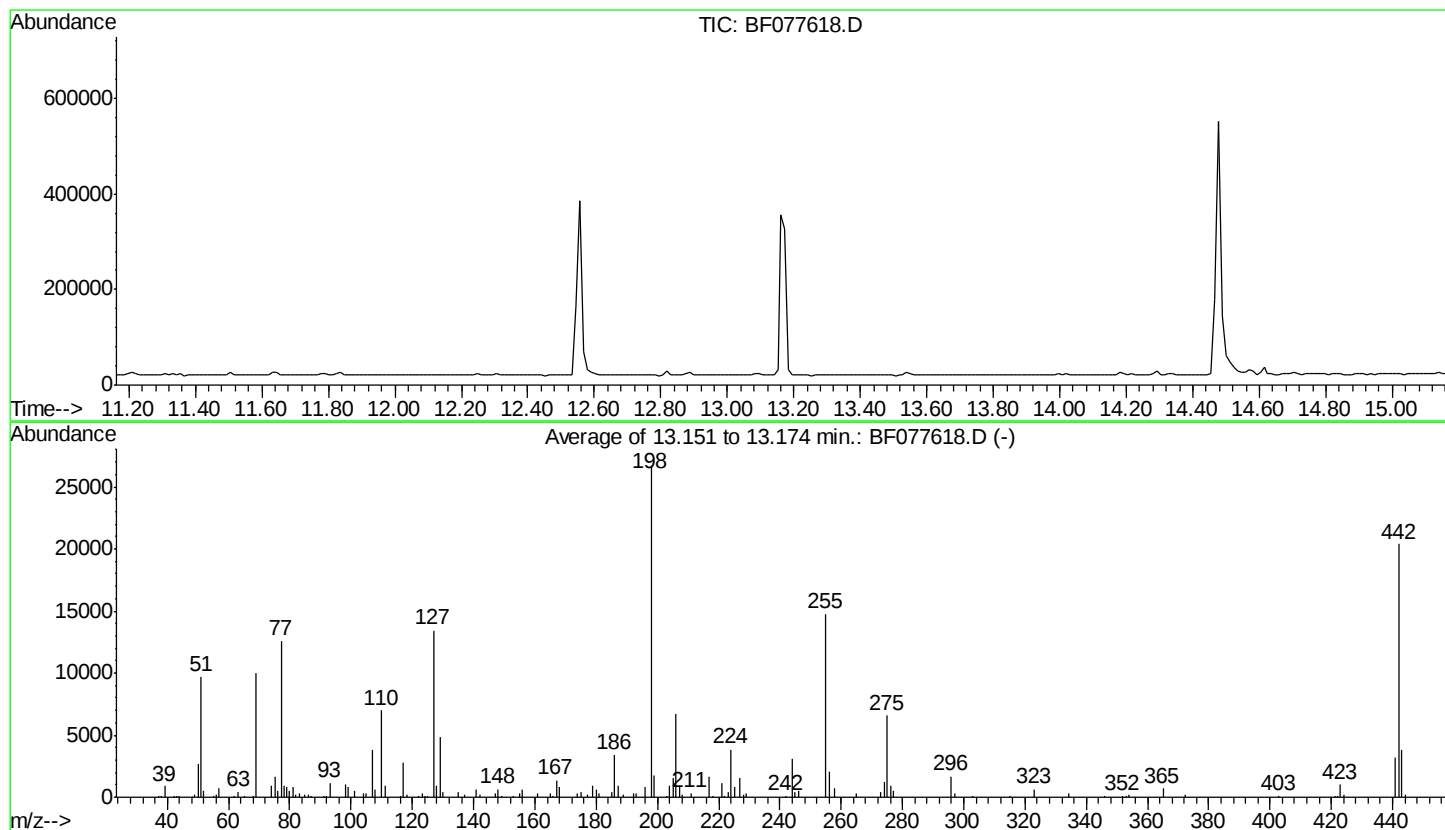

AutoFind: Scans 1073, 1074, 1075; Background Corrected with Scan 1070

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	9741	PASS
68	69	0.00	2	1.1	107	PASS
69	198	0.00	100	37.3	9963	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	13433	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26708	PASS
199	198	5	9	6.7	1780	PASS
275	198	10	60	24.6	6575	PASS
365	198	1	100	2.6	694	PASS
441	442	0.01	24	15.7	3212	PASS
442	198	50	100	76.4	20399	PASS
443	442	15	24	18.9	3864	PASS