


Data Path : W:\HPCHEM1\MSVOA_N\Data\VN030615\
Data File : VN022416BF.D
Acq On : 6 Mar 2015 21:39
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_N\METHODS\82N030615W.M
Title : SW846 8260
Last Update : Fri Mar 06 13:59:27 2015

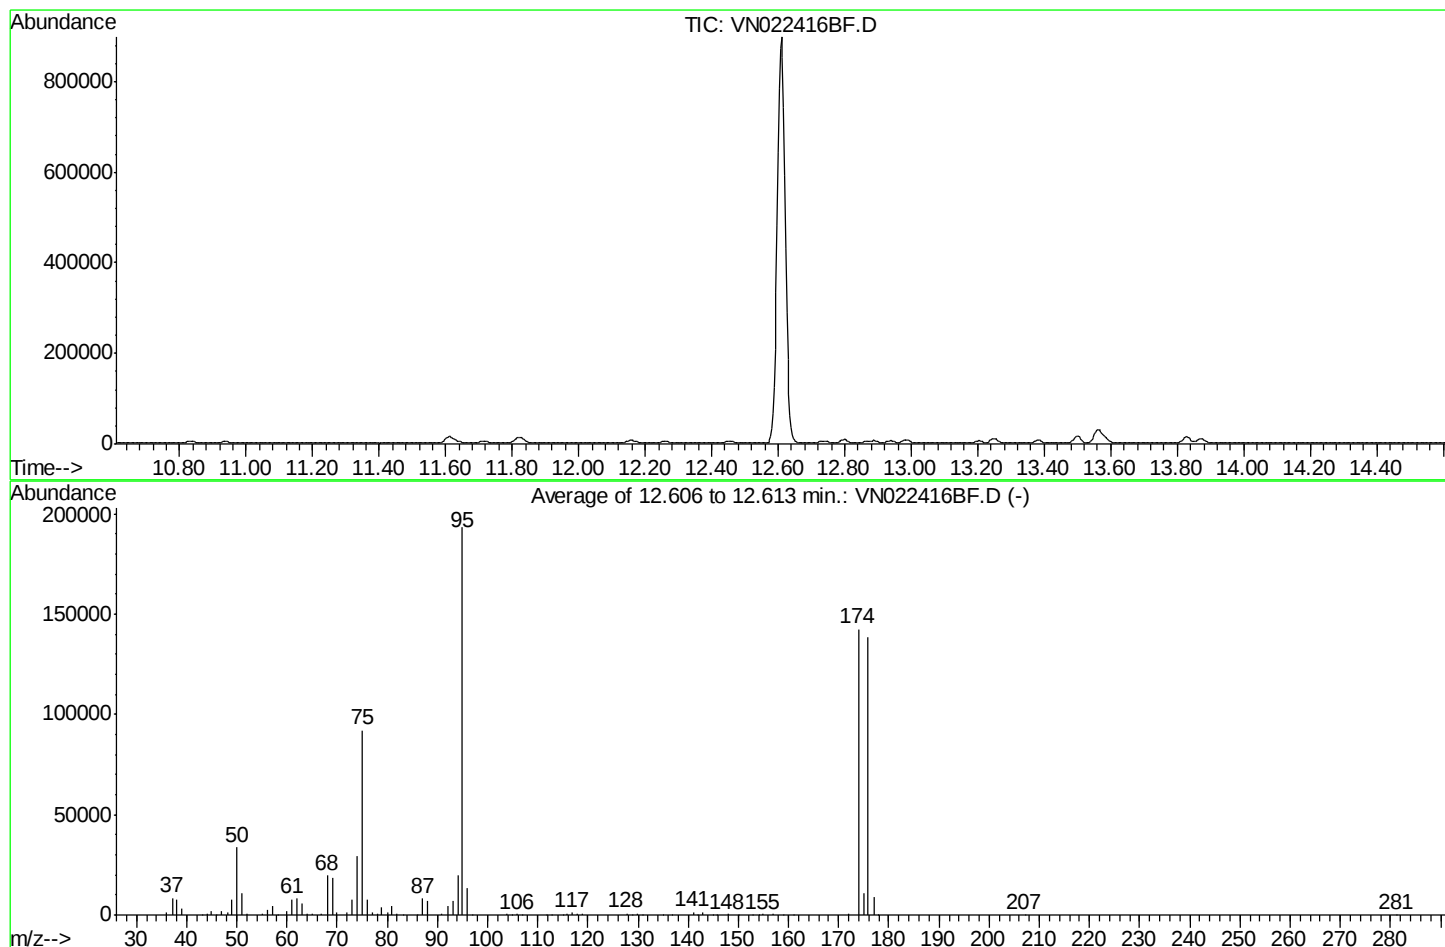

AutoFind: Scans 3364, 3365, 3366; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	33544	PASS
75	95	30	60	47.7	92224	PASS
95	95	100	100	100.0	193301	PASS
96	95	5	9	6.9	13253	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.8	142592	PASS
175	174	5	9	7.5	10683	PASS
176	174	95	101	97.4	138816	PASS
177	176	5	9	6.4	8895	PASS