

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030615\
 Data File : BF077634.D
 Acq On : 6 Mar 2015 21:02
 Operator : TP/IZ
 Sample : G1424-08DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SEP-1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: CENTROID

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.355	39	41	43	rVB	797557	936426	43.12%	3.263%
2	1.493	50	53	65	rVB	112057	281925	12.98%	0.983%
3	1.698	69	71	79	rVV2	32033	106789	4.92%	0.372%
4	1.813	79	81	110	rVB	1206602	2171564	100.00%	7.568%
5	3.413	217	221	226	rVB	28885	55520	2.56%	0.193%
6	4.967	352	357	363	rBV2	29488	59103	2.72%	0.206%
7	5.493	401	403	405	rVB	177950	231952	10.68%	0.808%
8	6.762	512	514	518	rVB	300672	281756	12.97%	0.982%
9	6.910	522	527	530	rBV	315403	304107	14.00%	1.060%
10	7.196	550	552	554	rBV	297304	381111	17.55%	1.328%
11	7.390	564	569	571	rBV2	200793	253699	11.68%	0.884%
12	7.893	610	613	615	rVB	162898	159046	7.32%	0.554%
13	8.773	688	690	695	rVB2	466885	702759	32.36%	2.449%
14	9.665	766	768	770	rVB	151651	132405	6.10%	0.461%
15	9.779	776	778	781	rVB	95296	105892	4.88%	0.369%
16	10.122	806	808	810	rVV	327236	275860	12.70%	0.961%
17	10.271	817	821	823	rVV3	63354	111064	5.11%	0.387%
18	10.442	833	836	839	rVV	39505	64564	2.97%	0.225%
19	10.533	841	844	845	rVV	91206	92171	4.24%	0.321%
20	10.671	855	856	860	rVV	33324	52303	2.41%	0.182%
21	10.945	878	880	882	rBV	577723	617521	28.44%	2.152%
22	10.991	882	884	886	rBV	233374	221293	10.19%	0.771%
23	11.208	901	903	905	rBV	110520	136687	6.29%	0.476%
24	11.631	937	940	942	rVB2	323894	346194	15.94%	1.207%
25	11.711	944	947	948	rBV	38751	52667	2.43%	0.184%
26	11.734	948	949	951	rVV	60254	51355	2.36%	0.179%
27	11.825	956	957	961	rVB2	45872	68445	3.15%	0.239%
28	11.928	963	966	969	rVV	214362	265961	12.25%	0.927%
29	12.305	997	999	1001	rVV2	53523	98079	4.52%	0.342%
30	12.339	1001	1002	1004	rVV2	41373	58653	2.70%	0.204%
31	12.408	1006	1008	1010	rVB	51154	67363	3.10%	0.235%
32	12.614	1023	1026	1028	rBV	34853	58671	2.70%	0.204%
33	12.659	1028	1030	1031	rVB	95877	88018	4.05%	0.307%
34	12.785	1039	1041	1042	rBV	599902	656367	30.23%	2.287%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030615\
 Data File : BF077634.D
 Acq On : 6 Mar 2015 21:02
 Operator : TP/IZ
 Sample : G1424-08DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SEP-1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: CENTROID

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.819	1042	1044	1046	rVV	2253450	2111610	97.24%	7.359%
36	12.877	1046	1049	1051	rVV	435651	484132	22.29%	1.687%
37	12.934	1051	1054	1056	rVV2	26801	55064	2.54%	0.192%
38	13.082	1066	1067	1069	rVV	106716	111296	5.13%	0.388%
39	13.208	1076	1078	1085	rVB5	31275	68558	3.16%	0.239%
40	13.414	1094	1096	1098	rBV	259100	294170	13.55%	1.025%
41	13.448	1098	1099	1102	rVB	339957	303108	13.96%	1.056%
42	13.505	1102	1104	1106	rBV	106400	112610	5.19%	0.392%
43	13.551	1106	1108	1109	rVV	371601	435015	20.03%	1.516%
44	13.585	1109	1111	1113	rVB	134305	186034	8.57%	0.648%
45	13.791	1127	1129	1133	rVB2	179485	256260	11.80%	0.893%
46	13.974	1143	1145	1147	rBV	56216	60768	2.80%	0.212%
47	14.008	1147	1148	1150	rVV	48928	58601	2.70%	0.204%
48	14.099	1153	1156	1158	rBV	111144	164235	7.56%	0.572%
49	14.145	1158	1160	1164	rVV2	82954	158718	7.31%	0.553%
50	14.214	1164	1166	1168	rVB2	56993	90829	4.18%	0.317%
51	14.294	1171	1173	1175	rVV	1699297	1605945	73.95%	5.597%
52	14.374	1178	1180	1181	rBV	103815	138372	6.37%	0.482%
53	14.477	1185	1189	1191	rBV2	59879	96041	4.42%	0.335%
54	14.568	1194	1197	1199	rVV	1390419	1791803	82.51%	6.245%
55	14.602	1199	1200	1202	rVV2	41373	60081	2.77%	0.209%
56	14.637	1202	1203	1205	rVV	45150	50885	2.34%	0.177%
57	14.728	1209	1211	1213	rBV	63720	75009	3.45%	0.261%
58	14.785	1213	1216	1218	rVB2	227925	316370	14.57%	1.103%
59	14.854	1218	1222	1224	rBV2	75697	132312	6.09%	0.461%
60	14.991	1228	1234	1236	rVB	207247	365430	16.83%	1.274%
61	15.071	1239	1241	1243	rVB	188755	189985	8.75%	0.662%
62	15.117	1243	1245	1247	rBV	157768	190040	8.75%	0.662%
63	15.231	1253	1255	1256	rBV	73255	84947	3.91%	0.296%
64	15.265	1256	1258	1261	rBV	78703	75282	3.47%	0.262%
65	15.494	1274	1278	1280	rBV5	36074	96851	4.46%	0.338%
66	15.620	1285	1289	1292	rVB2	45010	106000	4.88%	0.369%
67	15.757	1298	1301	1303	rBV2	87149	124672	5.74%	0.434%
68	15.803	1303	1305	1308	rVV2	100716	214651	9.88%	0.748%
69	15.883	1311	1312	1316	rVB	45662	62868	2.90%	0.219%
70	15.974	1316	1320	1324	rBV	35504	63321	2.92%	0.221%
71	16.077	1324	1329	1331	rBV2	894390	1687074	77.69%	5.880%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030615\
 Data File : BF077634.D
 Acq On : 6 Mar 2015 21:02
 Operator : TP/IZ
 Sample : G1424-08DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SEP-1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: CENTROID

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	16.111	1331	1332	1337	rVB	587918	551285	25.39%	1.921%
73	16.203	1337	1340	1343	rBV2	78809	137473	6.33%	0.479%
74	16.340	1349	1352	1354	rVB2	29155	51175	2.36%	0.178%
75	16.580	1371	1373	1375	rVV	111499	179221	8.25%	0.625%
76	16.625	1375	1377	1379	rVV	66622	84270	3.88%	0.294%
77	16.705	1379	1384	1386	rVV4	62367	135608	6.24%	0.473%
78	16.763	1386	1389	1391	rVV3	48207	114780	5.29%	0.400%
79	16.854	1395	1397	1401	rVB2	38582	53636	2.47%	0.187%
80	17.220	1424	1429	1431	rBV3	36453	99491	4.58%	0.347%
81	17.391	1441	1444	1450	rBV	442550	950820	43.79%	3.314%
82	17.506	1450	1454	1457	rVB2	93100	147321	6.78%	0.513%
83	17.631	1460	1465	1467	rBV4	29385	102645	4.73%	0.358%
84	17.711	1470	1472	1475	rVB	229421	331265	15.25%	1.154%
85	17.780	1475	1478	1481	rVB	434603	529146	24.37%	1.844%
86	17.848	1481	1484	1488	rBV2	596504	905649	41.70%	3.156%
87	18.031	1495	1500	1501	rBV4	23347	57732	2.66%	0.201%
88	18.203	1513	1515	1519	rVB	50304	79760	3.67%	0.278%
89	18.466	1535	1538	1540	rBV2	33142	51828	2.39%	0.181%
90	18.580	1546	1548	1552	rVB2	57804	109057	5.02%	0.380%
91	18.774	1562	1565	1567	rVB3	27902	51334	2.36%	0.179%
92	18.980	1580	1583	1588	rVB4	35804	100781	4.64%	0.351%
93	19.094	1589	1593	1597	rBV3	54305	135095	6.22%	0.471%
94	19.266	1604	1608	1613	rVB2	144990	340401	15.68%	1.186%
95	19.449	1621	1624	1626	rBV	25535	51454	2.37%	0.179%
96	19.677	1640	1644	1653	rVB2	406613	909784	41.90%	3.171%
97	19.814	1653	1656	1658	rBV3	31247	67212	3.10%	0.234%
98	19.894	1661	1663	1666	rVV	30970	64097	2.95%	0.223%
99	19.951	1666	1668	1671	rVV2	41375	88332	4.07%	0.308%
100	20.466	1709	1713	1718	rVB2	68334	187120	8.62%	0.652%


Sum of corrected areas: 28694009

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030615\
Data File : BF077634.D
Acq On : 6 Mar 2015 21:02
Operator : TP/IZ
Sample : G1424-08DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP-1DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

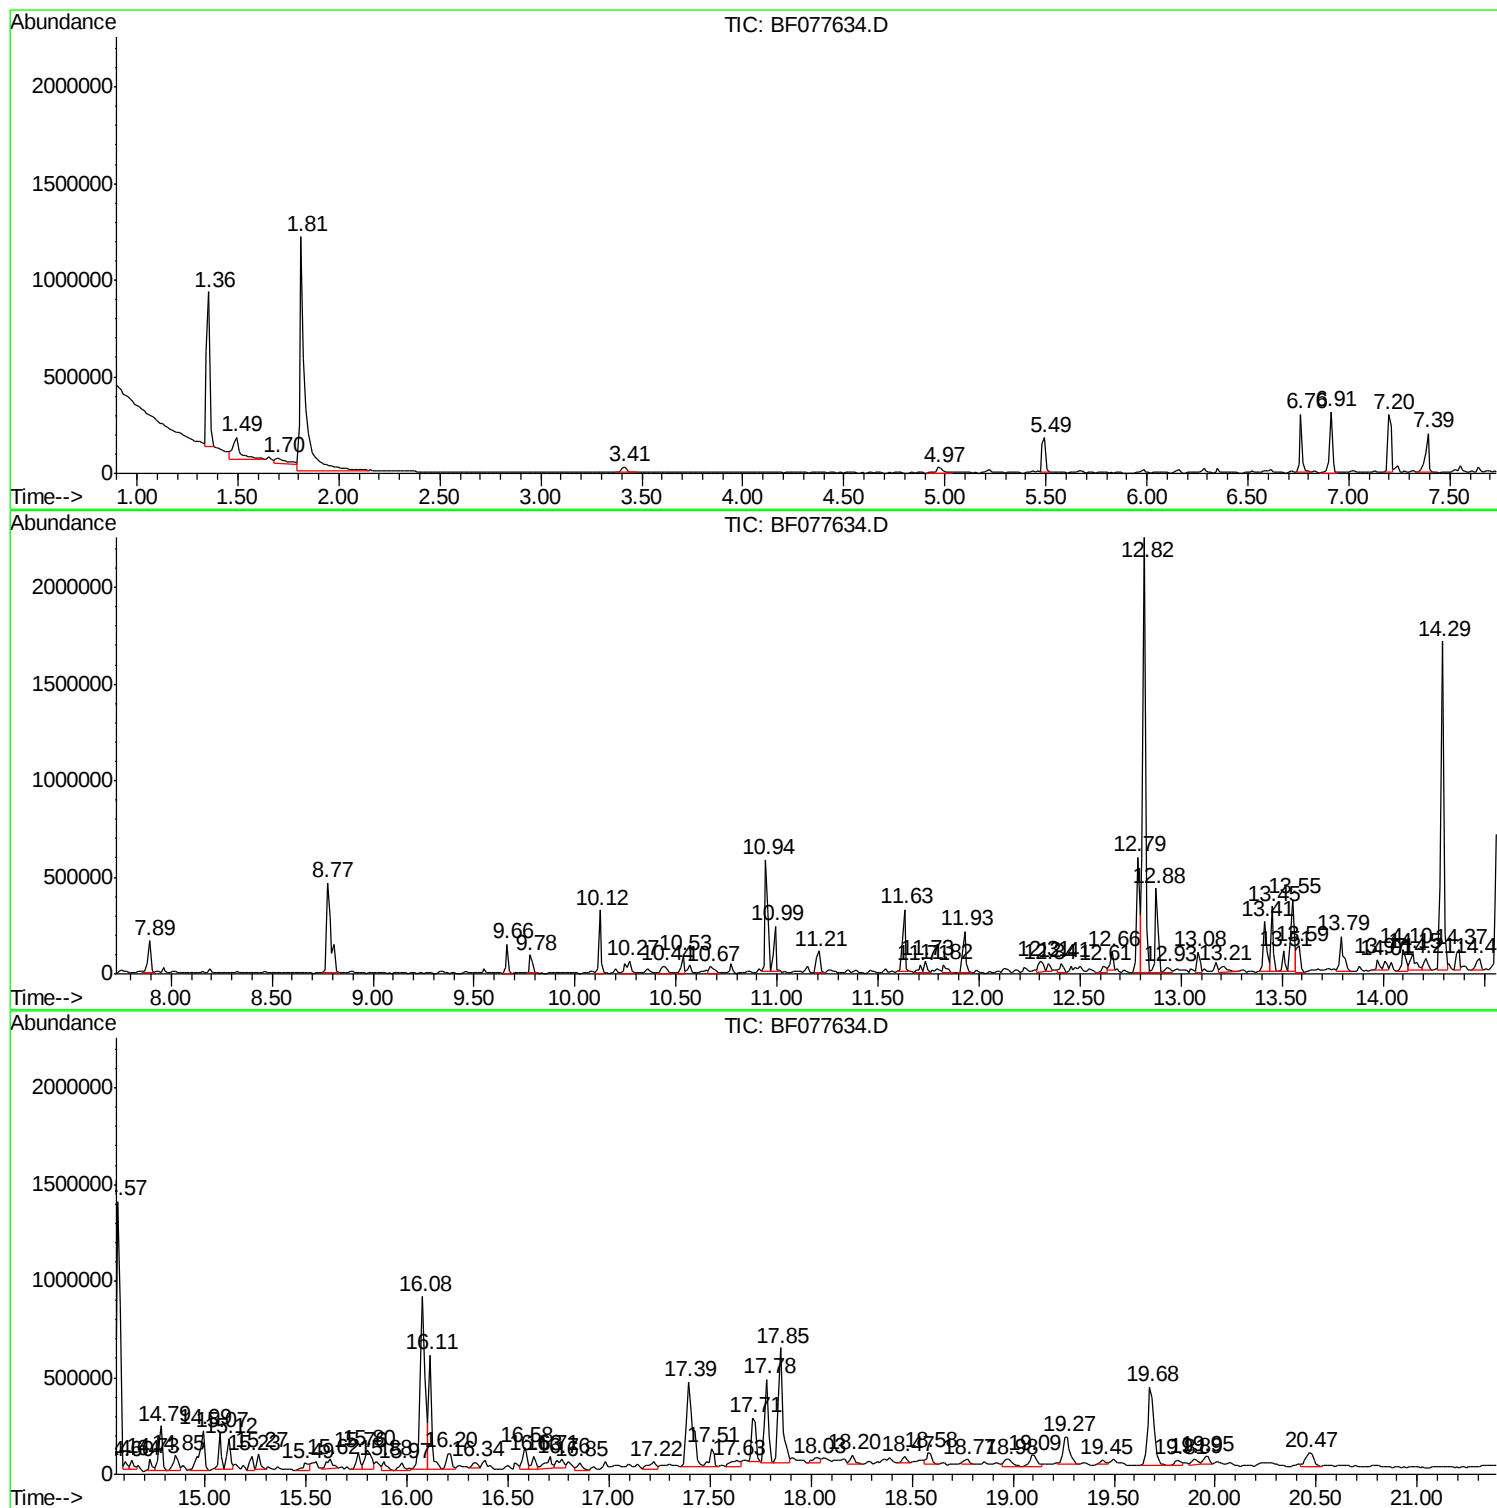

DbaaaPathh::ZZ\NRPBHHM1BBAFNDAAABBB000655\
 DbaaaFile::BB070834DD
 Aeqq00n :: 66Mar2005 221002
 Opeaaor ::TPPIZ
 Sample ::GC1224000DL5X
 Misc ::
 AASSVaal ::17 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 SEP-1DL

QqaabMebbdd::ZZ\NRPBHHM1BBAFMEH00S8270BB021915MM
 QqaabTitle ::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICLibrary :CC\DATAABBS6EN0\$5002LL
 TICIntegratioonParameters:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
