
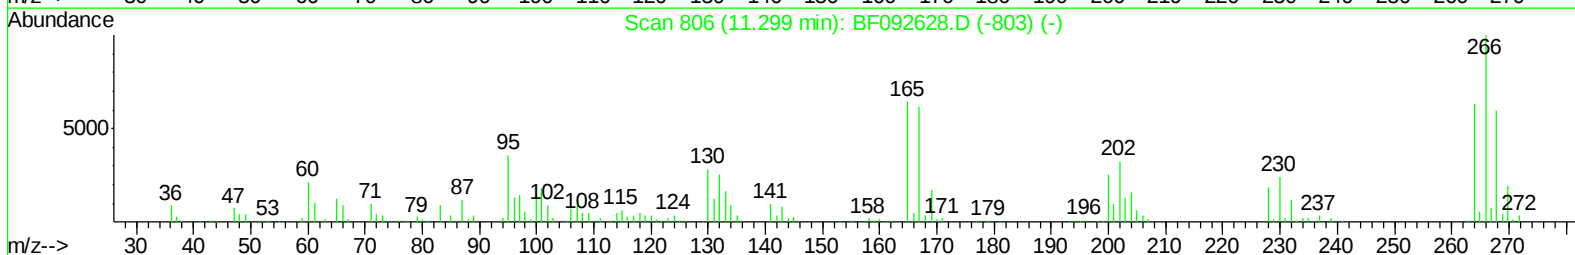
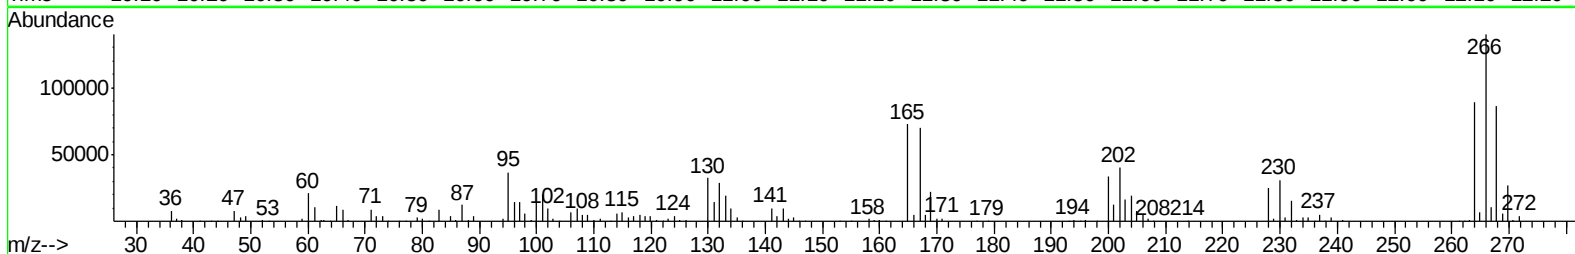


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030617\
Data File : BF093399.D
Acq On : 6 Mar 2017 14:32
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 00:52:51 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 00:03:56 2017
Response via : Initial Calibration

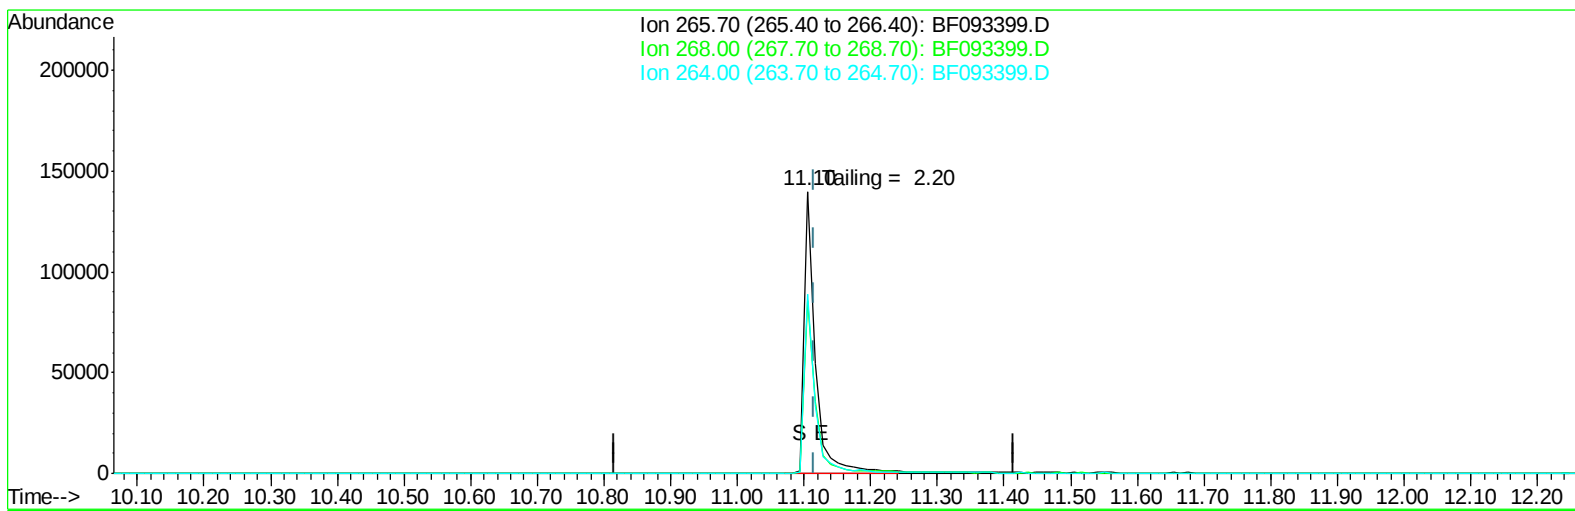

TIC: BF093399.D

(69) Pentachlorophenol (C)




11.105min (-0.011) 0.00ng

response 164218

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	61.49
264.00	62.90	63.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030617\
Data File : BF093399.D
Acq On : 6 Mar 2017 14:32
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 00:52:51 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 00:03:56 2017
Response via : Initial Calibration

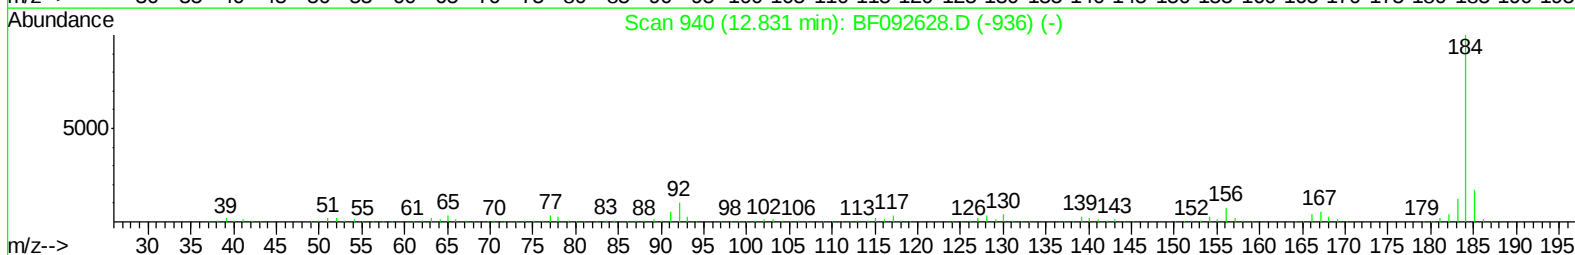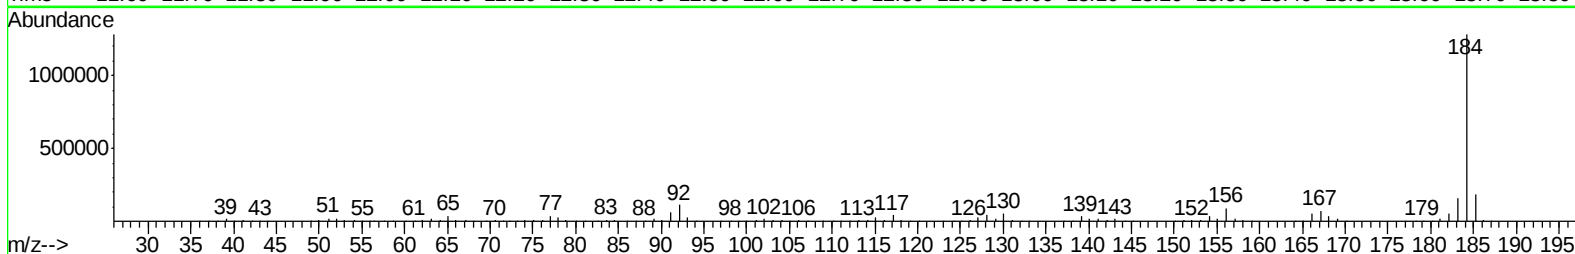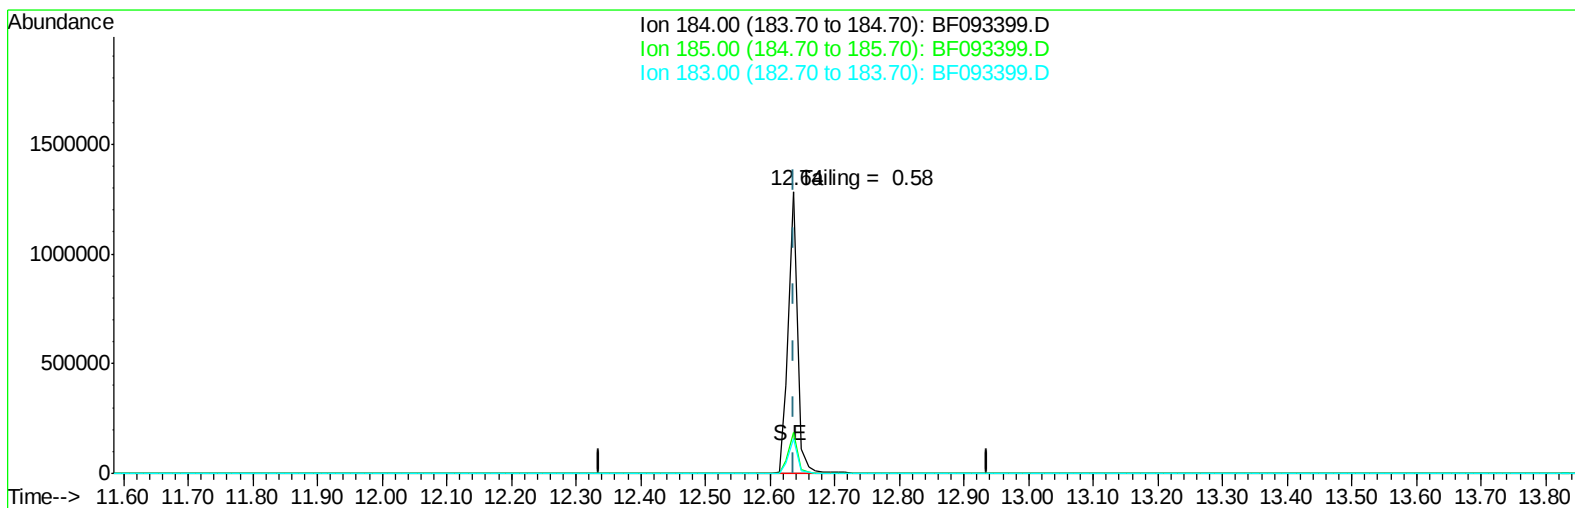

TIC: BF093399.D

(76) Benzidine

12.636min (+0.000) 0.00ng

response 1293559

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.63
183.00	11.50	12.45
0.00	0.00	0.00