


Data Path : Z:\HPCHEM1\BNA F\Data\BF030617\
 Data File : BF093399.D
 Acq On : 6 Mar 2017 14:32
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

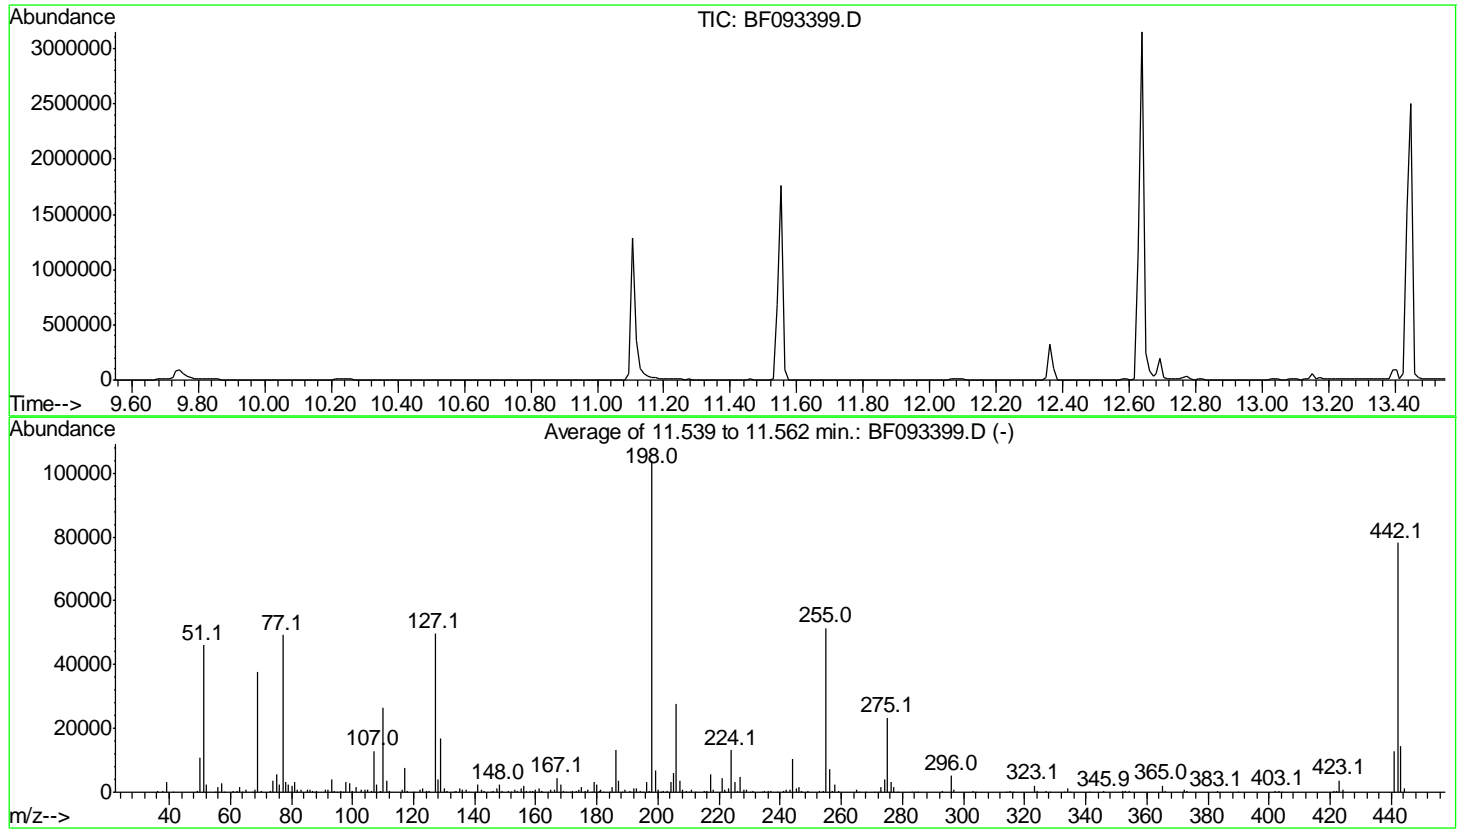

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	46100	PASS
68	69	0.00	2	2.0	742	PASS
69	198	0.00	100	36.4	37812	PASS
70	69	0.00	2	0.7	274	PASS
127	198	10	80	47.7	49583	PASS
197	198	0.00	2	0.3	281	PASS
198	198	100	100	100.0	103885	PASS
199	198	5	9	6.7	6956	PASS
275	198	10	60	22.4	23301	PASS
365	198	1	100	1.9	2020	PASS
441	442	0.01	24	16.3	12751	PASS
442	198	50	100	75.2	78088	PASS
443	442	15	24	18.6	14507	PASS