

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030618\
 Data File : BF103452.D
 Acq On : 6 Mar 2018 13:37
 Operator : SJ/JU
 Sample : J1723-19RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 06 14:50:59 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 06 11:52:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	120103	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	505393	20.00	ng	0.00
38) Acenaphthene-d10	9.91	164	212064	20.00	ng	0.00
63) Phenanthrene-d10	11.41	188	323301	20.00	ng	0.00
75) Chrysene-d12	14.07	240	212234	20.00	ng	0.00
86) Perylene-d12	15.58	264	179788	20.00	ng	0.00

System Monitoring Compounds

5) 2-Fluorophenol	5.50	112	783894	98.71	ng	0.00
7) Phenol-d6	6.51	99	956007	98.38	ng	0.00
23) Nitrobenzene-d5	7.44	82	586000	66.22	ng	0.00
41) 2,4,6-Tribromophenol	10.71	330	126209	70.31	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	813847	61.87	ng	0.00
78) Terphenyl-d14	12.99	244	517291	58.59	ng	0.00

Target Compounds


						Qvalue
9) Benzaldehyde	6.47	77	730	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.44	70	77874	12.877 ng	#	79
25) Isophorone	7.44	82	586000	33.621 ng	#	64
50) 2,6-Dinitrotoluene	9.91	165	27887	7.811 ng	#	26
51) Acenaphthene	9.95	154	26720	2.118 ng		98
55) 4-Nitrophenol	10.12	139	10921	3.890 ng	#	17
57) Fluorene	10.46	166	31213	2.116 ng		99
64) 4,6-Dinitro-2-methylphenol	10.71	198	243	5.056 ng	#	1
66) 4-Bromophenyl-phenylether	10.71	248	8498	2.523 ng	#	1
70) Phenanthrene	11.43	178	282762	15.892 ng		98
71) Anthracene	11.49	178	96796	5.305 ng		99
72) Carbazole	11.65	167	37265	2.051 ng		94
74) Fluoranthene	12.63	202	385016	21.534 ng		98
77) Pyrene	12.86	202	382113	23.092 ng		99
80) Benzo(a)anthracene	14.06	228	184562	13.403 ng		99
82) Chrysene	14.09	228	173881	13.005 ng		97
85) Indeno(1,2,3-cd)pyrene	17.13	276	58350	5.512 ng		96
87) Benzo(b)fluoranthene	15.13	252	243315	20.583 ng	#	92
88) Benzo(k)fluoranthene	15.13	252	243315	21.859 ng	#	95
89) Benzo(a)pyrene	15.52	252	123256	11.676 ng	#	93
91) Benzo(g,h,i)perylene	17.60	276	56568	7.096 ng		93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF030618\
Data File : BF103452.D
Acq On : 6 Mar 2018 13:37
Operator : SJ/JU
Sample : J1723-19RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 06 14:50:59 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 11:52:59 2018
Response via : Initial Calibration

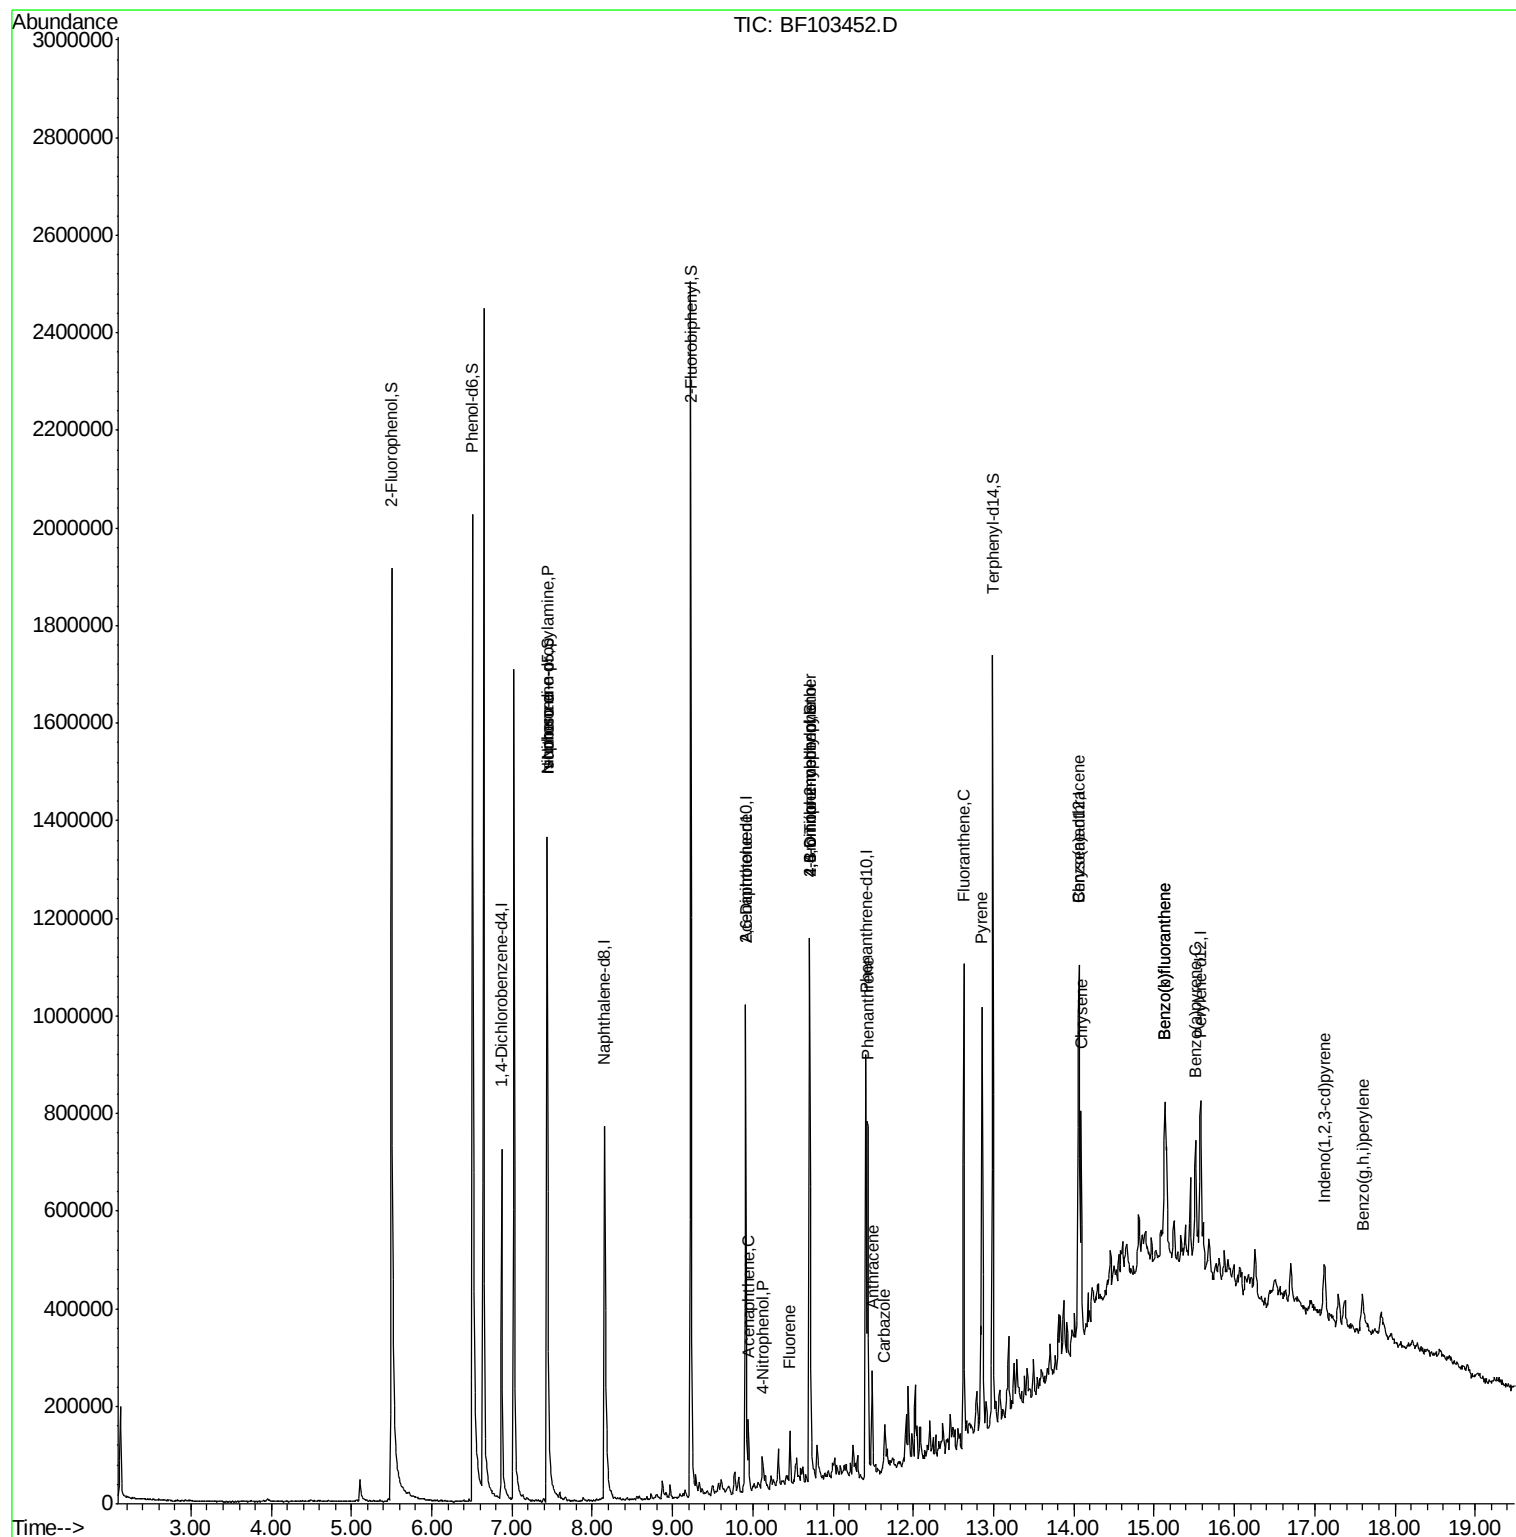




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.87 min Scan# 813
Delta R.T. 0.00 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Instrument :
BNA_F
ClientSampled :

Tot Ion	152	Resp	120103
Ion Ratio	Lower	Upper	
152	100		
150	158.0	124.6	186.8
115	68.1	50.1	75.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

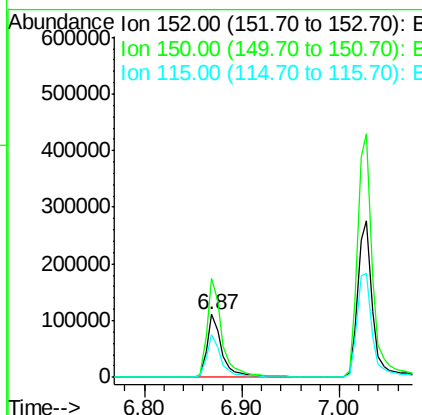



#5


2-Fluorophenol
Concen: 98.714 ng
RT: 5.50 min Scan# 580
Delta R.T. 0.00 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion	112	Resp	783894
Ion Ratio	Lower	Upper	
112	100		
64	66.2	47.9	71.9
63	34.3	23.7	35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

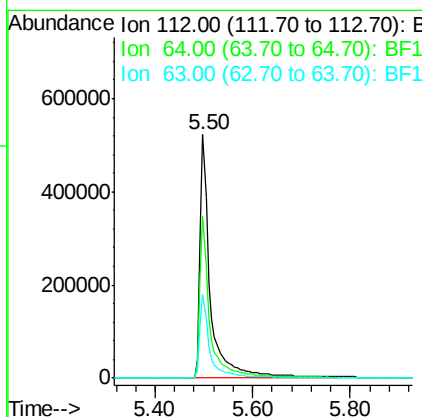

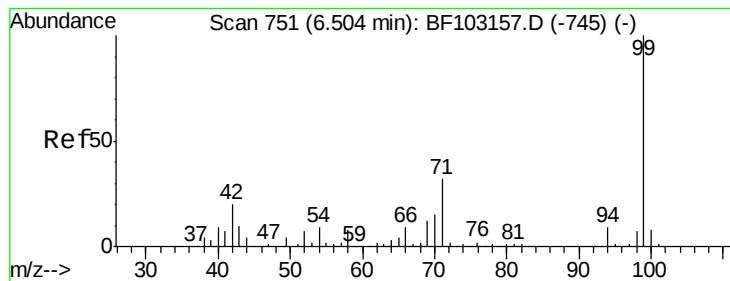

#7

Phenol-d6

Concen: 98.384 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 956007

Ion Ratio Lower Upper

99 100

42 20.6 14.5 21.7

71 32.0 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

800000

600000



400000

200000

0

6.40 6.51 6.60 6.80

Time-->

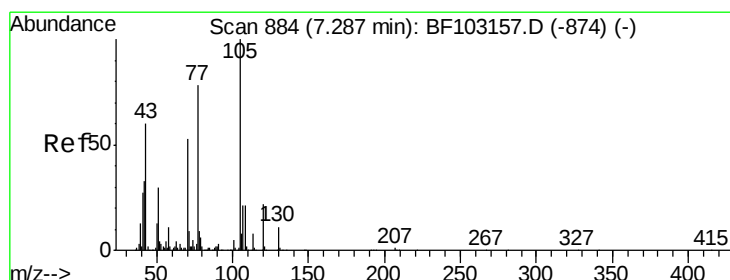

#19

n-Nitroso-di-n-propylamine

Concen: 12.877 ng

RT: 7.44 min Scan# 910

Delta R.T. 0.15 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37

Tgt Ion: 70 Resp: 77874


Ion Ratio Lower Upper

70 100

42 49.5 47.5 71.3

101 0.0 7.4 11.2#

130 1.8 16.6 25.0#



Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

80000

60000


40000


20000

0

7.35 7.40 7.44 7.50 7.55

Time-->









#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.16 min Scan# 1032
Delta R.T. 0.00 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	505393
Ion	Ratio	Lower Upper
136	100	
137	10.9	8.9 13.3
54	8.6	6.6 9.8
68	6.1	5.0 7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

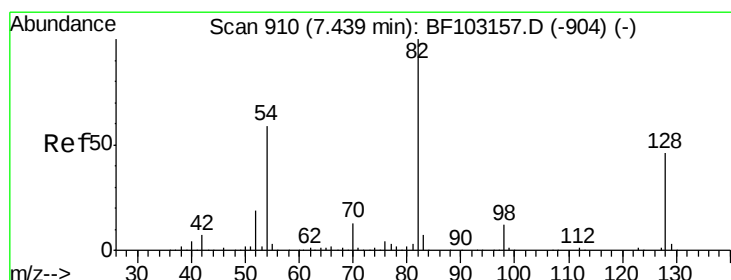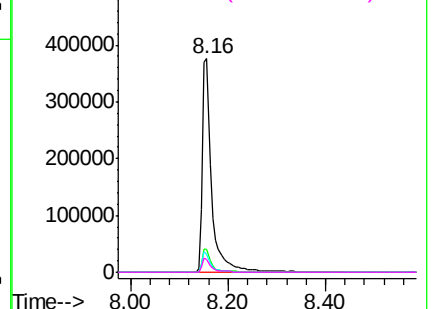




#23
Nitrobenzene-d5
Concen: 66.217 ng
RT: 7.44 min Scan# 910
Delta R.T. -0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion: 82	Resp:	586000
Ion	Ratio	Lower Upper
82	100	
128	44.9	36.1 54.1
54	58.9	41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

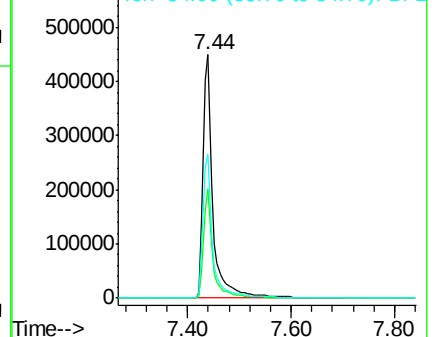

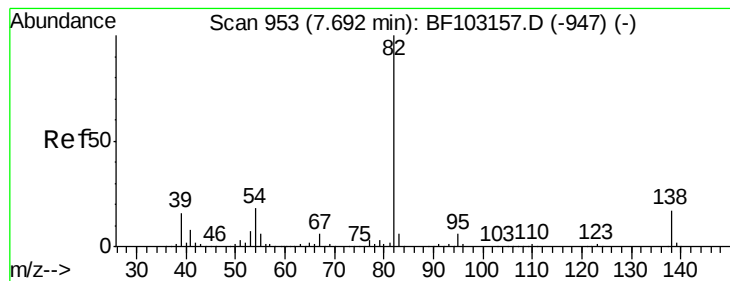

#25

Isophorone

Concen: 33.621 ng

RT: 7.44 min Scan# 910

Delta R.T. -0.25 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 586000

Ion Ratio Lower Upper




82 100

95 0.1 5.2 7.8#

138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

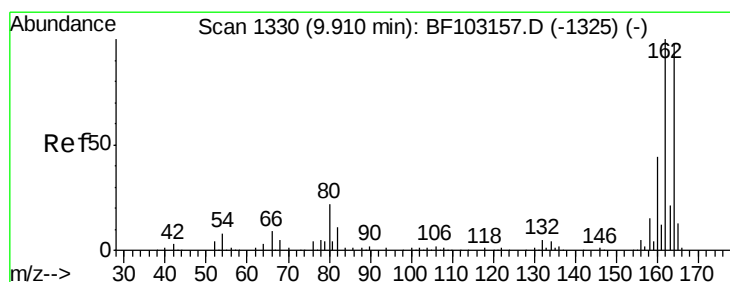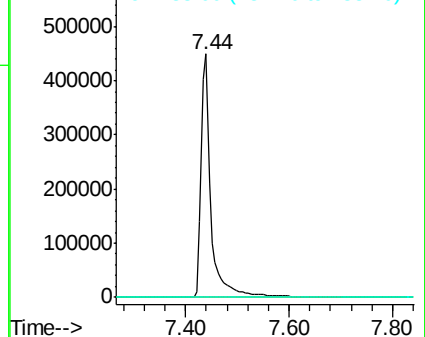

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.91 min Scan# 1330

Delta R.T. -0.01 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37


Tgt Ion: 164 Resp: 212064

Ion Ratio Lower Upper



164 100


162 102.8 86.1 129.1

160 44.5 38.3 57.5

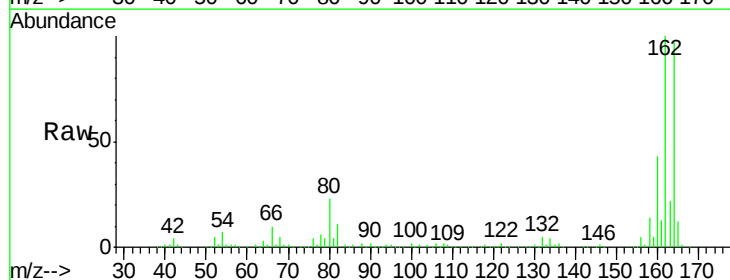

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

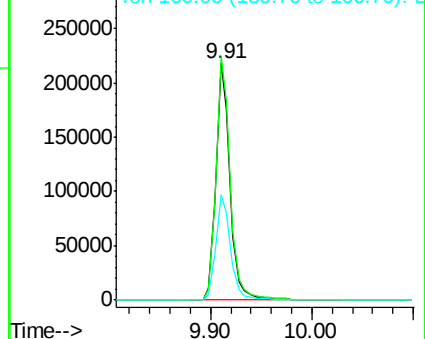







#41
 2,4,6-Tribromophenol
 Concen: 70.311 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.01 min
 Lab File: BF103452.D
 Acq: 6 Mar 2018 13:37

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 126209
 Ion Ratio Lower Upper
 330 100
 332 103.4 77.0 115.6
 141 46.3 29.9 44.9#

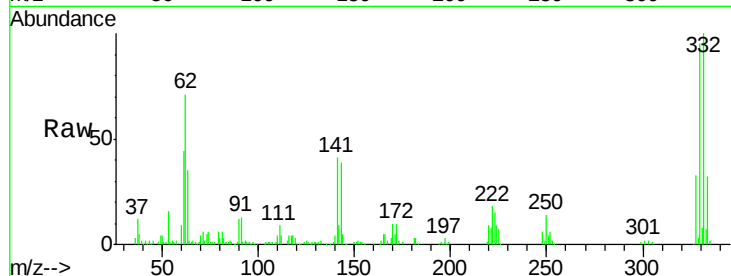


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


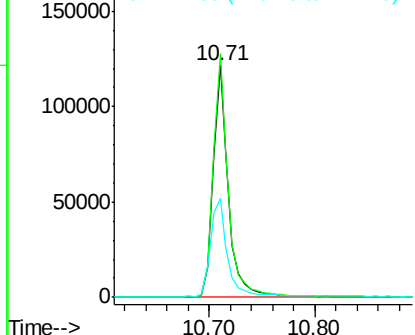



#44
 2-Fluorobiphenyl
 Concen: 61.874 ng
 RT: 9.23 min Scan# 1214
 Delta R.T. 0.00 min
 Lab File: BF103452.D
 Acq: 6 Mar 2018 13:37

Tgt Ion:172 Resp: 813847
 Ion Ratio Lower Upper
 172 100
 171 35.4 29.7 44.5
 170 23.8 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




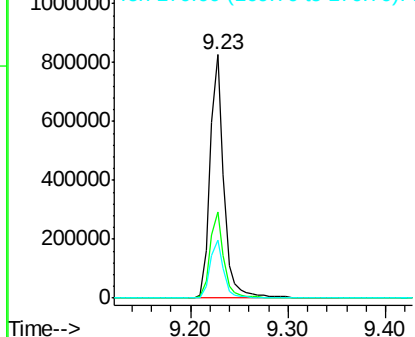




#50
2,6-Dinitrotoluene
Concen: 7.811 ng
RT: 9.91 min Scan# 1330
Delta R.T. 0.21 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37




Instrument :
BNA_F
ClientSampleId :


Tot Ion:165 Resp: 27887
Ion Ratio Lower Upper
165 100
63 1.6 44.7 67.1#
89 1.2 44.0 66.0#

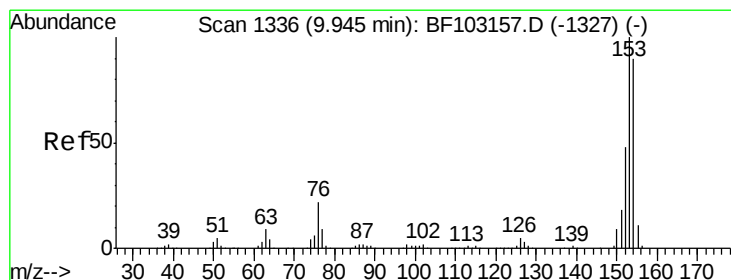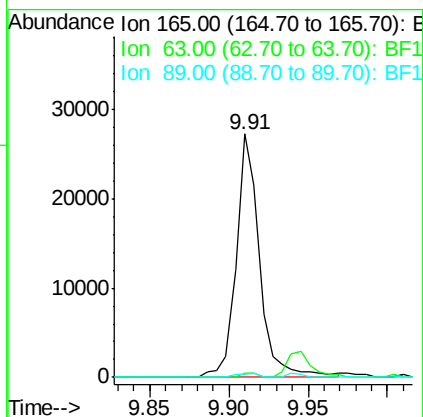

#51
Acenaphthene
Concen: 2.118 ng
RT: 9.95 min Scan# 1336
Delta R.T. -0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion:154 Resp: 26720
Ion Ratio Lower Upper
154 100
153 111.6 91.2 136.8
152 54.3 43.8 65.8

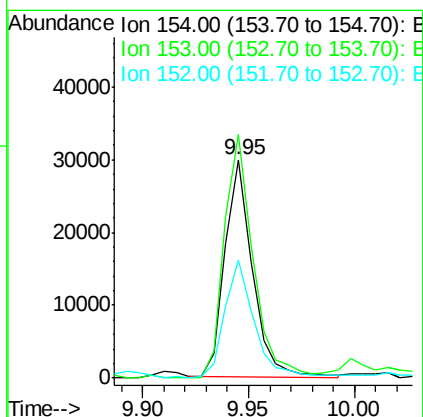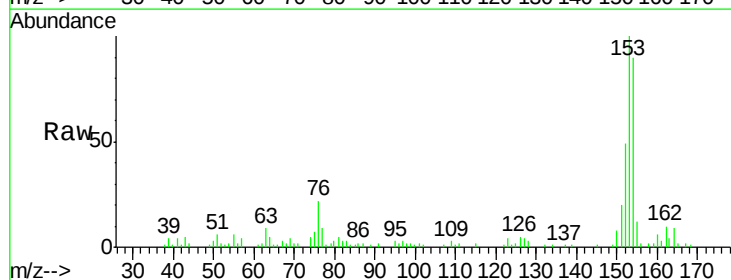







#55
4-Nitrophenol
Concen: 3.890 ng
RT: 10.12 min Scan# 1366
Delta R.T. 0.06 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Instrument :
BNA_F
ClientSampleId :

Tot Ion:139 Resp: 10921
Ion Ratio Lower Upper
139 100
109 10.0 48.4 88.4#
65 6.2 72.6 112.6#

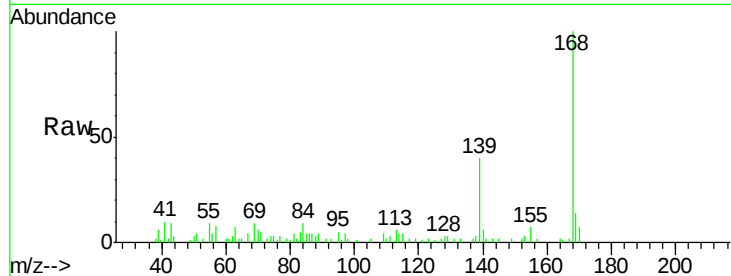


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF1

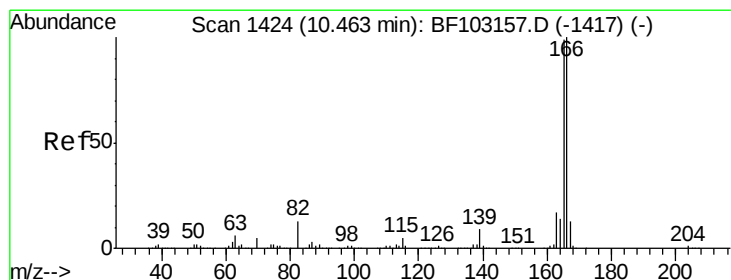
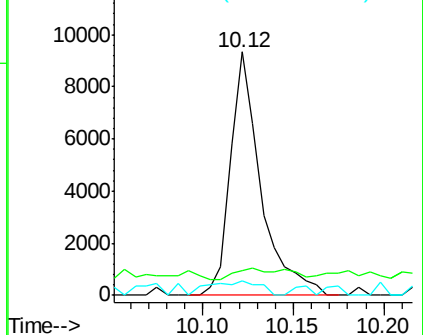



#57
Fluorene
Concen: 2.116 ng
RT: 10.46 min Scan# 1424
Delta R.T. -0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion:166 Resp: 31213
Ion Ratio Lower Upper
166 100
165 98.7 79.8 119.8
167 14.7 10.6 16.0



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

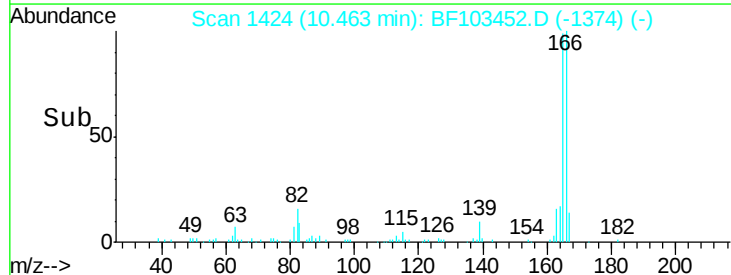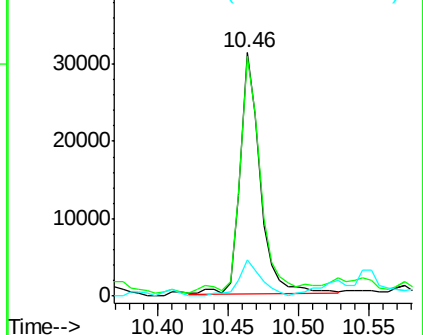



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.41 min Scan# 1585

Delta R.T. 0.00 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37

Instrument :

BNA_F

ClientSampleId :


Tot Ion:188 Resp: 323301

Ion Ratio Lower Upper

188 100

94 10.7 8.5 12.7




80 11.4 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

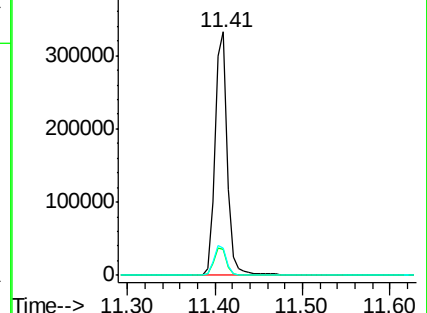

#64

4,6-Dinitro-2-methylphenol

Concen: 5.056 ng

RT: 10.71 min Scan# 1466

Delta R.T. 0.18 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37


Tgt Ion:198 Resp: 243

Ion Ratio Lower Upper

198 100

51 319.3 37.7 77.7#



105 269.3 36.3 76.3#




Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

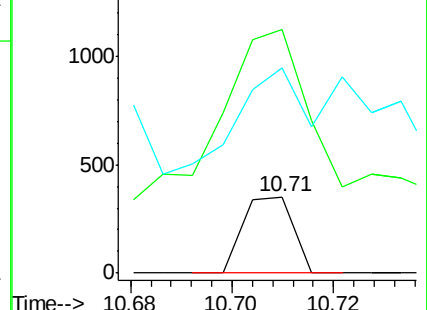


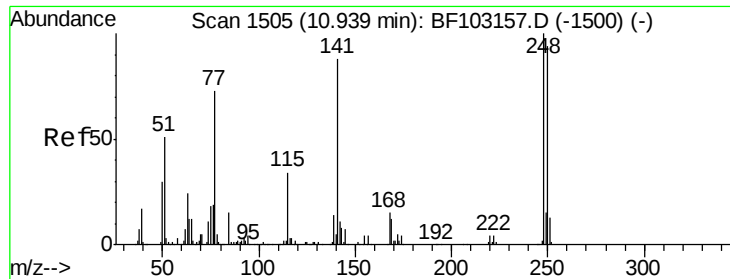




#66
4-Bromophenyl-phenylether
Concen: 2.523 ng
RT: 10.71 min Scan# 1466
Delta R.T. -0.24 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 8498
Ion Ratio Lower Upper
248 100
250 212.2 76.9 115.3#
141 626.2 74.4 111.6#

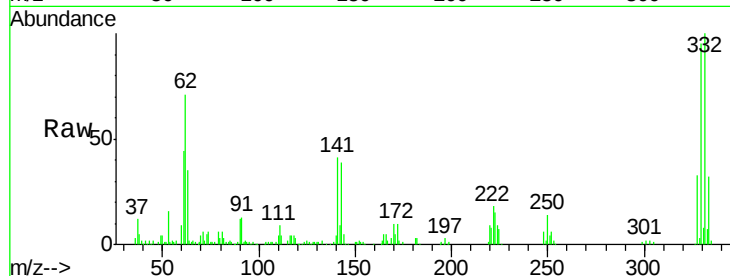


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E


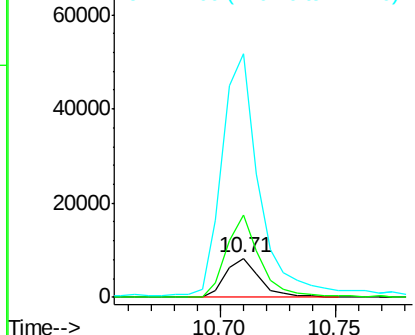



#70
Phenanthrene
Concen: 15.892 ng
RT: 11.43 min Scan# 1589
Delta R.T. 0.00 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion:178 Resp: 282762
Ion Ratio Lower Upper
178 100
176 19.5 15.8 23.8
179 15.2 13.0 19.6



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

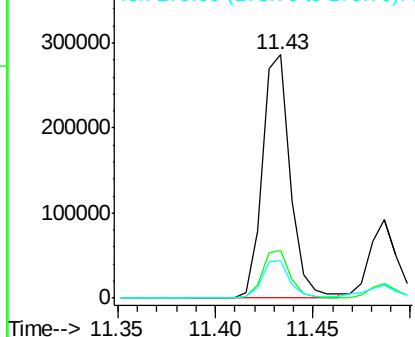


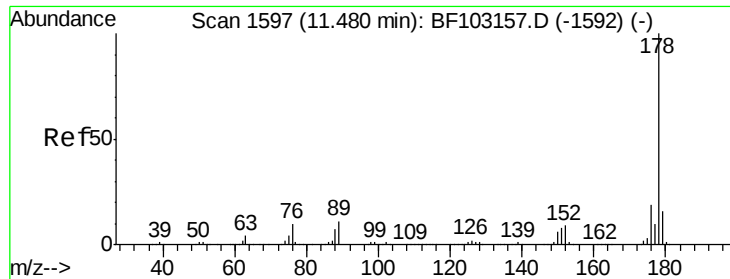




#71
 Anthracene
 Concen: 5.305 ng
 RT: 11.49 min Scan# 1598
 Delta R.T. 0.00 min
 Lab File: BF103452.D
 Acq: 6 Mar 2018 13:37

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:178 Resp: 96796
 Ion Ratio Lower Upper
 178 100
 176 18.8 15.4 23.2
 179 16.2 12.6 19.0




Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E


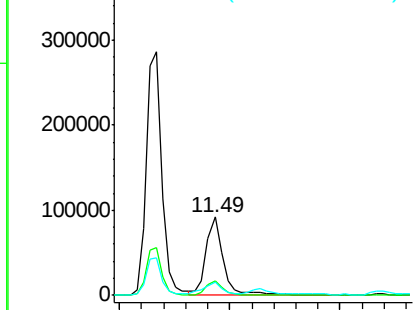



#72
 Carbazole
 Concen: 2.051 ng
 RT: 11.65 min Scan# 1625
 Delta R.T. 0.00 min
 Lab File: BF103452.D
 Acq: 6 Mar 2018 13:37

Tgt Ion:167 Resp: 37265
 Ion Ratio Lower Upper
 167 100
 166 25.0 17.6 26.4
 139 15.9 10.9 16.3



Abundance Ion 167.00 (166.70 to 167.70): E
 Ion 166.00 (165.70 to 166.70): E
 Ion 139.00 (138.70 to 139.70): E




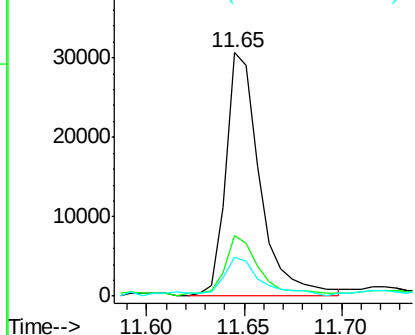




#74
 Fluoranthene
 Concen: 21.534 ng
 RT: 12.63 min Scan# 1792
 Delta R.T. -0.01 min
 Lab File: BF103452.D
 Acq: 6 Mar 2018 13:37




Instrument :
 BNA_F
 ClientSampleID :


Tot Ion	Ratio	Lower	Upper
202	100		
101	14.8	0.0	34.1
203	17.3	0.0	38.1

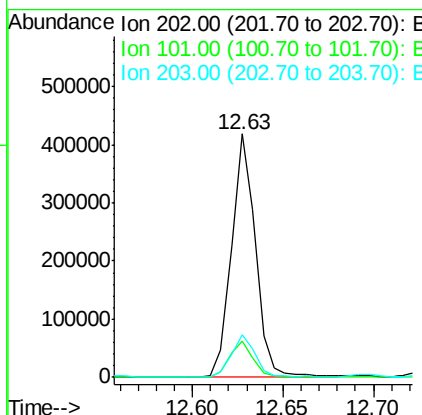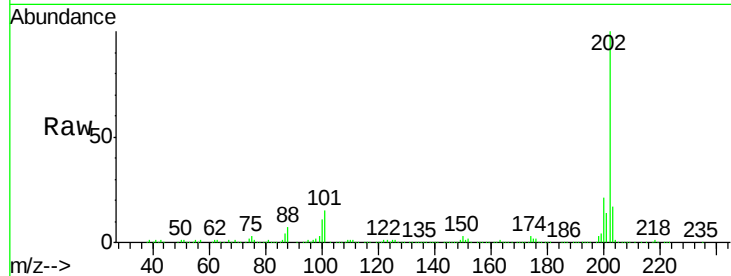

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.07 min Scan# 2037
 Delta R.T. 0.00 min
 Lab File: BF103452.D
 Acq: 6 Mar 2018 13:37

Tgt Ion	Ratio	Lower	Upper
240	100		
120	14.1	9.5	14.3
236	27.4	20.7	31.1



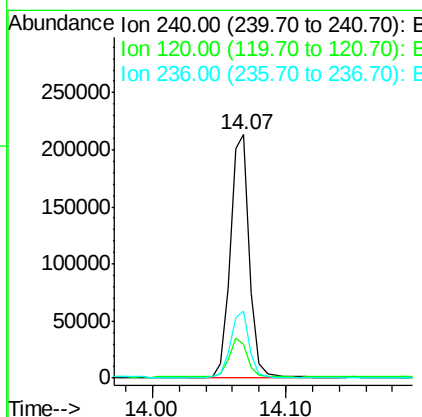





#77
Pvrene
Concen: 23.092 ng
RT: 12.86 min Scan# 1831
Delta R.T. -0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37




Instrument :
BNA_F
ClientSampleId :


Tot Ion:202 Resp: 382113
Ion Ratio Lower Upper
202 100
200 22.0 17.4 26.2
203 18.4 14.3 21.5

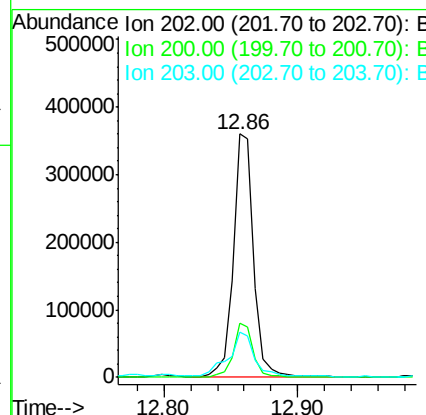

#78
Terphenyl-d14
Concen: 58.591 ng
RT: 12.99 min Scan# 1854
Delta R.T. -0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion:244 Resp: 517291
Ion Ratio Lower Upper
244 100
212 6.8 5.4 8.0
122 13.9 11.0 16.4



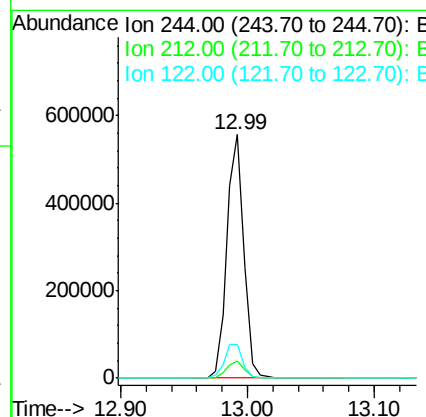





#80
Benzo(a)anthracene
Concen: 13.403 ng
RT: 14.06 min Scan# 2035
Delta R.T. 0.00 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 184562
Ion Ratio Lower Upper
228 100
226 27.4 22.6 33.8
229 20.4 15.8 23.6

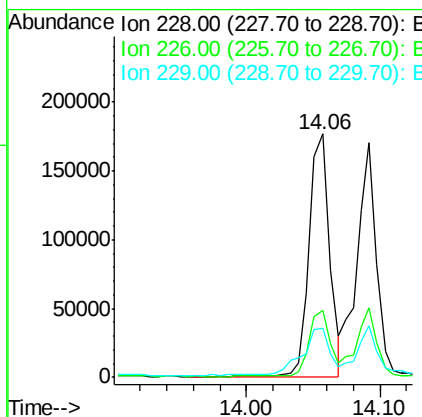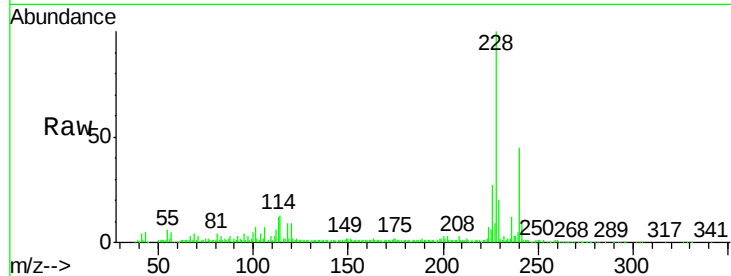

#82
Chrysene
Concen: 13.005 ng
RT: 14.09 min Scan# 2041
Delta R.T. -0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion:228 Resp: 173881
Ion Ratio Lower Upper
228 100
226 29.6 25.0 37.6
229 22.1 16.2 24.4

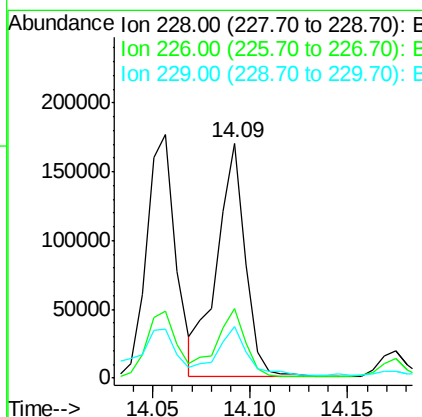







#85
Indeno(1,2,3-cd)pyrene
Concen: 5.512 ng
RT: 17.13 min Scan# 2557
Delta R.T. -0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	27.7	25.0	37.6
277	24.5	20.1	30.1

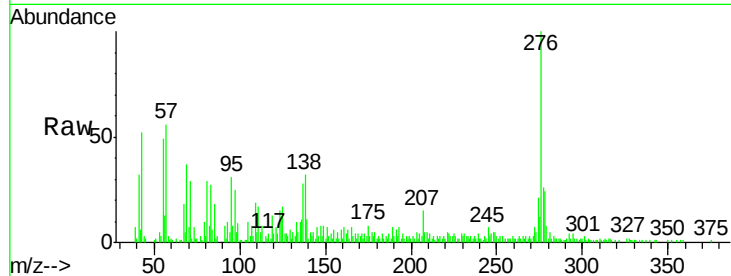


Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E


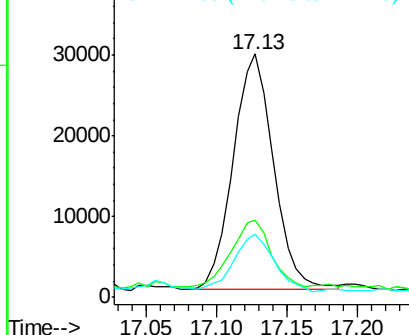



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.58 min Scan# 2294
Delta R.T. 0.01 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.2	28.8
265	21.9	17.5	26.3



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E



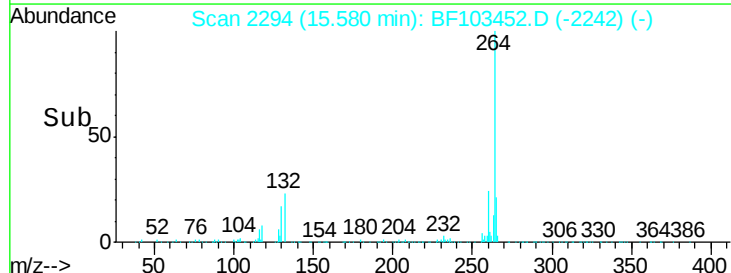
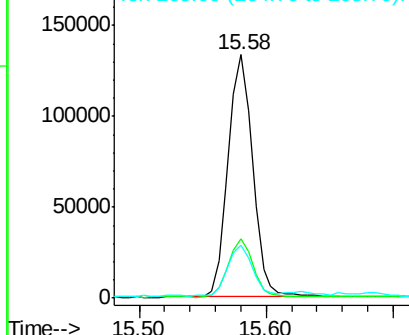




#87
Benzo(b)fluoranthene
Concen: 20.583 ng
RT: 15.13 min Scan# 2218
Delta R.T. 0.00 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.0	25.6
125	16.2	9.0	13.6

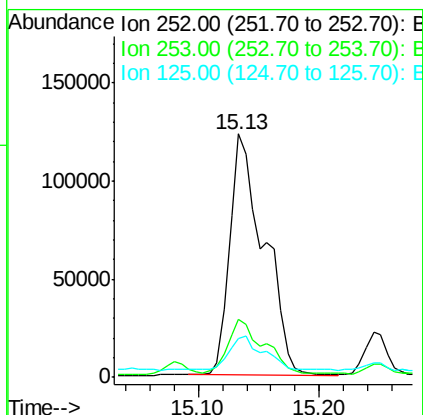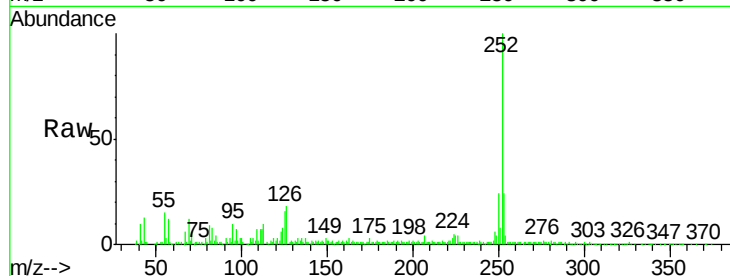

#88
Benzo(k)fluoranthene
Concen: 21.859 ng
RT: 15.13 min Scan# 2218
Delta R.T. -0.03 min
Lab File: BF103452.D
Acq: 6 Mar 2018 13:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.9	26.9
125	16.2	10.2	15.2

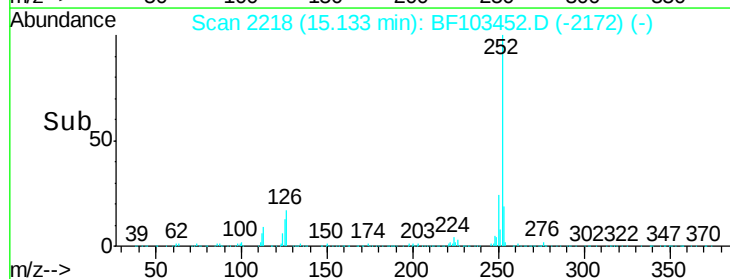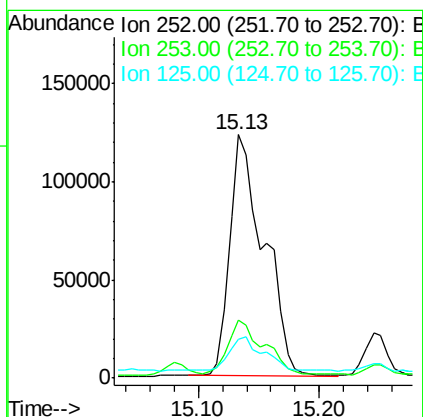

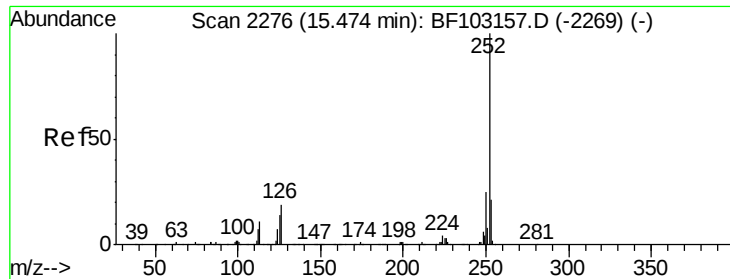

#89

Benzo(a)pyrene

Concen: 11.676 ng

RT: 15.52 min Scan# 2283

Delta R.T. 0.00 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37

Instrument :

BNA_F

ClientSampleId :


Tot Ion:252 Resp: 123256

Ion Ratio Lower Upper

252 100

253 23.5 17.1 25.7




125 16.4 9.8 14.6#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

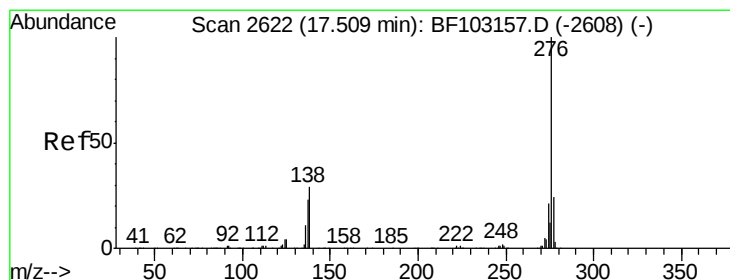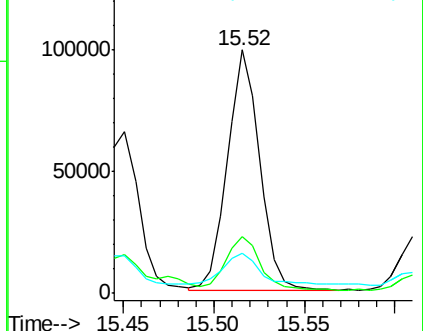

#91

Benzo(g,h,i)perylene

Concen: 7.096 ng

RT: 17.60 min Scan# 2637

Delta R.T. 0.00 min

Lab File: BF103452.D

Acq: 6 Mar 2018 13:37


Tgt Ion:276 Resp: 56568

Ion Ratio Lower Upper

276 100

277 24.8 17.9 26.9

138 32.2 21.8 32.8



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

