

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030618\
 Data File : BF103488.D
 Acq On : 7 Mar 2018 6:45
 Operator : SJ/JU
 Sample : J1802-01 50X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 07 07:59:42 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\DDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 11:24:24 2006
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.40	152	511	40.00	ng	-0.01
2) Naphthalene-d8	12.86	136	3735	40.00	ng	-0.02
3) Acenaphthene-d10	18.09	164	108	40.00	ng	0.02
4) Phenanthrene-d10	17.06	188	106	40.00	ng	0.01
8) Chrysene-d12	0.00	240	0	0.00	ng	-30.48
9) Perylene-d12	0.00	264	0	0.00	ng	-34.55


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) DDE	10.82	246	817	1253.446	ng/uL#	82
6) DDD	11.20	235	1168	812.624	ng/uL#	44
7) DDT	11.56	235	1269	1361.352	ng/uL#	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030618\
Data File : BF103488.D
Acq On : 7 Mar 2018 6:45
Operator : SJ/JU
Sample : J1802-01 50X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 07 07:59:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\DDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:24:24 2006
Response via : Initial Calibration

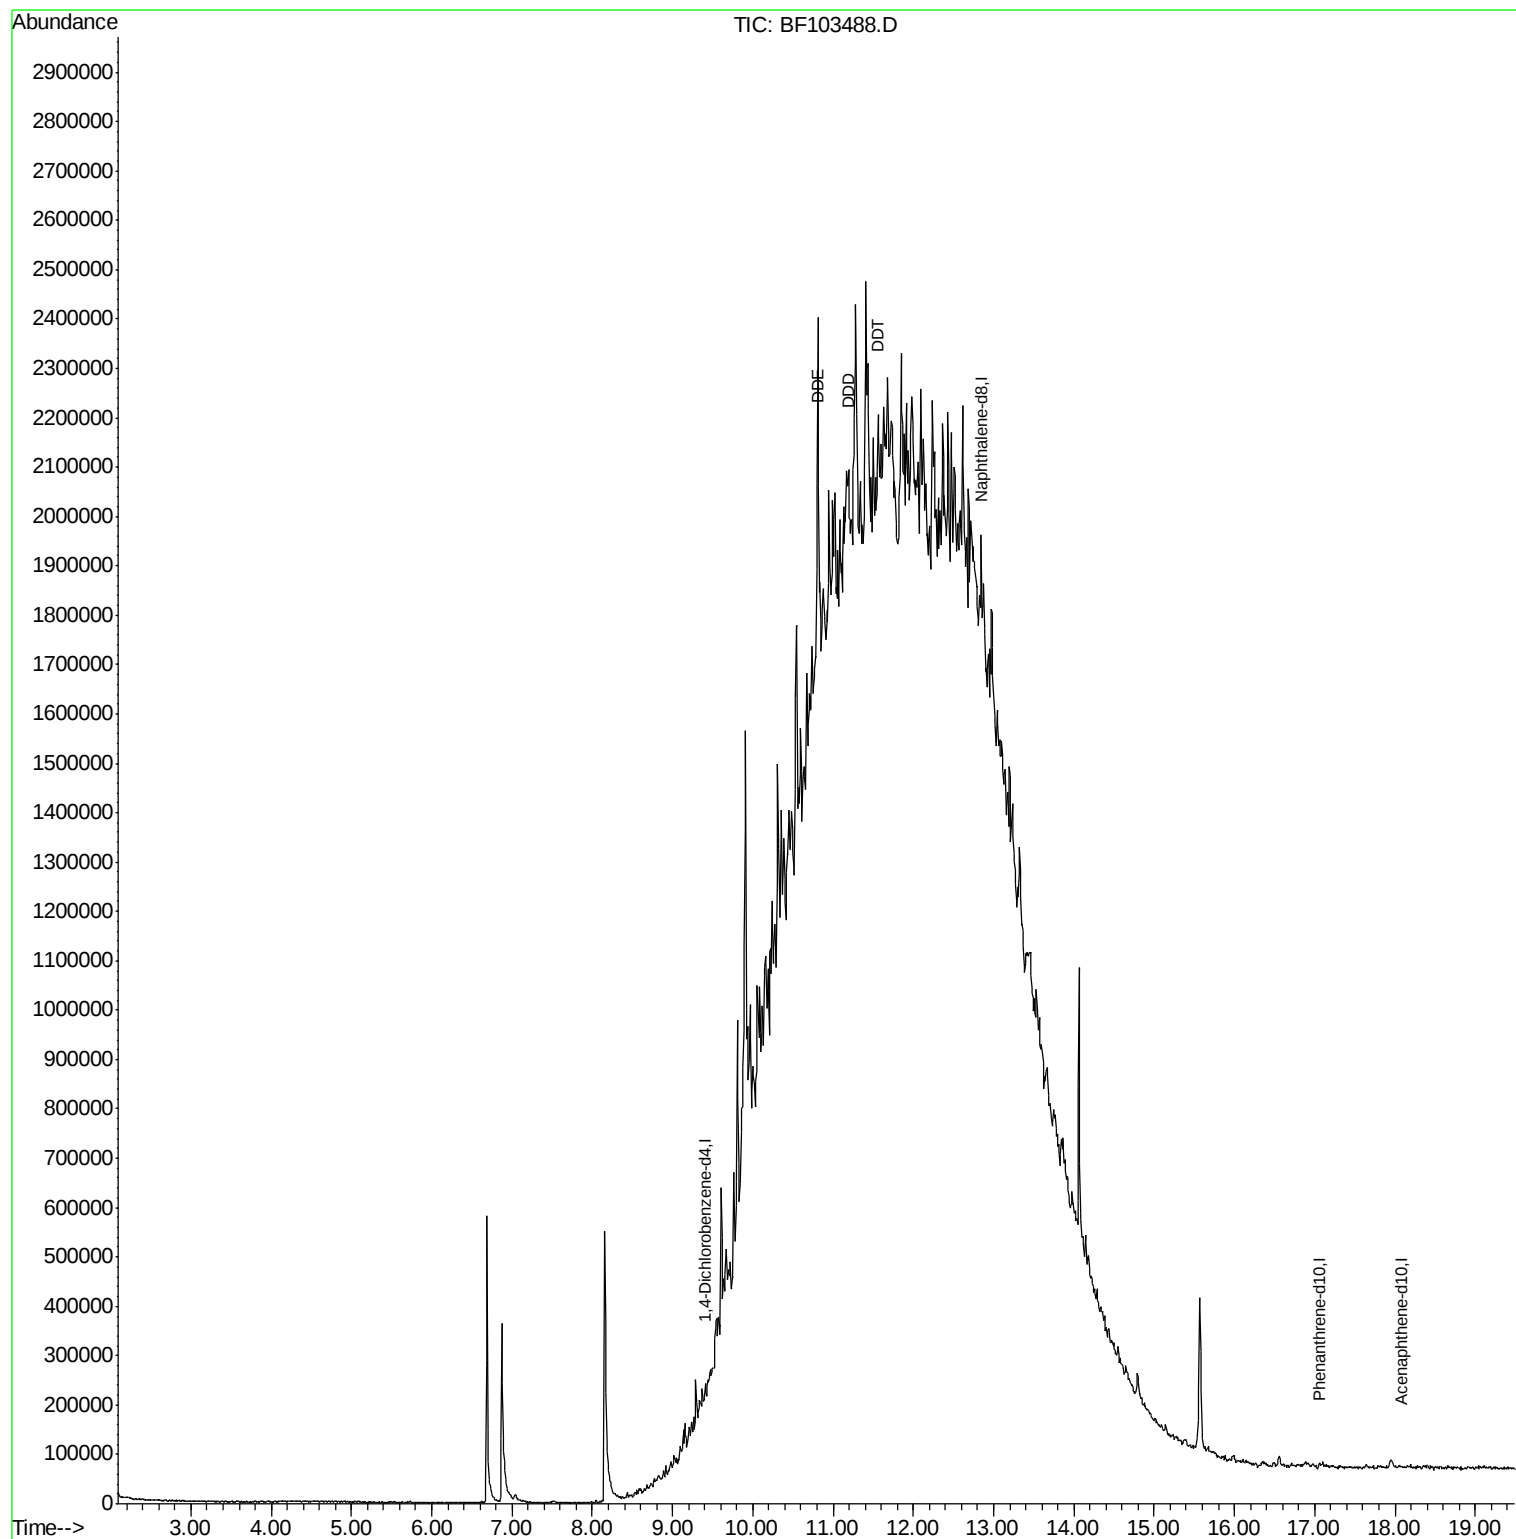

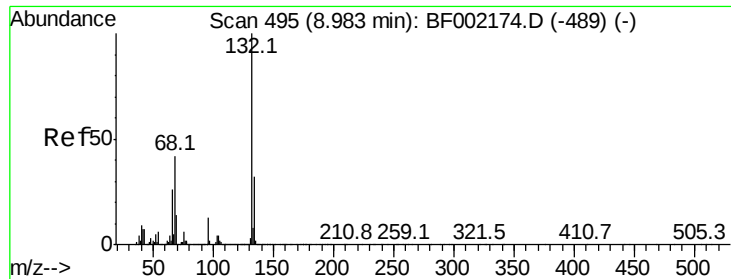

#5

DDE

Concen: 1253.446 ng/uL

RT: 10.82 min Scan# 1485

Delta R.T. 0.03 min

Lab File: BF103488.D

Acq: 7 Mar 2018 6:45

Instrument :

BNA_F

ClientSampleId :

Tot Ion:246 Resp: 817


Ion Ratio Lower Upper

246 100

248 39.3 41.8 62.6#

318 0.0 0.0 0.0

176 119.5 0.0 0.0#



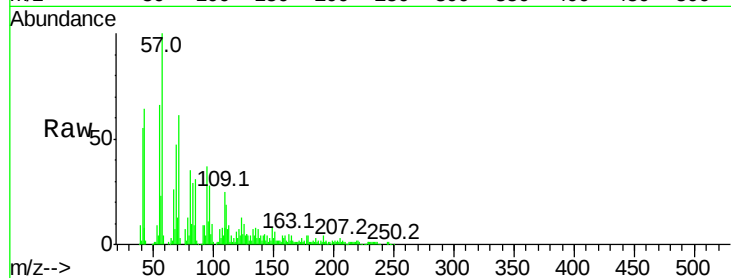


Abundance Ion 246.00 (245.70 to 246.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 318.00 (317.70 to 318.70): E

Ion 176.00 (175.70 to 176.70): E

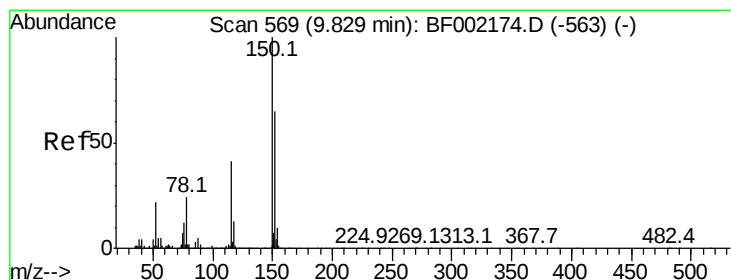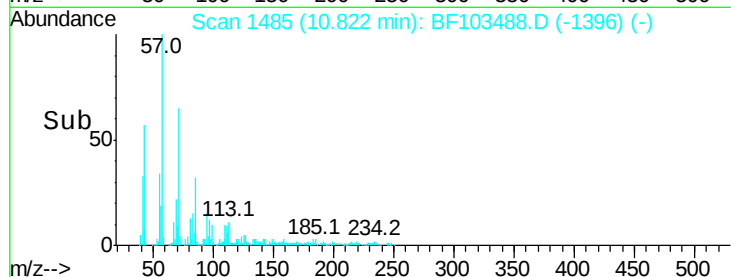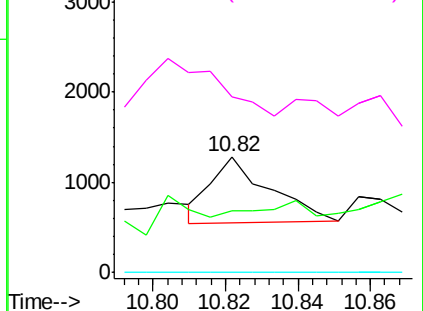

#6

DDD

Concen: 812.624 ng/uL

RT: 11.20 min Scan# 1549

Delta R.T. -0.00 min

Lab File: BF103488.D

Acq: 7 Mar 2018 6:45


Tgt Ion:235 Resp: 1168

Ion Ratio Lower Upper

235 100

237 33.7 51.7 77.5#



165 0.0 44.0 66.0#



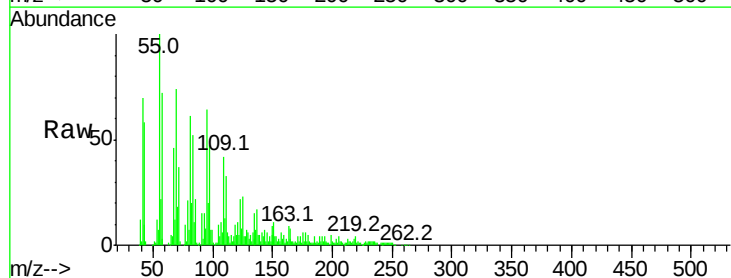


Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E

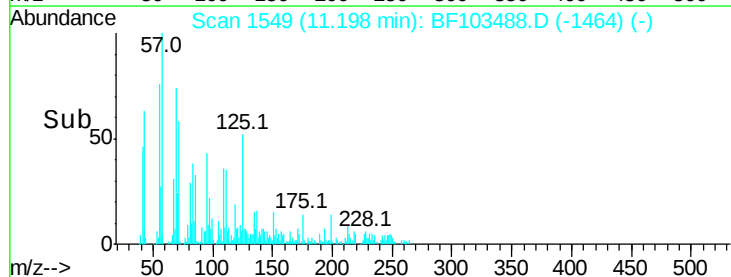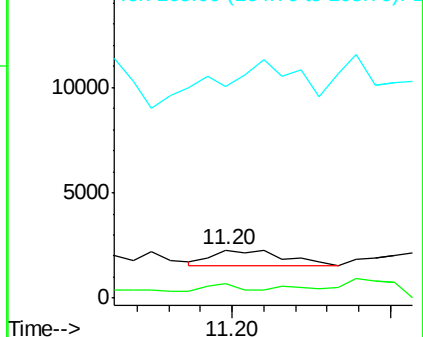

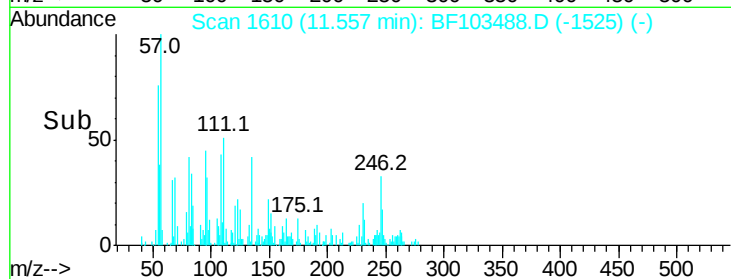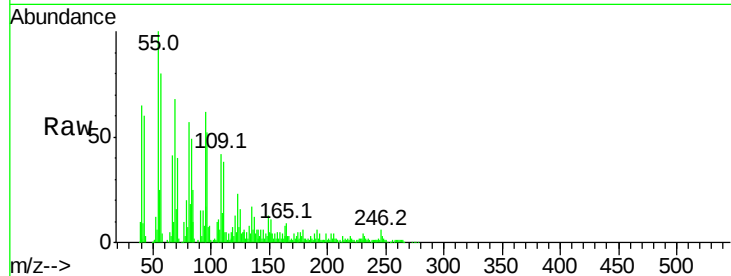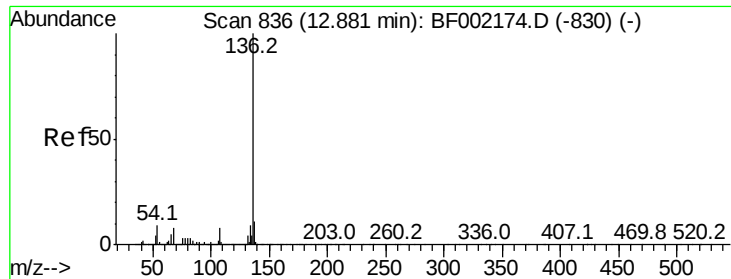

#7

DDT

Concen: 1361.352 ng/uL

RT: 11.56 min Scan# 1610

Delta R.T. 0.00 min

Lab File: BF103488.D

Acq: 7 Mar 2018 6:45

Instrument :

BNA_F

ClientSampleId :

Tot Ion:235 Resp: 1269

Ion Ratio Lower Upper

235 100

237 0.0 0.0 0.0

165 130.9 0.0 0.0#

Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E

