

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030618\
 Data File : BF103489.D
 Acq On : 7 Mar 2018 7:11
 Operator : SJ/JU
 Sample : J1809-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 07 07:59:49 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\DDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 11:24:24 2006
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.43	152	3517	40.00	ng	0.01
2) Naphthalene-d8	12.99	136	23562	40.00	ng	0.11
3) Acenaphthene-d10	18.65	164	234	40.00	ng	0.58
4) Phenanthrene-d10	17.59	188	118	40.00	ng	0.54
8) Chrysene-d12	0.00	240	0	0.00	ng	-30.48
9) Perylene-d12	0.00	264	0	0.00	ng	-34.55


Target Compounds					Ovalue
5) DDE	11.13	246	472	650.503 ng/uL#	26
6) DDD	11.55	235	275	171.871 ng/uL#	21
7) DDT	11.55	235	275	265.012 ng/uL#	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030618\
Data File : BF103489.D
Acq On : 7 Mar 2018 7:11
Operator : SJ/JU
Sample : J1809-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 07 07:59:49 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\DDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:24:24 2006
Response via : Initial Calibration

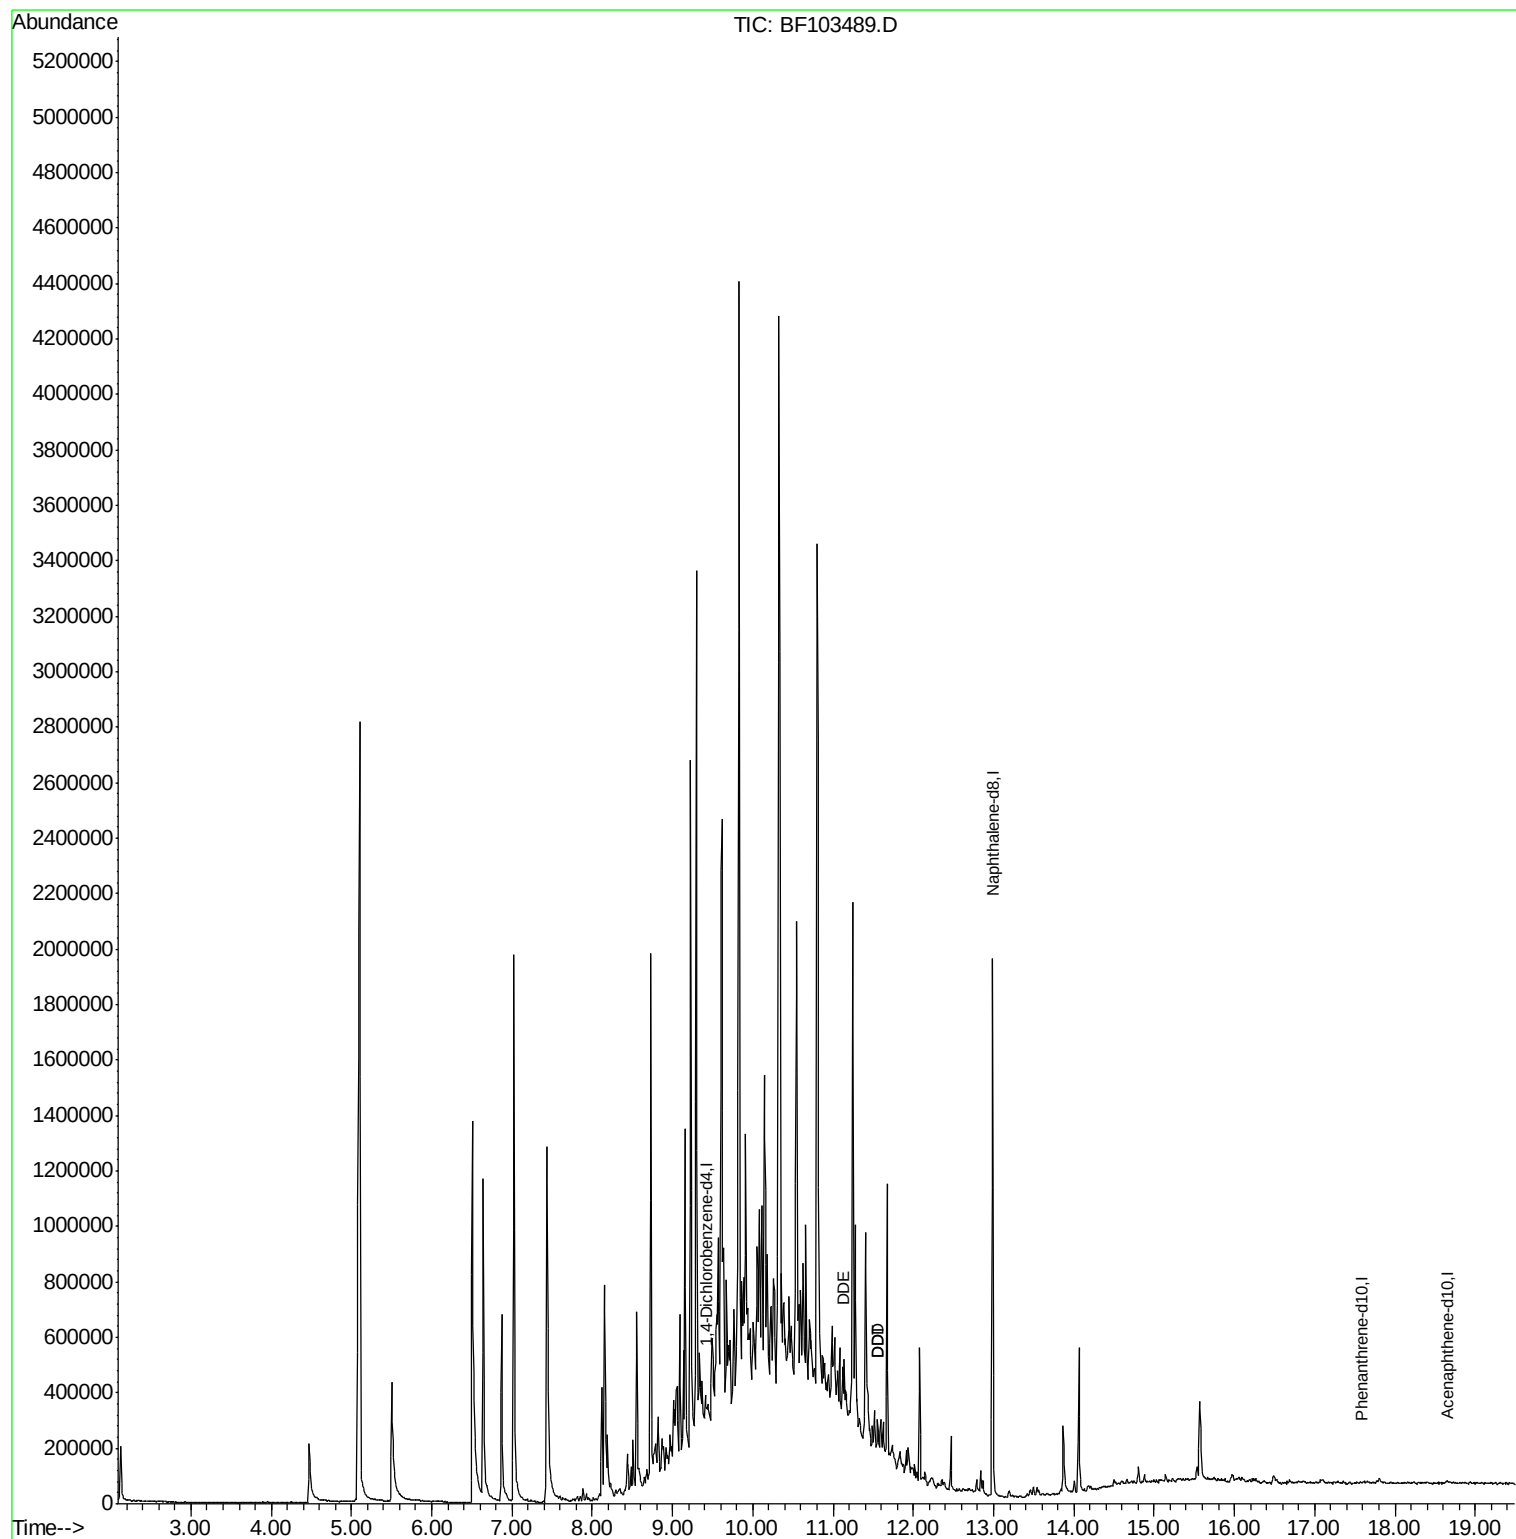

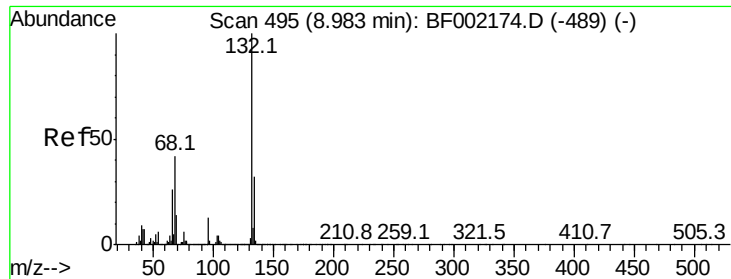

#5

DDE

Concen: 650.503 ng/uL

RT: 11.13 min Scan# 1537

Delta R.T. 0.33 min

Lab File: BF103489.D

Acq: 7 Mar 2018 7:11

Instrument :

BNA_F

ClientSampleId :

Tot Ion:246 Resp: 472


Ion Ratio Lower Upper

246 100

248 0.0 41.8 62.6#

318 0.0 0.0 0.0

176 414.0 0.0 0.0#



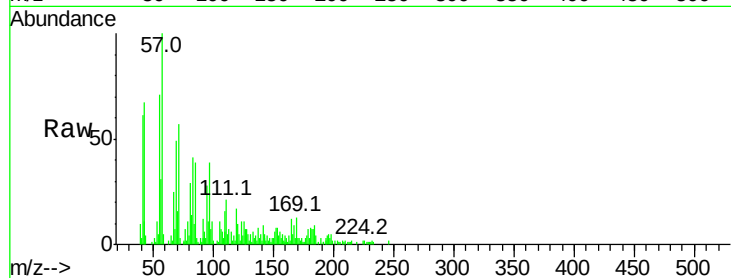


Abundance Ion 246.00 (245.70 to 246.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 318.00 (317.70 to 318.70): E

Ion 176.00 (175.70 to 176.70): E

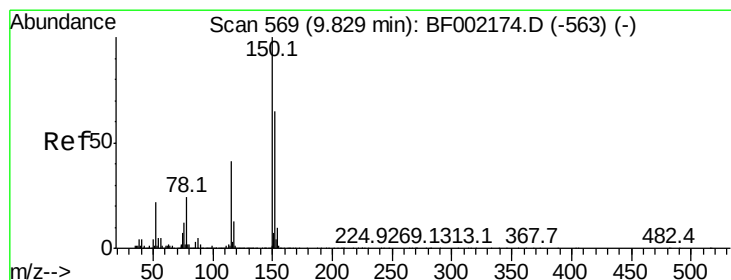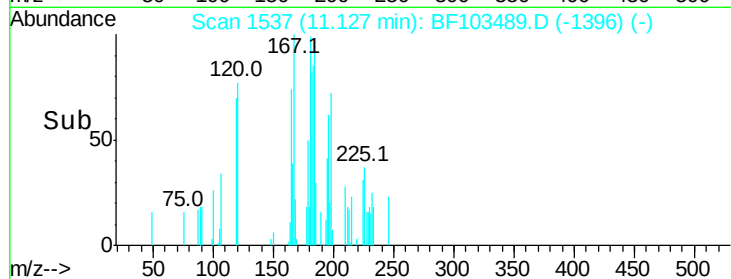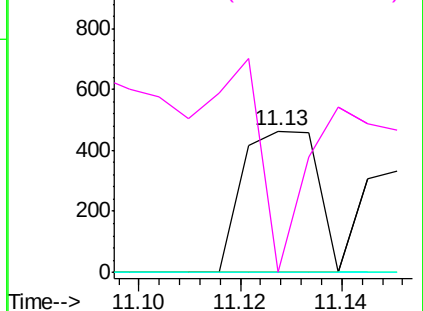

#6

DDD

Concen: 171.871 ng/uL

RT: 11.55 min Scan# 1609

Delta R.T. 0.35 min

Lab File: BF103489.D

Acq: 7 Mar 2018 7:11


Tgt Ion:235 Resp: 275

Ion Ratio Lower Upper

235 100

237 0.0 51.7 77.5#



165 0.0 44.0 66.0#

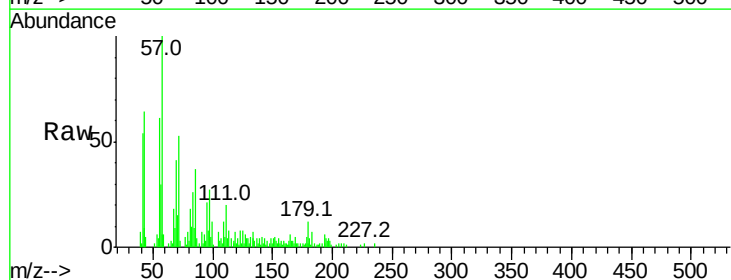


Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E

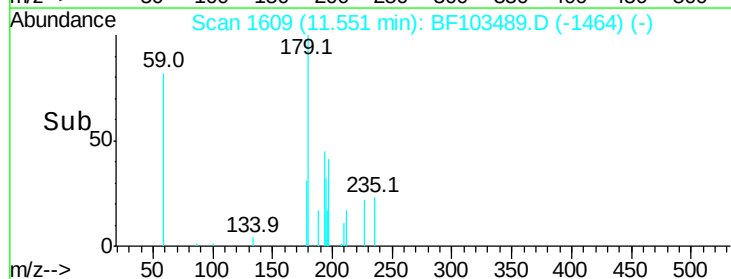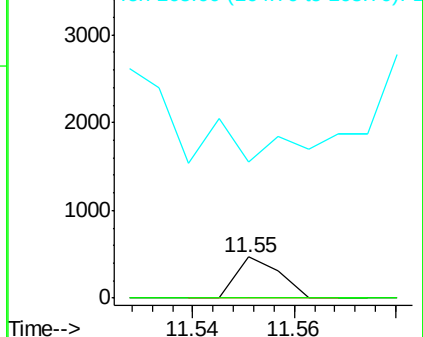

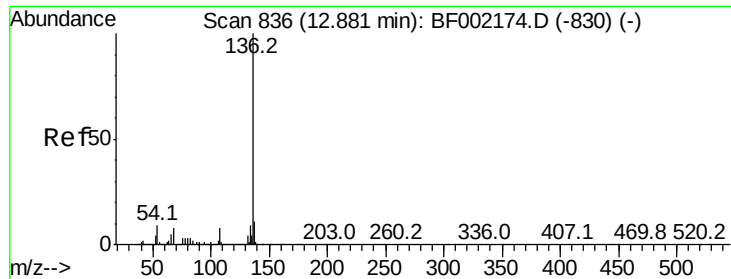

#7

DDT

Concen: 265.012 ng/uL

RT: 11.55 min Scan# 1609

Delta R.T. -0.00 min


Lab File: BF103489.D

Acq: 7 Mar 2018 7:11

Instrument :

BNA_F

ClientSampleId :

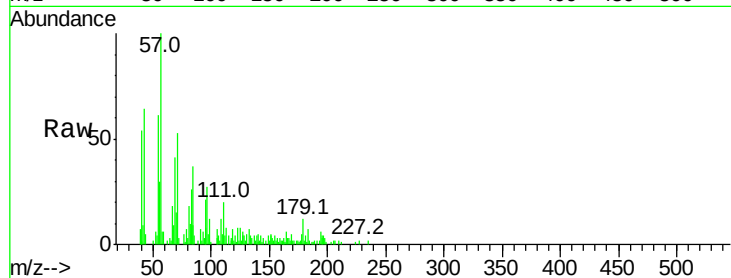


Tot Ion: 235 Resp: 275

Ion Ratio Lower Upper

235 100

237 0.0 0.0 0.0

165 0.0 0.0 0.0

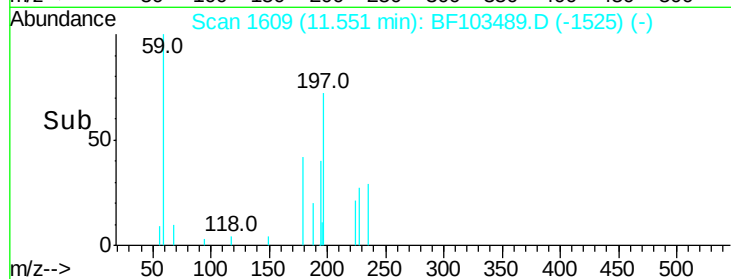

Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E

