

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030618\
 Data File : BF103479.D
 Acq On : 7 Mar 2018 1:54
 Operator : SJ/JU
 Sample : J1810-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MHA-WCS

Manual Integrations
 APPROVED

Sohil
 3/7/2018 12:17:45 PM

Quant Time: Mar 07 06:42:18 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 06 11:52:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	129442	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	525769	20.00	ng	0.00
38) Acenaphthene-d10	9.91	164	206180	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	299695	20.00	ng	0.00
75) Chrysene-d12	14.06	240	185161	20.00	ng	0.00
86) Perylene-d12	15.57	264	143166	20.00	ng	0.00

Sohil

System Monitoring Compounds

5) 2-Fluorophenol	5.50	112	847959	99.08	ng	0.00
7) Phenol-d6	6.51	99	1071446	102.31	ng	0.00
23) Nitrobenzene-d5	7.43	82	698114	75.83	ng	-0.01
41) 2,4,6-Tribromophenol	10.71	330	131430	75.31	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	870868	69.67	ng	0.00
78) Terphenyl-d14	12.99	244	560573	72.78	ng	0.00

3/7/2018 12:17:45 PM

Target Compounds

						Qvalue
49) Dimethylphthalate	9.62	163	93200	5.635	ng	99
51) Acenaphthene	9.95	154	27323	2.228	ng	92
57) Fluorene	10.46	166	36652	2.556	ng	# 96
70) Phenanthrene	11.43	178	447819	27.152	ng	99
71) Anthracene	11.49	178	129440	7.653	ng	100
72) Carbazole	11.65	167	48767	2.896	ng	# 94
74) Fluoranthene	12.63	202	637856	38.486	ng	98
77) Pyrene	12.86	202	584795	40.509	ng	100
80) Benzo(a)anthracene	14.05	228	258800	21.542	ng	98
82) Chrysene	14.09	228	243994	20.916	ng	98
85) Indeno(1,2,3-cd)pyrene	17.12	276	93472	10.121	ng	96
87) Benzo(b)fluoranthene	15.13	252	244756m	26.002	ng	
88) Benzo(k)fluoranthene	15.16	252	69236m	7.811	ng	
89) Benzo(a)pyrene	15.51	252	164833	19.609	ng	# 90
90) Dibenzo(a,h)anthracene	17.12	278	24203	3.726	ng	# 75
91) Benzo(g,h,i)perylene	17.60	276	88281	13.907	ng	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF030618\
Data File : BF103479.D
Acq On : 7 Mar 2018 1:54
Operator : SJ/JU
Sample : J1810-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MHA-WCS

Manual Integrations
APPROVED

Sohil
3/7/2018 12:17:45 PM

Quant Time: Mar 07 06:42:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 11:52:59 2018
Response via : Initial Calibration

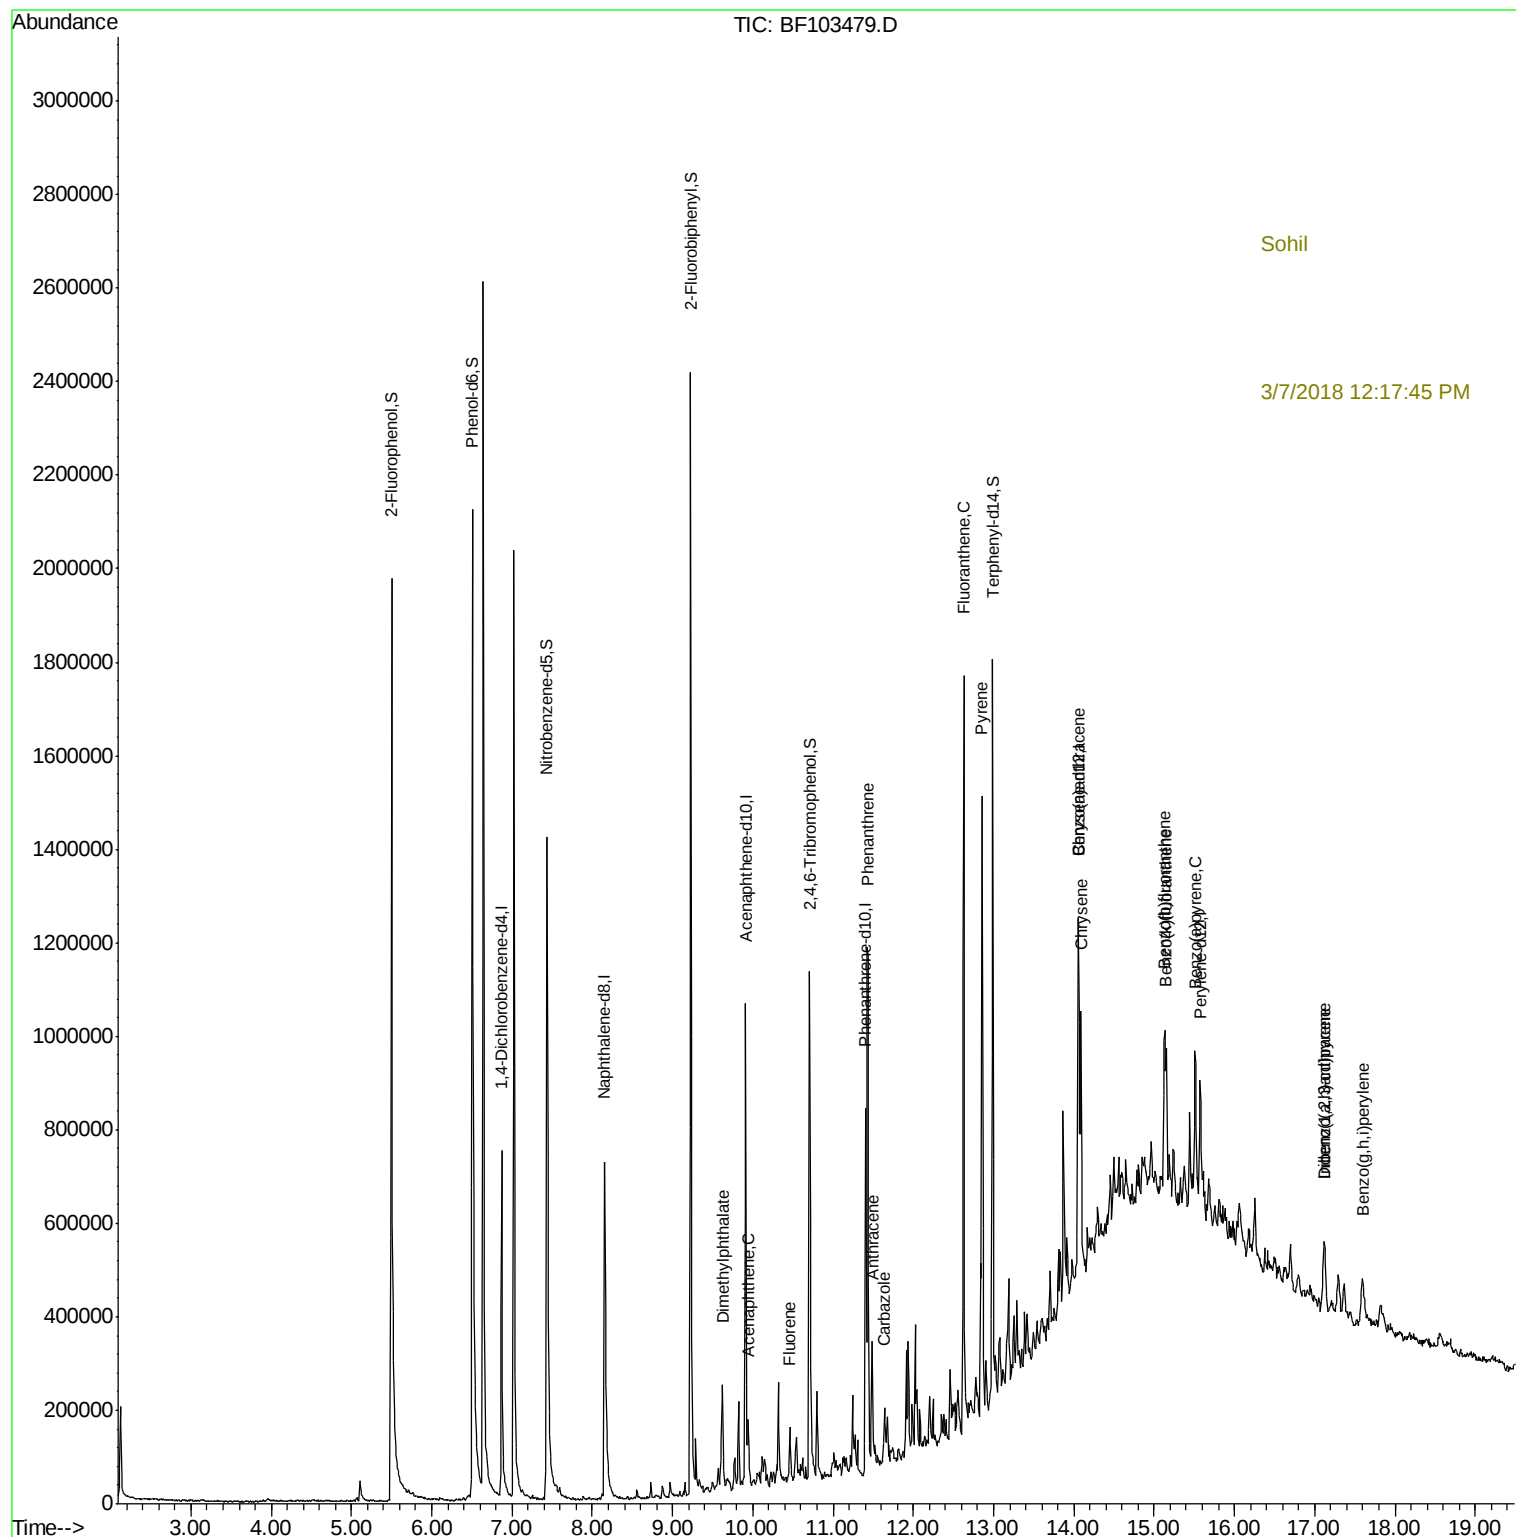

Sohil

3/7/2018 12:17:45 PM