


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF030618\
 Data File : BF103486.D
 Acq On : 7 Mar 2018 5:51
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 07 11:40:36 2018

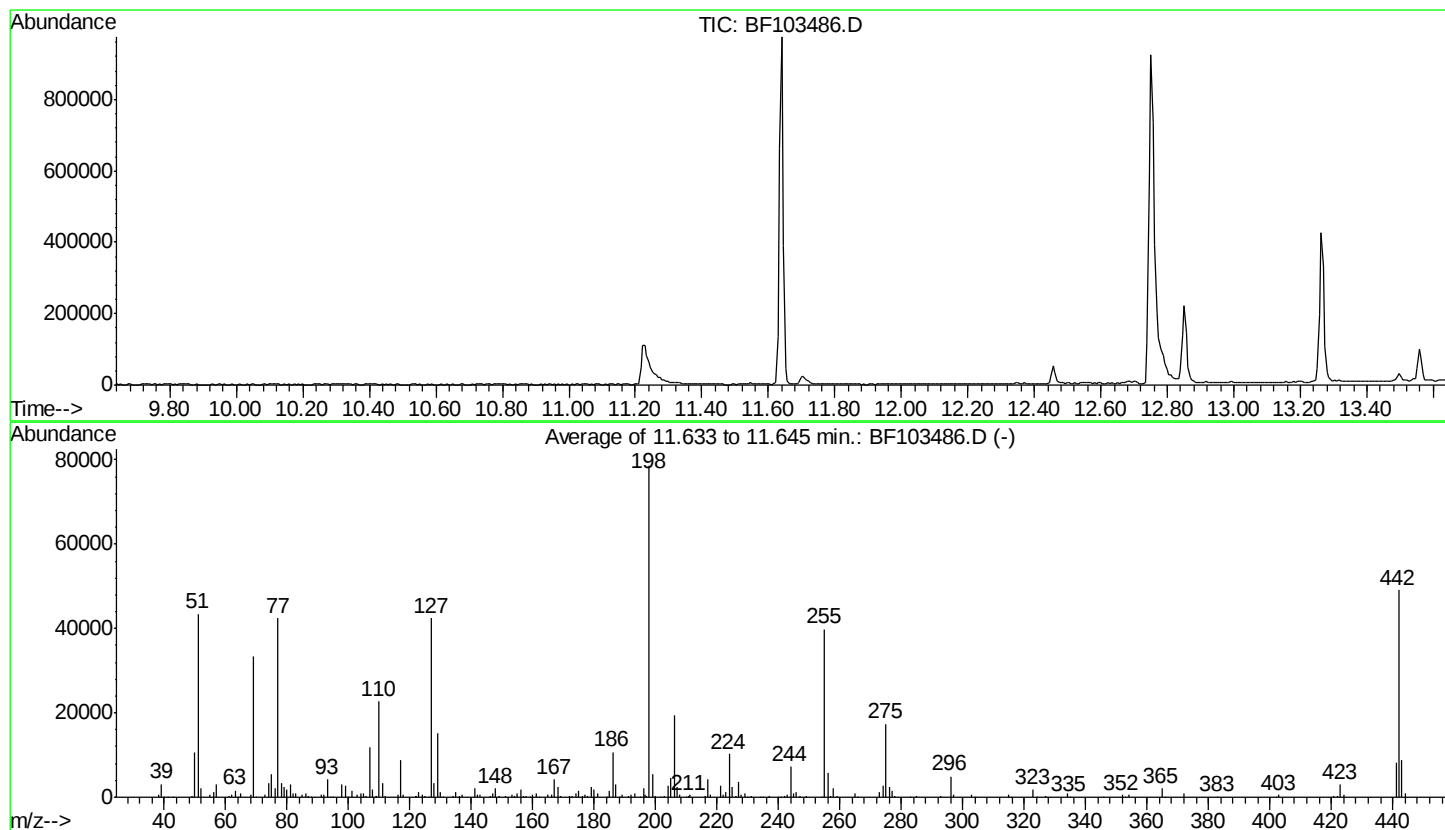

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	43413	PASS
68	69	0.00	2	1.7	575	PASS
69	198	0.00	100	42.6	33525	PASS
70	69	0.00	2	0.3	115	PASS
127	198	10	80	53.9	42354	PASS
197	198	0.00	2	0.4	288	PASS
198	198	100	100	100.0	78629	PASS
199	198	5	9	6.8	5356	PASS
275	198	10	60	22.1	17384	PASS
365	198	1	100	2.7	2117	PASS
441	443	0.01	100	92.1	8238	PASS
442	198	50	100	62.4	49085	PASS
443	442	15	24	18.2	8947	PASS