
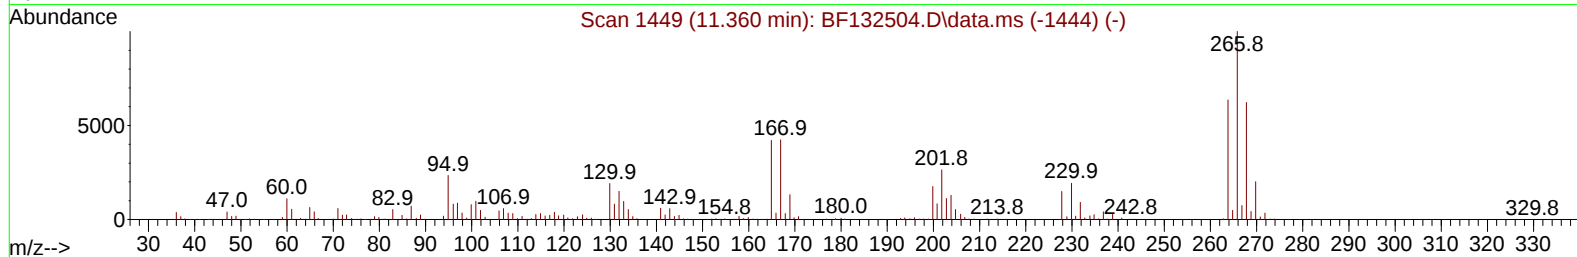
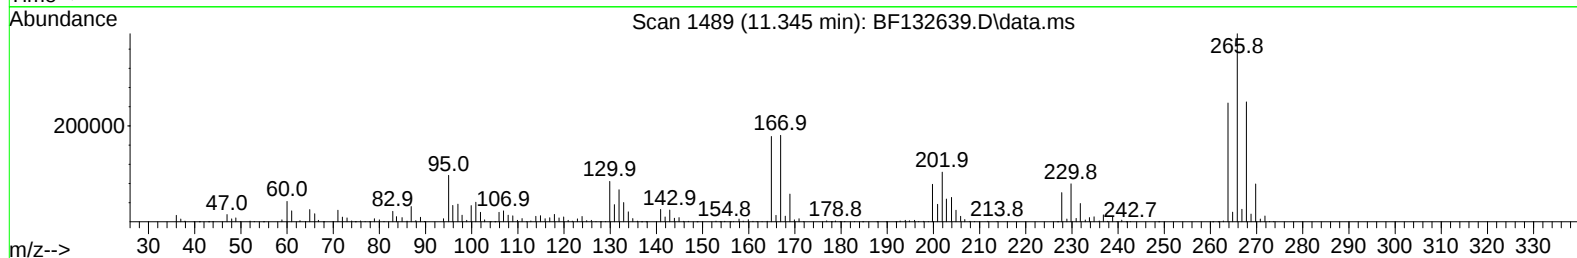


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132639.D
Acq On : 06 Mar 2023 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 05:35:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

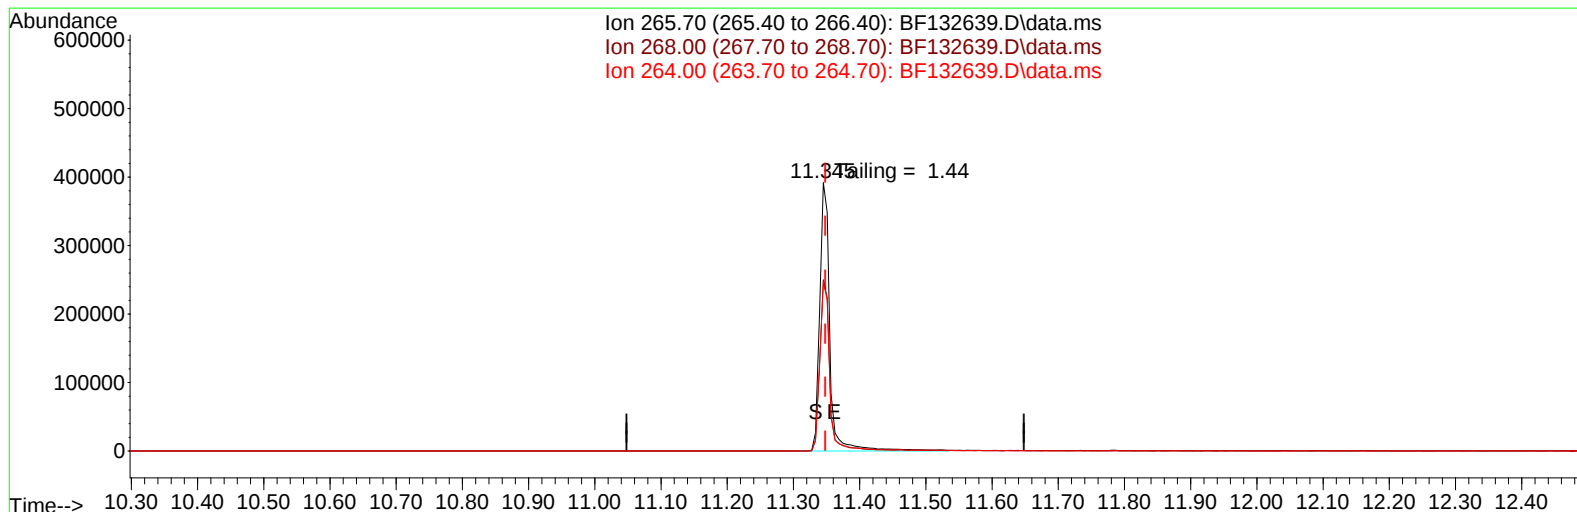




TIC: BF132639.D\data.ms

(70) Pentachlorophenol (C)**11.345min (-0.003) 180966.54 ng****response 415211**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.78
264.00	63.60	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
 Data File : BF132639.D
 Acq On : 06 Mar 2023 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 05:35:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 23:17:30 2023
 Response via : Initial Calibration

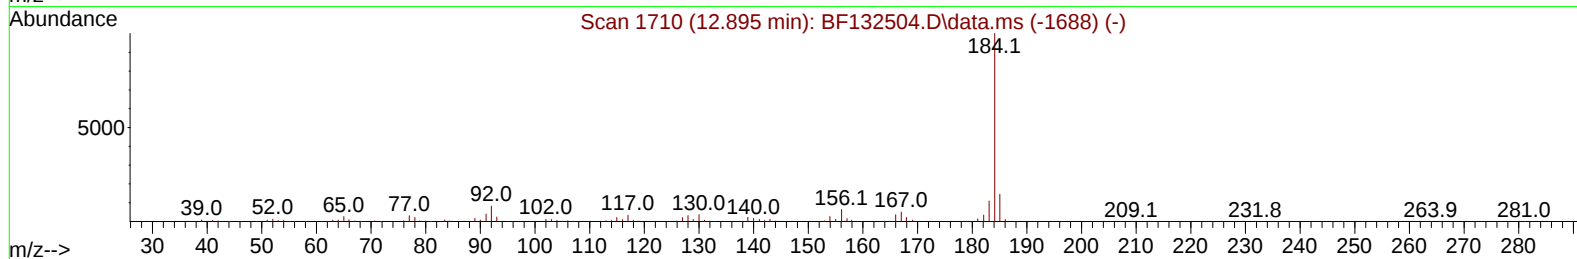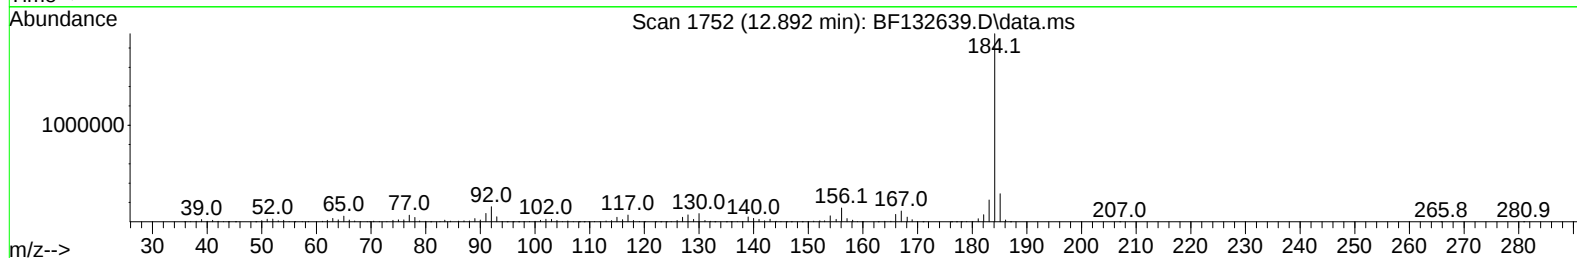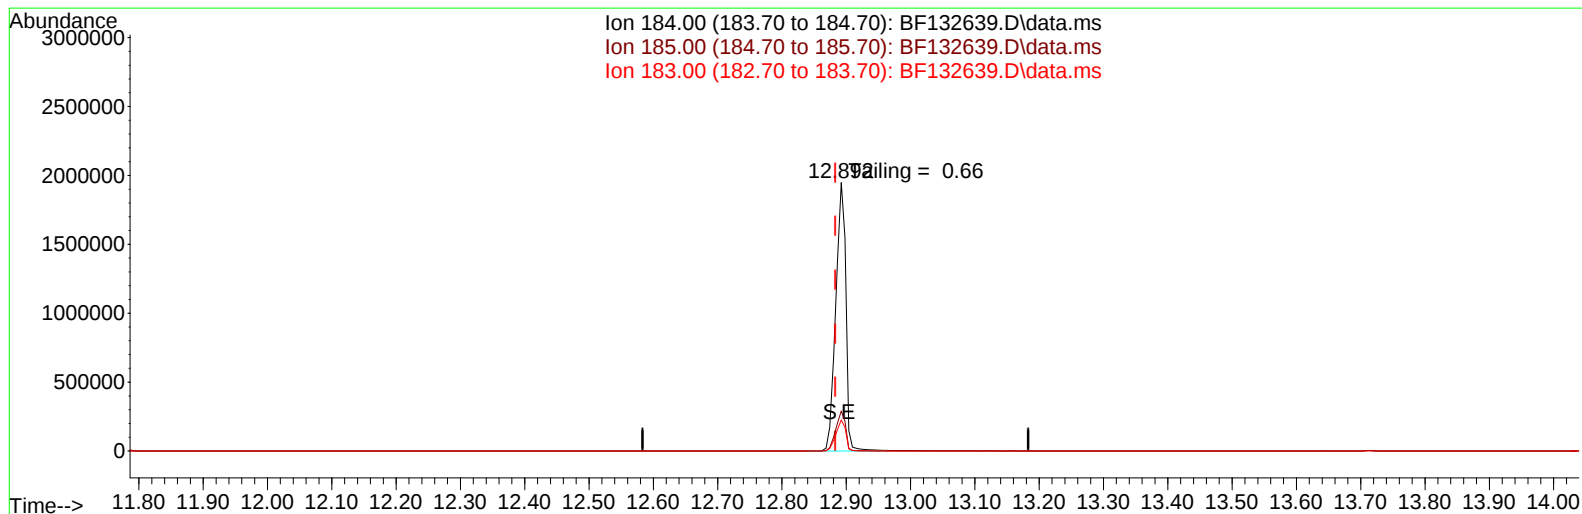

TIC: BF132639.D\data.ms

(77) Benzidine**12.892min (+ 0.009) 290725.51 ng****response 2137281**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.91
183.00	10.90	11.56
0.00	0.00	0.00