
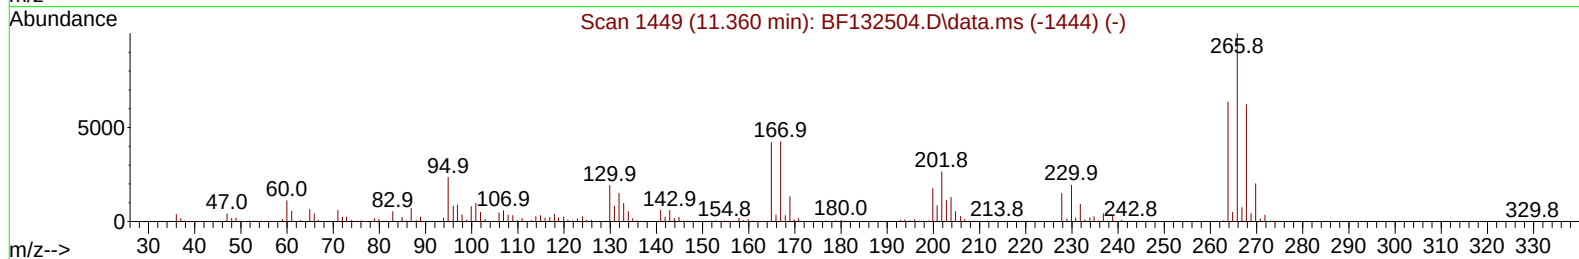
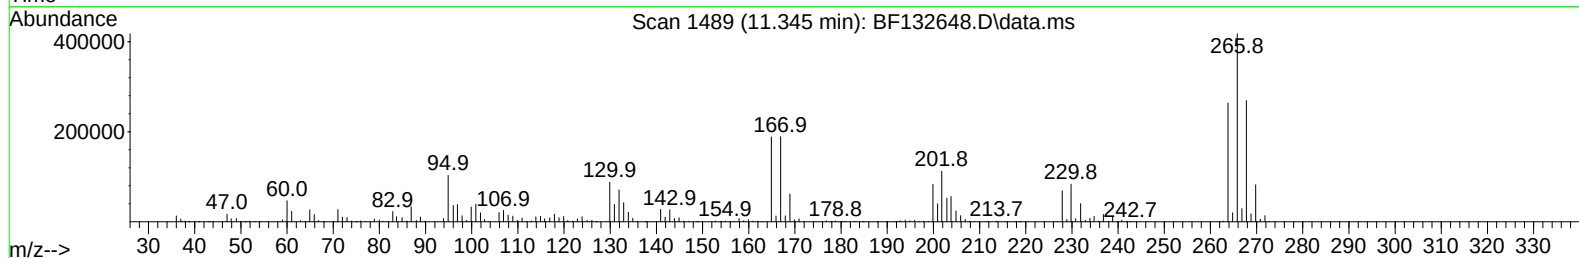


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132648.D
Acq On : 06 Mar 2023 14:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 05:36:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

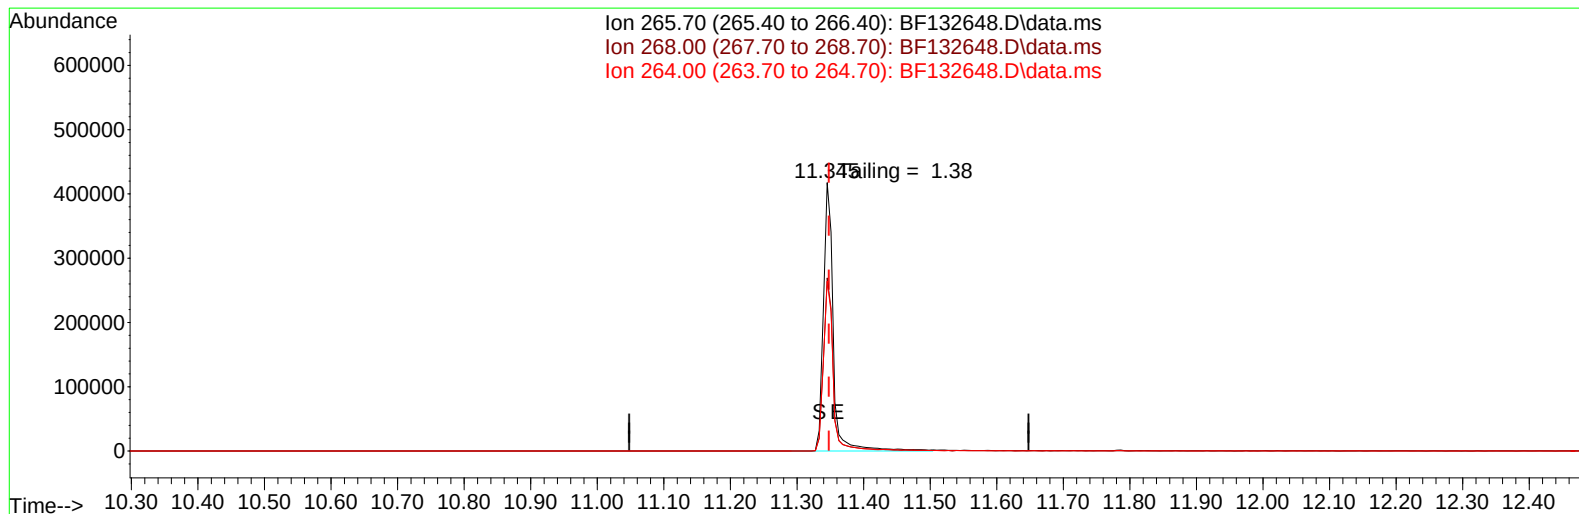

TIC: BF132648.D\data.ms

(70) Pentachlorophenol (C)




11.345min (-0.003) 279512.02 ng

response 427543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.46
264.00	63.60	63.19
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\  
Data File : BF132648.D  
Acq On    : 06 Mar 2023  14:48  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 07 05:36:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

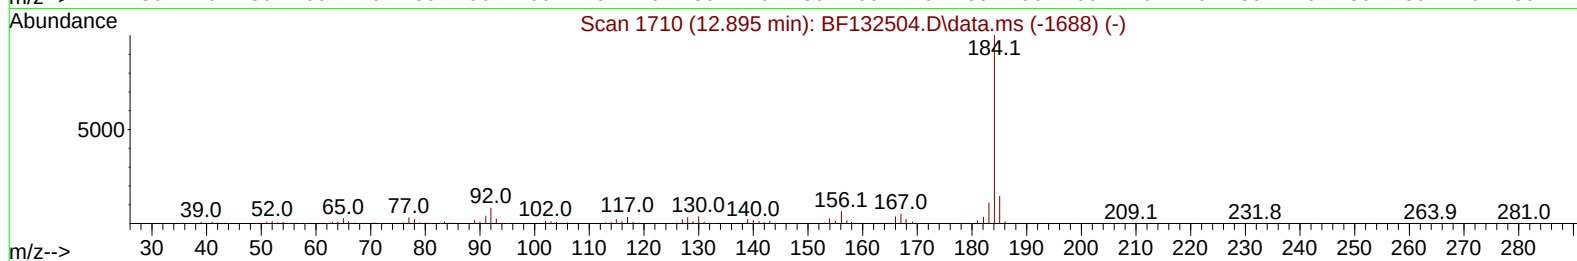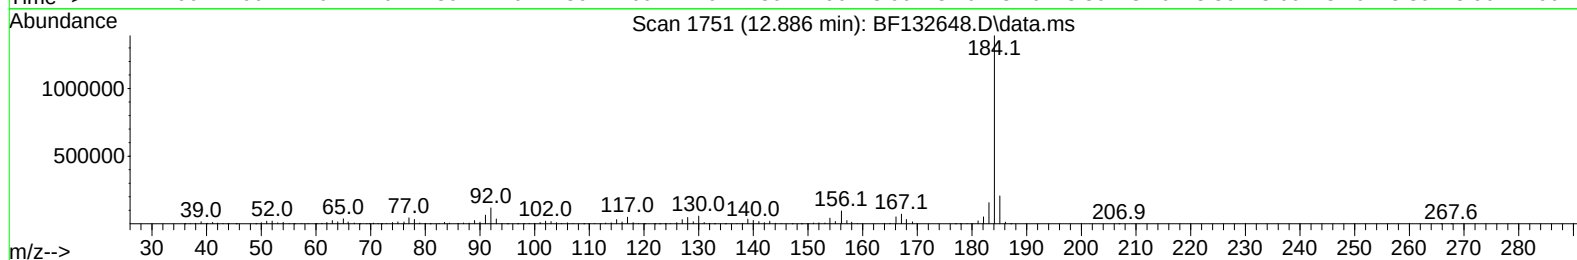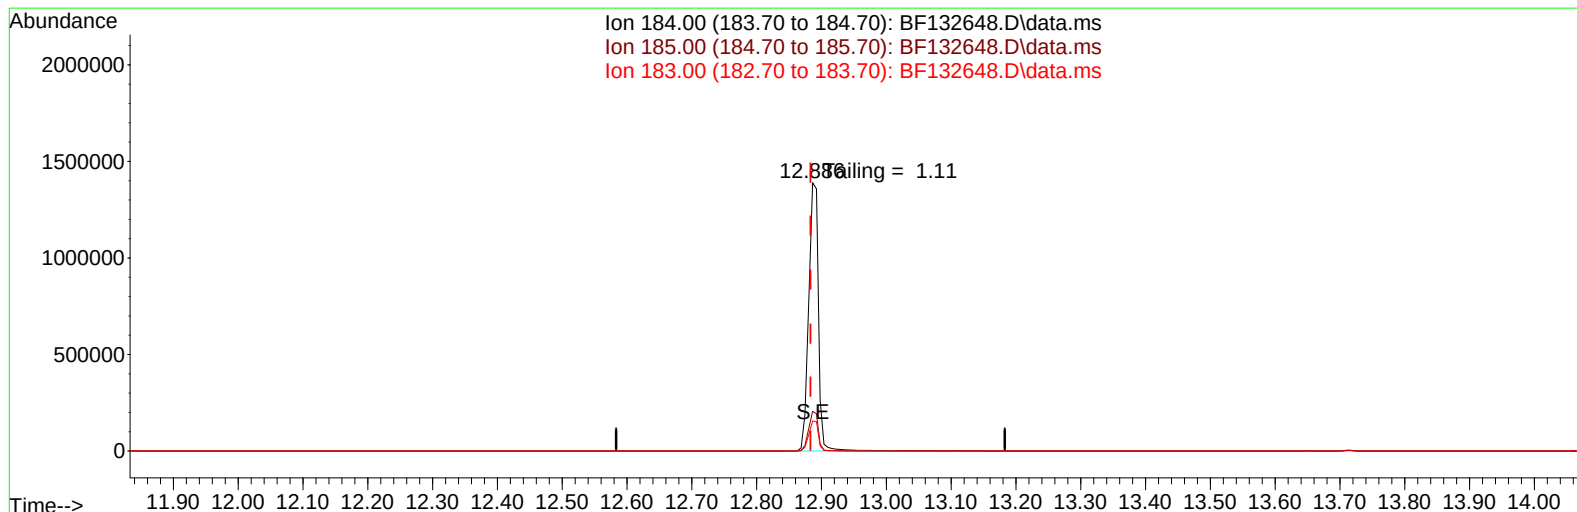

TIC: BF132648.D\data.ms

(77) Benzidine

12.886min (+ 0.003) 255996.11 ng

```
response      1464444
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.82
183.00	10.90	11.22
0.00	0.00	0.00