

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
 Data File : BF132641.D
 Acq On : 06 Mar 2023 10:13
 Operator : CG\JU
 Sample : PB151188BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB151188BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	446	452	462	rBV	1751280	2427791	35.83%	5.736%
2	5.634	513	518	522	rBV	4510144	5070533	74.83%	11.980%
3	6.628	682	687	690	rBV	4343393	5123526	75.61%	12.105%
4	6.998	746	750	754	rBV	1524208	1193057	17.61%	2.819%
5	7.569	841	847	850	rBV	3310715	3445287	50.84%	8.140%
6	8.286	965	969	972	rBV	1856597	1542269	22.76%	3.644%
7	9.363	1146	1152	1155	rBV	6642682	5919051	87.35%	13.984%
8	10.045	1264	1268	1272	rBV	2170167	1840566	27.16%	4.348%
9	10.845	1399	1404	1407	rBV	4064488	4008438	59.15%	9.470%
10	11.539	1519	1522	1526	rBV	2058341	1961166	28.94%	4.633%
11	13.139	1789	1794	1797	rBV	6795652	6776211	100.00%	16.009%
12	14.204	1971	1975	1979	rBV	1859672	1671986	24.67%	3.950%
13	15.757	2233	2239	2246	rBV	1022510	1346642	19.87%	3.182%




Sum of corrected areas: 42326523

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132641.D
Acq On : 06 Mar 2023 10:13
Operator : CG\JU
Sample : PB151188BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

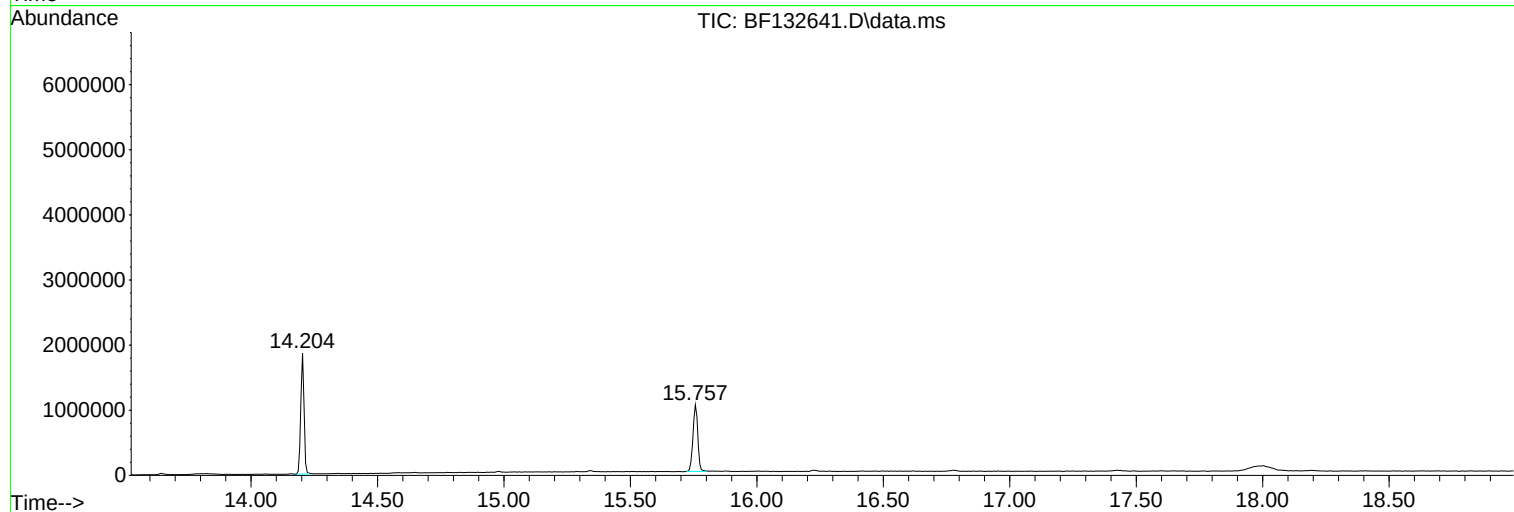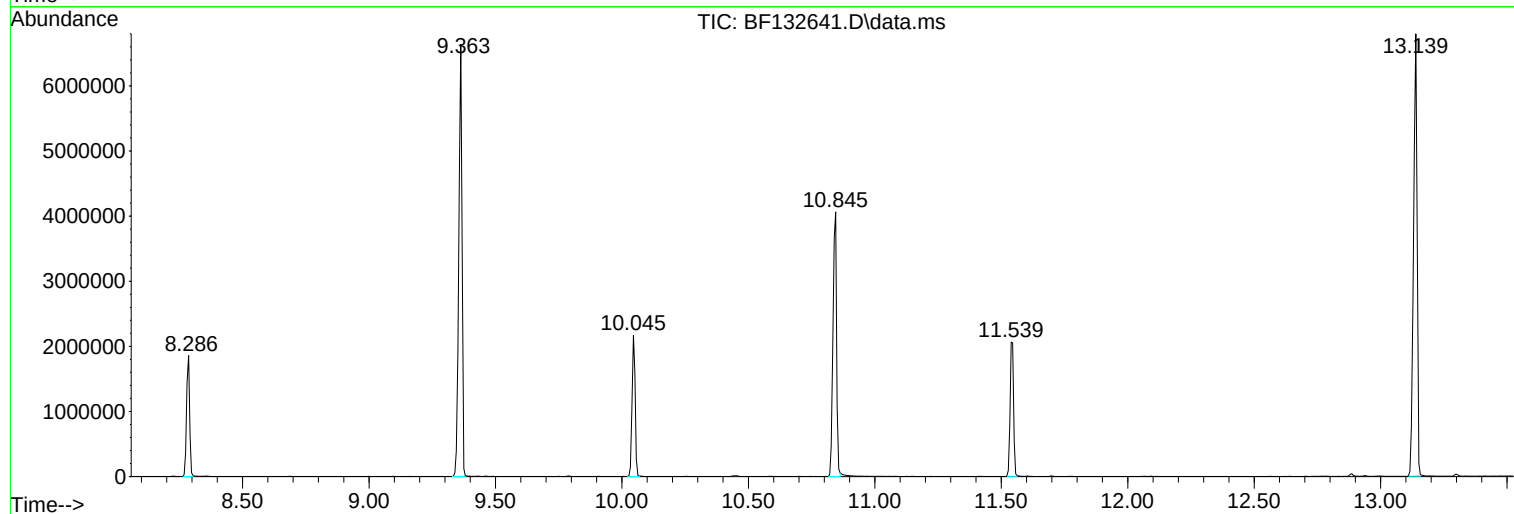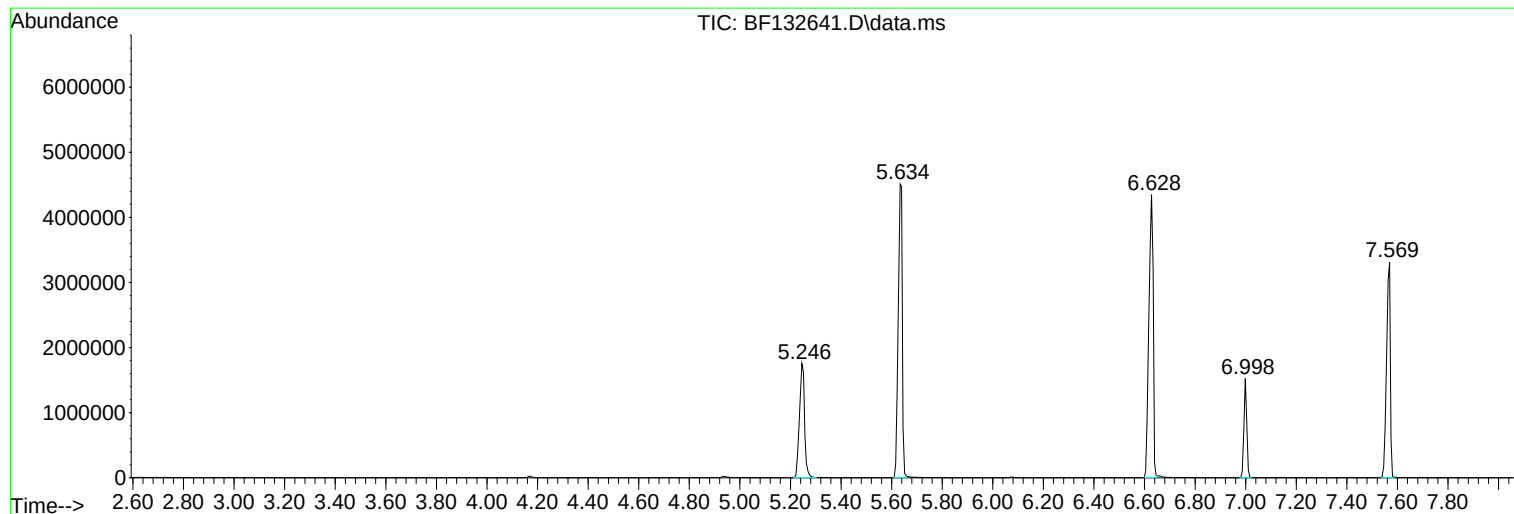

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132641.D
Acq On : 06 Mar 2023 10:13
Operator : CG\JU
Sample : PB151188BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151188BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.246	40.70 ng	2427790	1,4-Dichlorobenzene-d4	6.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	50		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

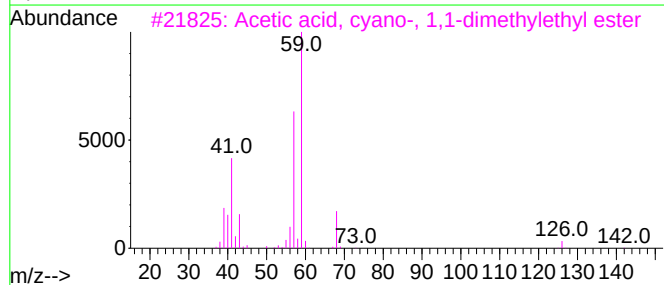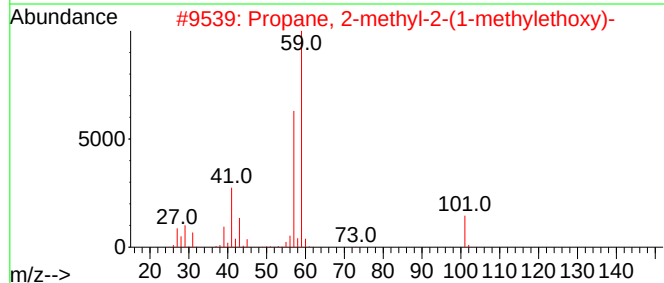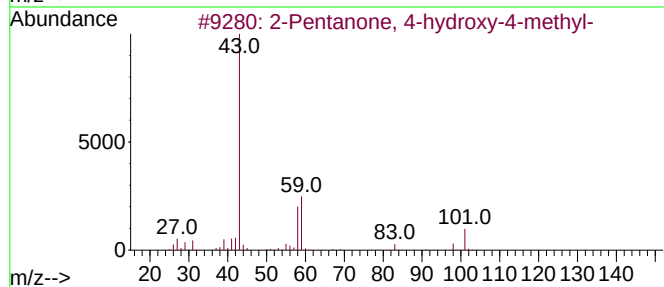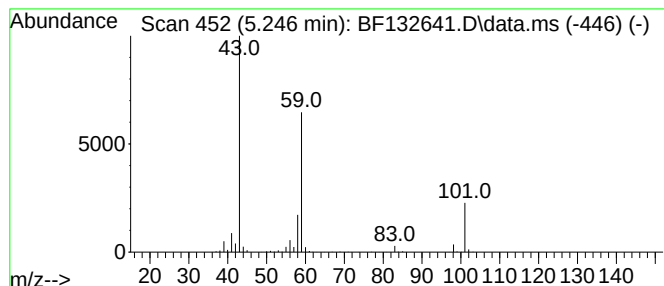

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132641.D
Acq On : 06 Mar 2023 10:13
Operator : CG\JU
Sample : PB151188BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.246	40.7	ng	2427790	1	6.998	1193060	20.0