

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
 Data File : BF132645.D
 Acq On : 06 Mar 2023 12:31
 Operator : CG\JU
 Sample : PB151233BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB151233BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	446	452	464	rBV	1693113	2420257	36.14%	5.777%
2	5.634	513	518	522	rBV	4493395	5018561	74.93%	11.978%
3	6.628	681	687	690	rBV	4262980	5015903	74.89%	11.972%
4	6.998	746	750	753	rBV	1509276	1178792	17.60%	2.813%
5	7.569	841	847	850	rBV	3208853	3415010	50.99%	8.151%
6	8.287	965	969	972	rBV	1777469	1521989	22.72%	3.633%
7	9.363	1146	1152	1155	rBV	6380811	5956125	88.93%	14.216%
8	10.045	1264	1268	1272	rBV	2159447	1833727	27.38%	4.377%
9	10.845	1399	1404	1407	rBV	4056171	3987281	59.53%	9.517%
10	11.545	1519	1523	1526	rBV	2242727	1987395	29.67%	4.743%
11	13.139	1789	1794	1797	rBV	6631948	6697716	100.00%	15.986%
12	14.204	1971	1975	1981	rBV	1746674	1573671	23.50%	3.756%
13	15.757	2233	2239	2248	rBV2	940717	1291753	19.29%	3.083%




Sum of corrected areas: 41898180

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132645.D
Acq On : 06 Mar 2023 12:31
Operator : CG\JU
Sample : PB151233BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151233BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

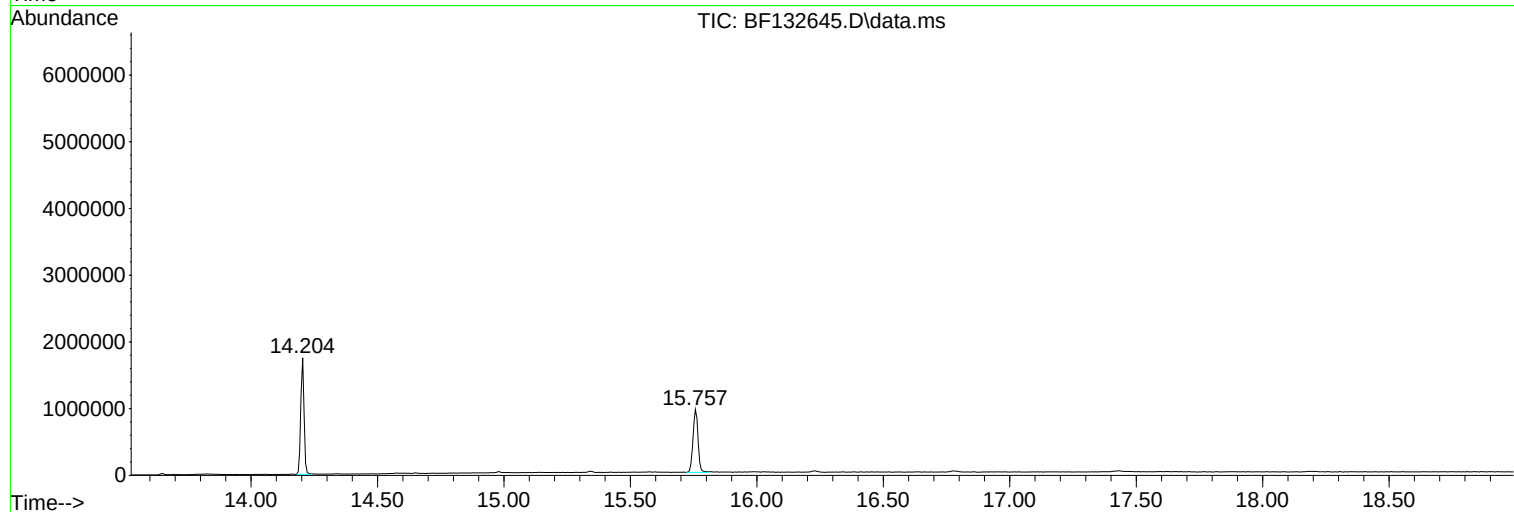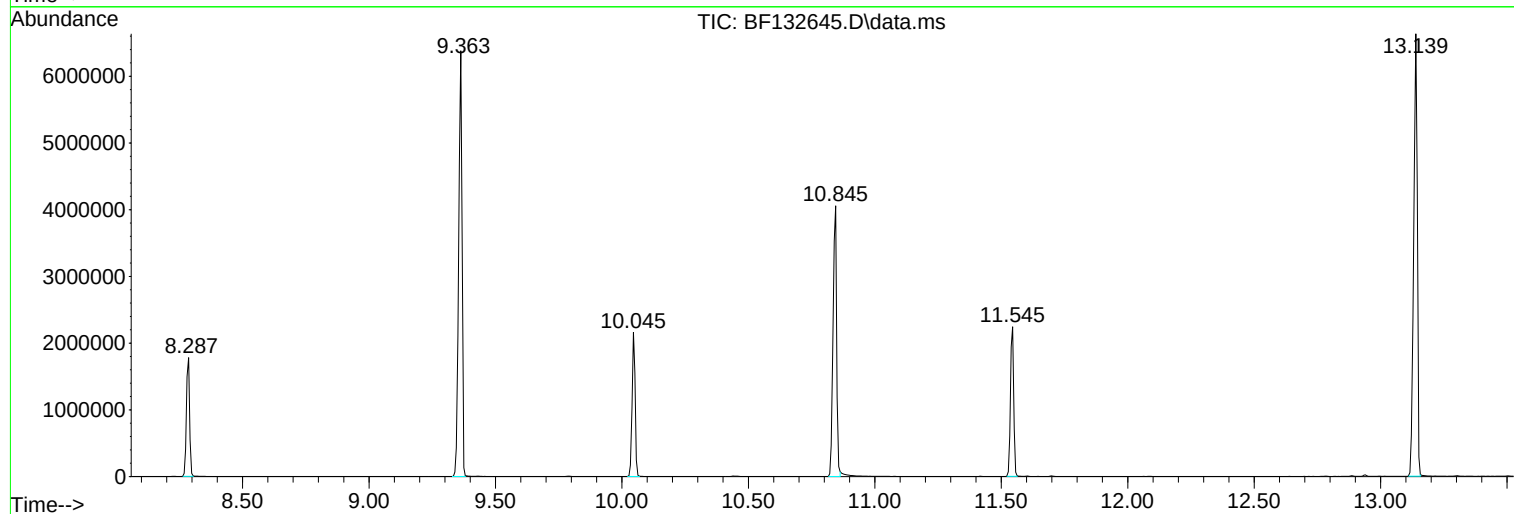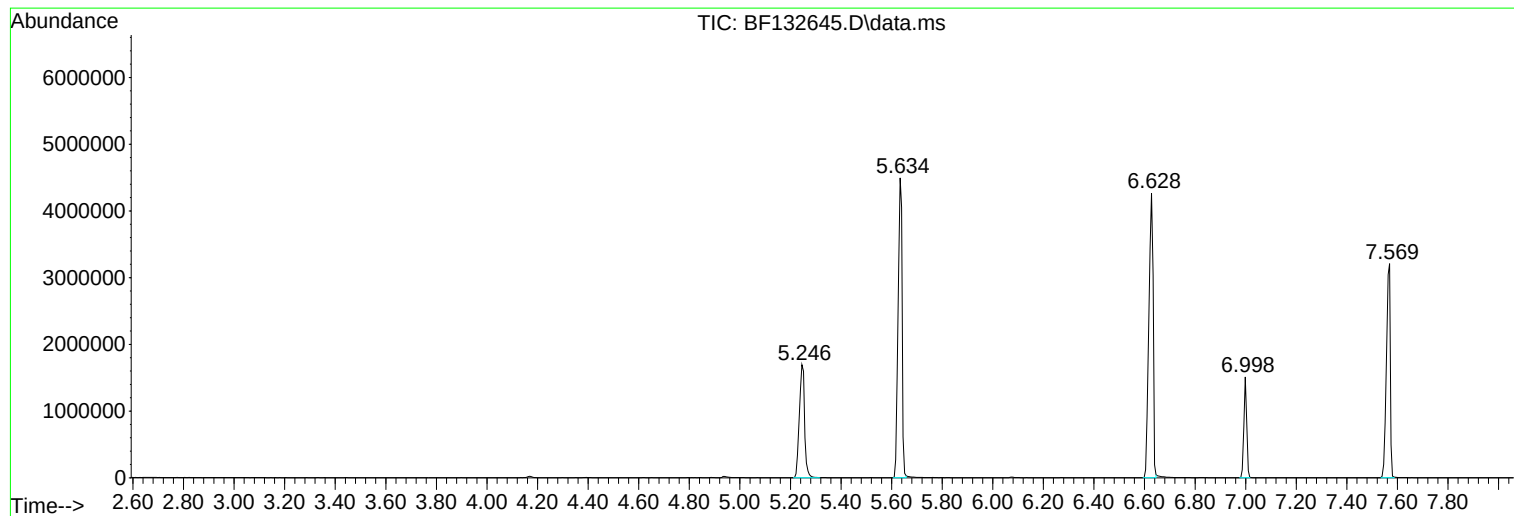

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132645.D
Acq On : 06 Mar 2023 12:31
Operator : CG\JU
Sample : PB151233BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151233BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.246	41.06 ng	2420260	1,4-Dichlorobenzene-d4	6.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		
5	Acetone	58	C3H6O	000067-64-1	9		

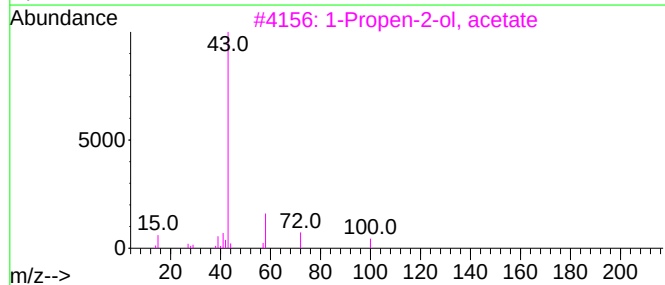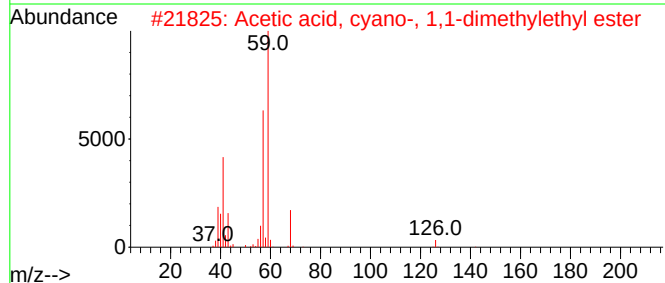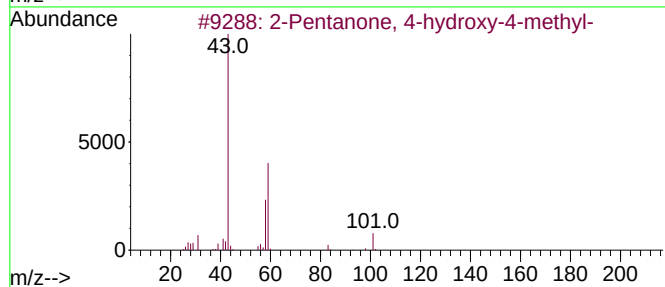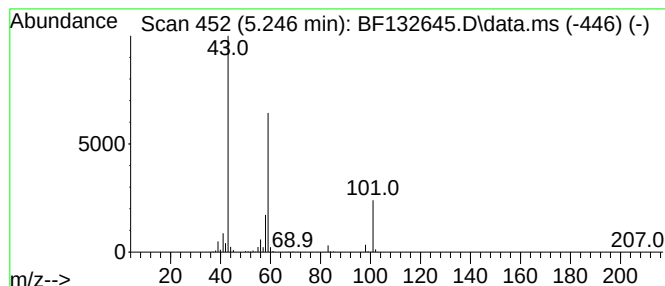

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132645.D
Acq On : 06 Mar 2023 12:31
Operator : CG\JU
Sample : PB151233BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151233BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.246	41.1	ng	2420260	1	6.998	1178790	20.0