
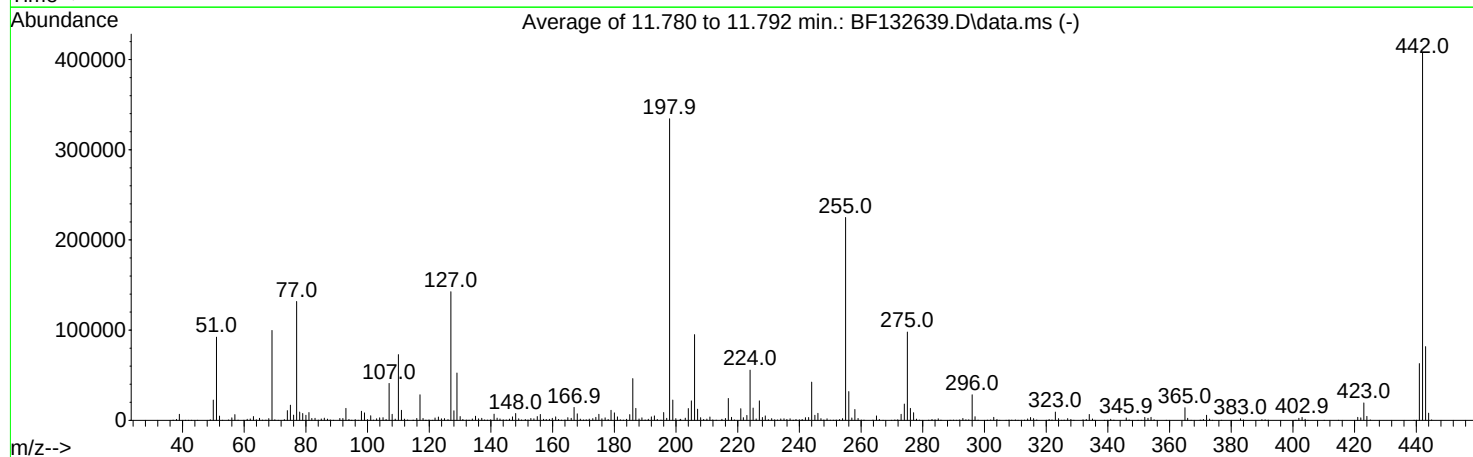


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132639.D
Acq On : 06 Mar 2023 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 23:17:30 2023

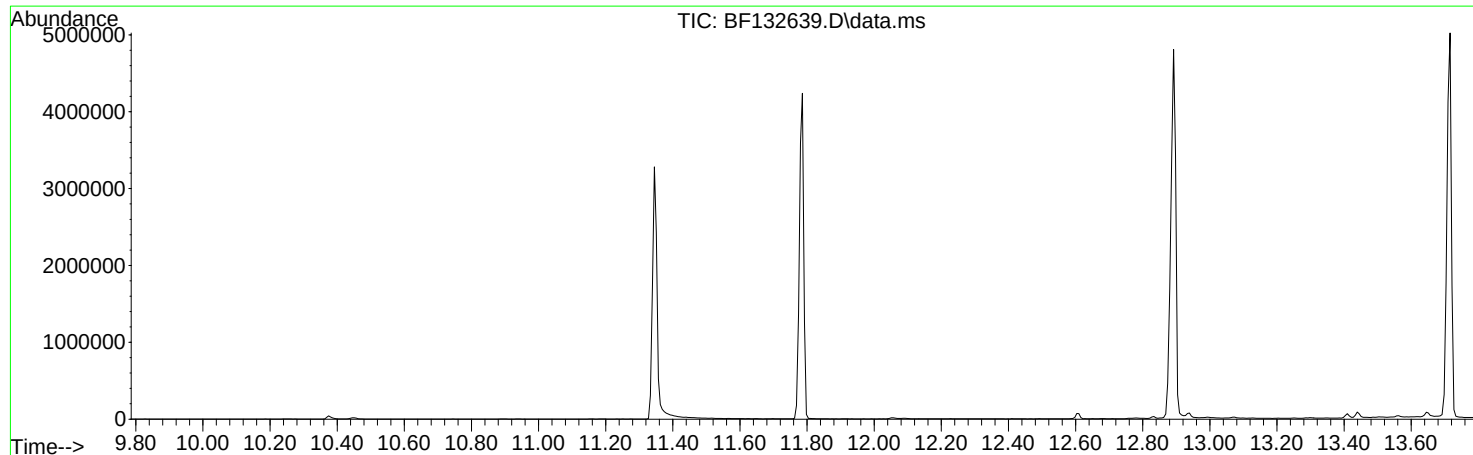




AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	92112	PASS
68	69	0.00	2	1.9	1903	PASS
69	198	0.00	100	29.8	99584	PASS
70	69	0.00	2	0.6	635	PASS
127	198	10	80	42.6	142576	PASS
197	198	0.00	2	0.7	2296	PASS
198	198	100	100	100.0	334373	PASS
199	198	5	9	6.7	22417	PASS
275	198	10	60	29.3	97837	PASS
365	198	1	100	4.2	14023	PASS
441	198	0.01	100	18.8	62979	PASS
442	442	50	100	100.0	407957	PASS
443	442	15	24	20.0	81707	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
 Data File : BF132639.D
 Acq On : 06 Mar 2023 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 07 05:35:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 23:17:30 2023
 Response via : Initial Calibration

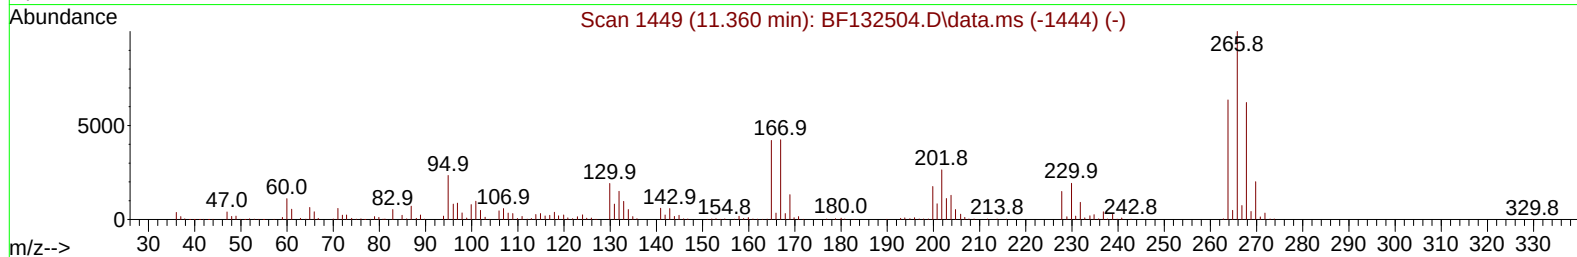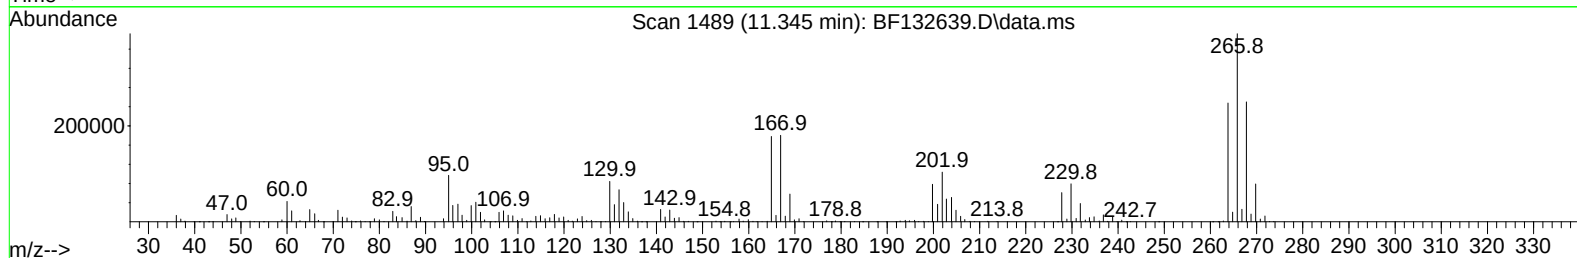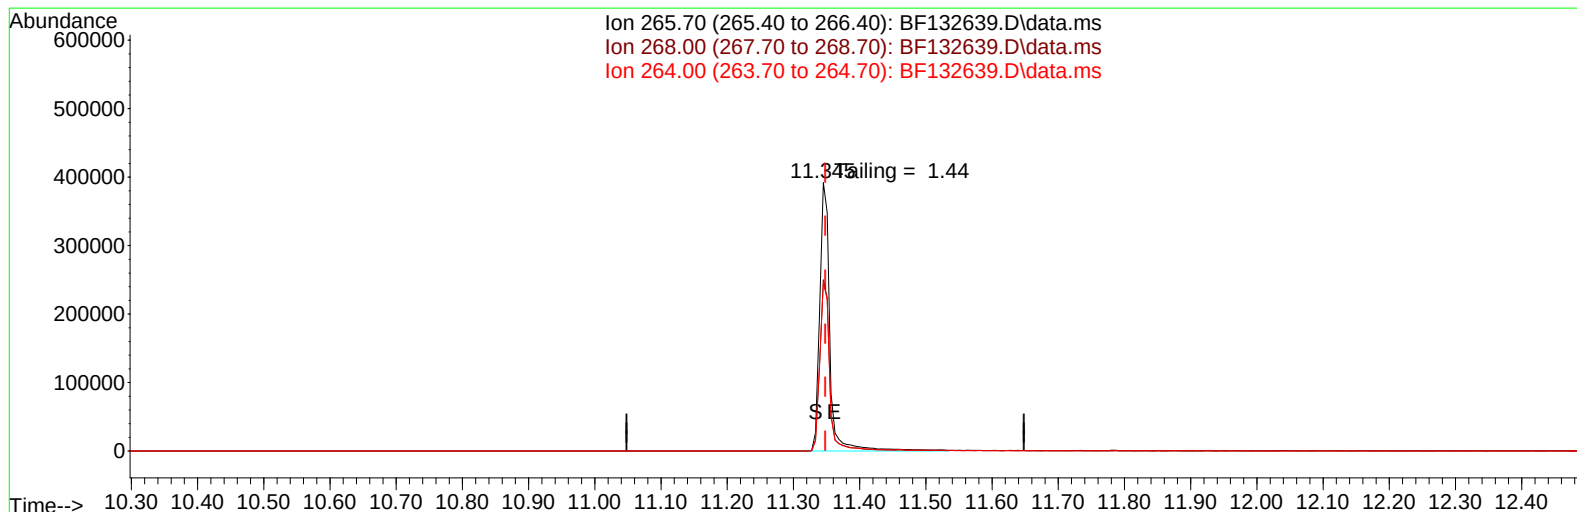

TIC: BF132639.D\data.ms

(70) Pentachlorophenol (C)

11.345min (-0.003) 180966.54 ng




response 415211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.78
264.00	63.60	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132639.D
Acq On : 06 Mar 2023 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 05:35:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

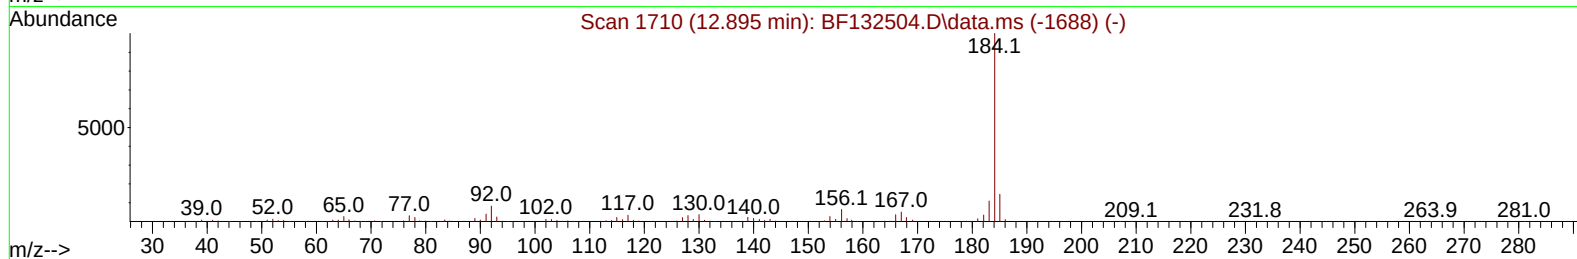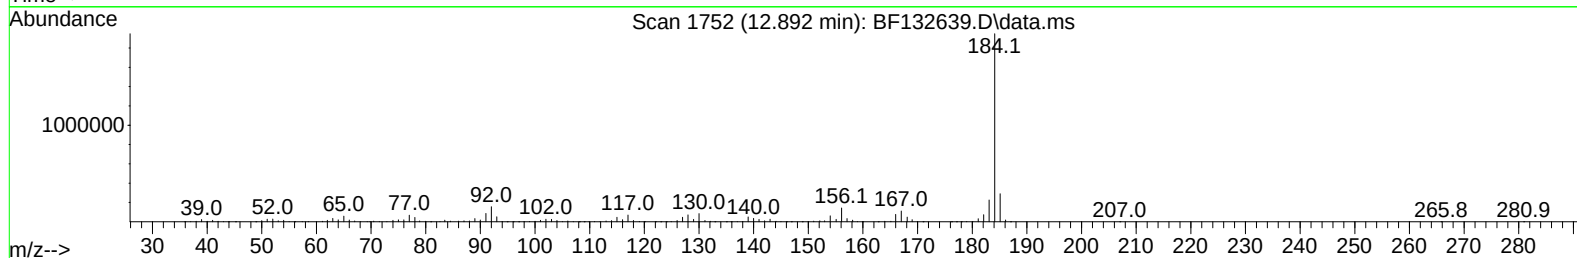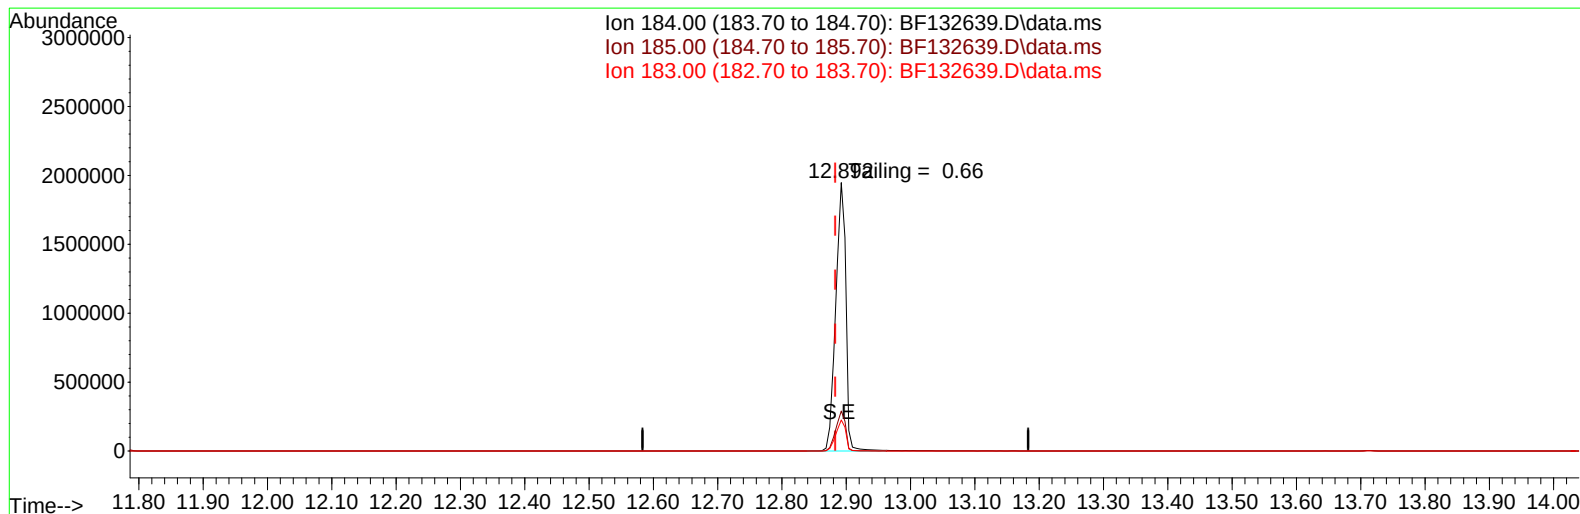

TIC: BF132639.D\data.ms

(77) Benzidine

12.892min (+ 0.009) 290725.51 ng

response 2137281

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.91
183.00	10.90	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/6/2023	BNA_F	<u>BF132639.D</u>
Compound Name	Response	Retention Time
DDT	962737	13.716
DDD	24145	13.439
DDE	2897	13.069
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27042	989779	2.73

Instrument :
BNA_F
ClientSampleId :
DFTPP