
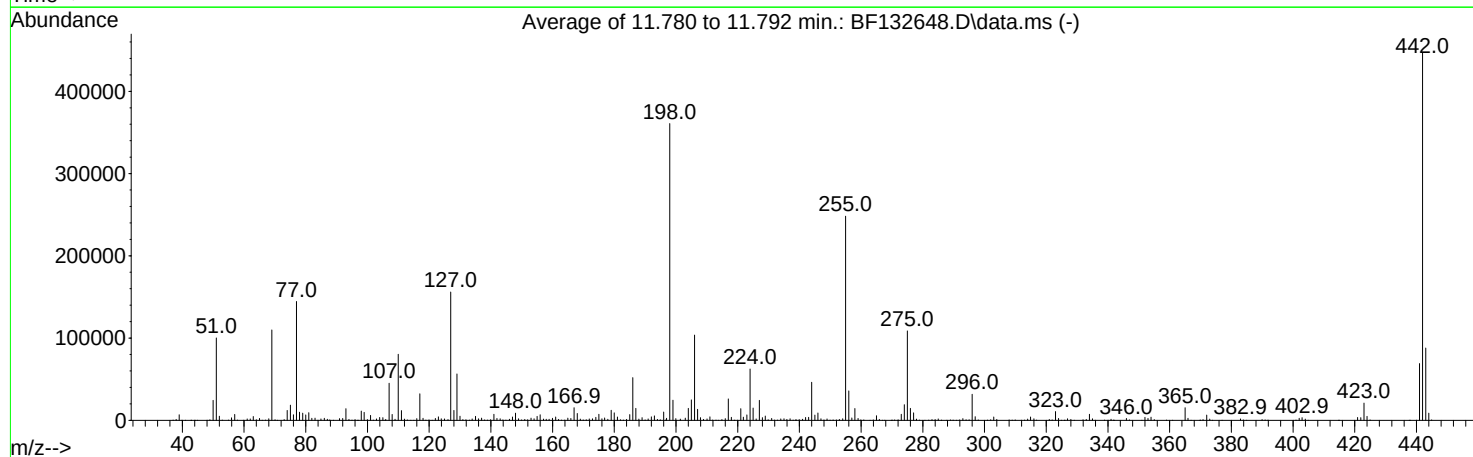


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132648.D
Acq On : 06 Mar 2023 14:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 23:17:30 2023

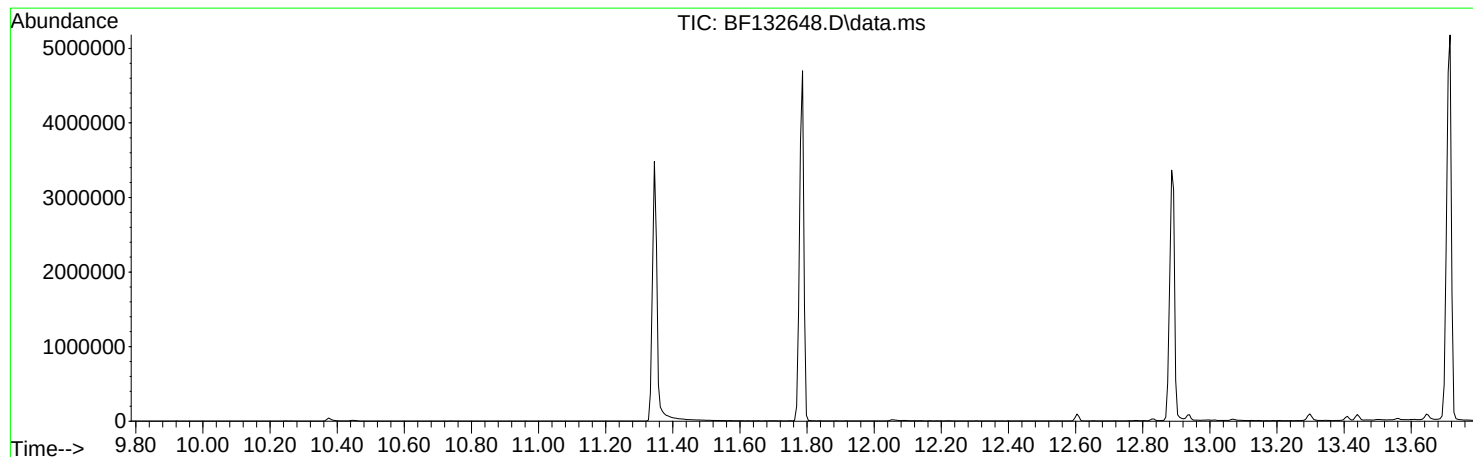




AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	100048	PASS
68	69	0.00	2	1.7	1909	PASS
69	198	0.00	100	30.5	109947	PASS
70	69	0.00	2	0.6	672	PASS
127	198	10	80	43.2	156043	PASS
197	198	0.00	2	0.7	2397	PASS
198	198	100	100	100.0	360917	PASS
199	198	5	9	6.8	24455	PASS
275	198	10	60	30.1	108651	PASS
365	198	1	100	4.2	15254	PASS
441	198	0.01	100	19.1	68971	PASS
442	442	50	100	100.0	447339	PASS
443	442	15	24	19.7	87955	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132648.D
Acq On : 06 Mar 2023 14:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 05:36:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

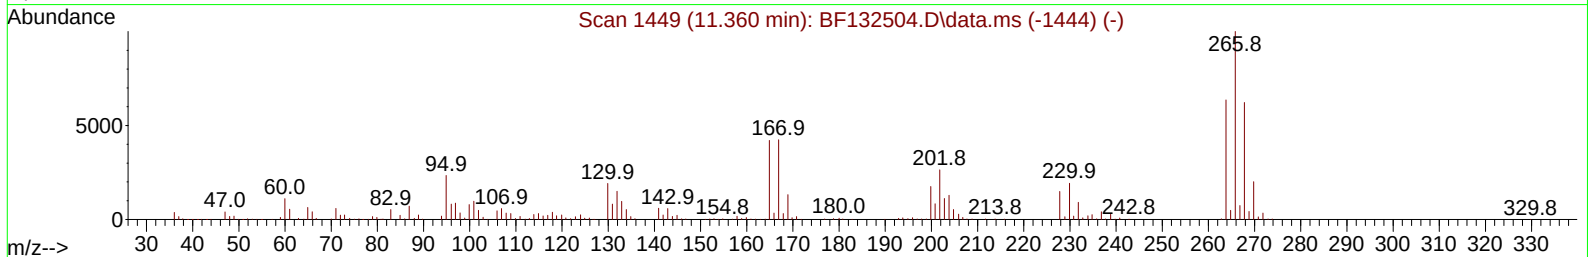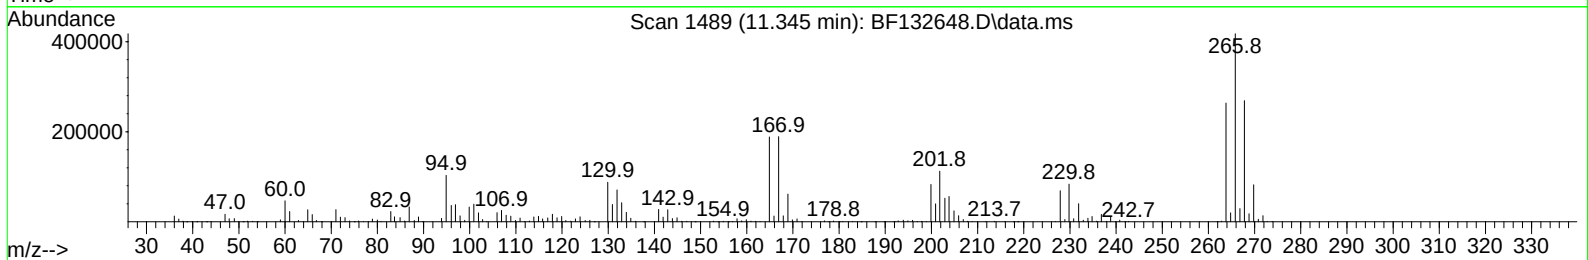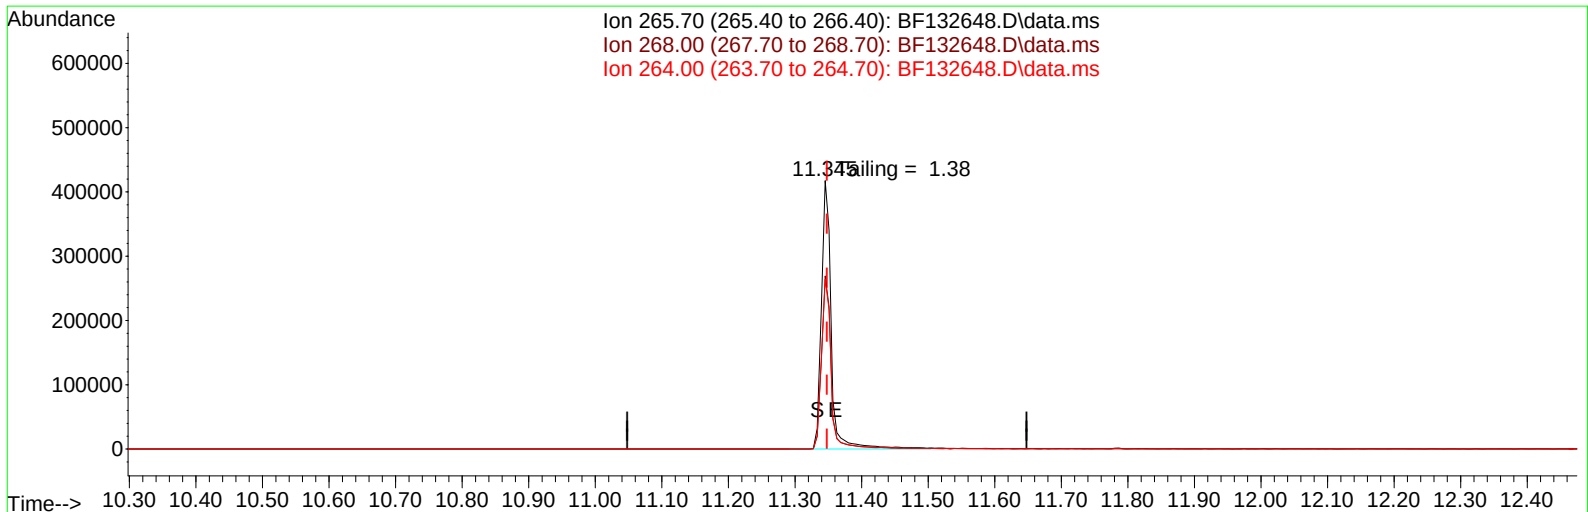

TIC: BF132648.D\data.ms

(70) Pentachlorophenol (C)

11.345min (-0.003) 279512.02 ng




response 427543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.46
264.00	63.60	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030623\
Data File : BF132648.D
Acq On : 06 Mar 2023 14:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 05:36:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

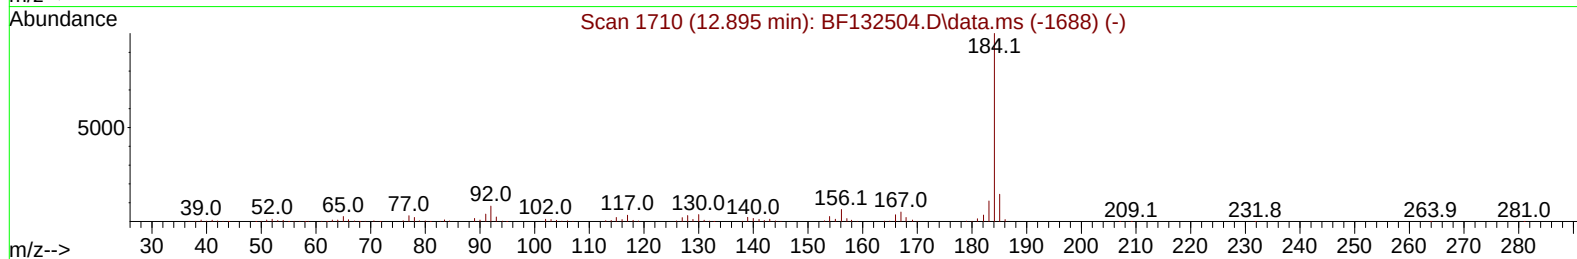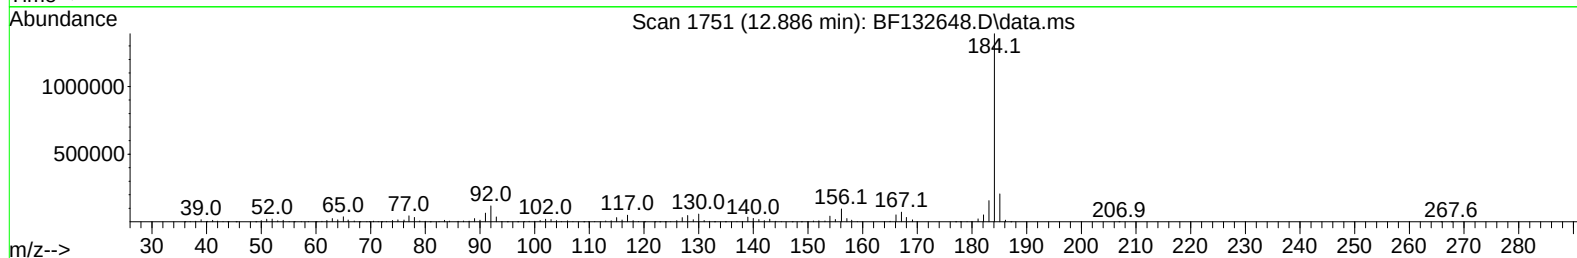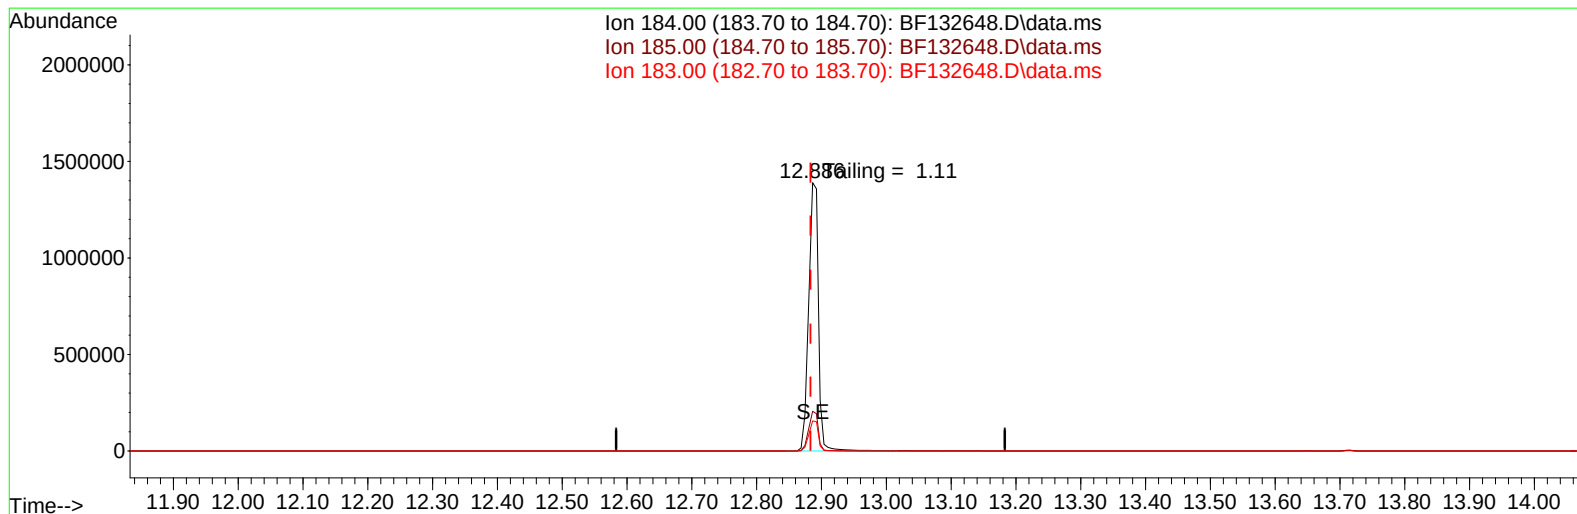

TIC: BF132648.D\data.ms

(77) Benzidine

12.886min (+ 0.003) 255996.11 ng

response 1464444

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.82
183.00	10.90	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/6/2023	BNA_F	<u>BF132648.D</u>
Compound Name	Response	Retention Time
DDT	1058444	13.716
DDD	24671	13.439
DDE	4492	13.069
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29163	1087607	2.68

Instrument :
BNA_F
ClientSampleId :
DFTPP