
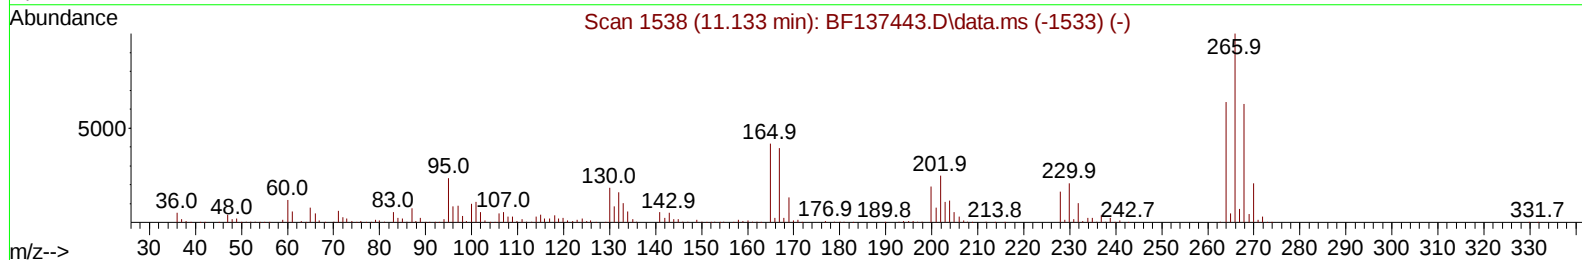
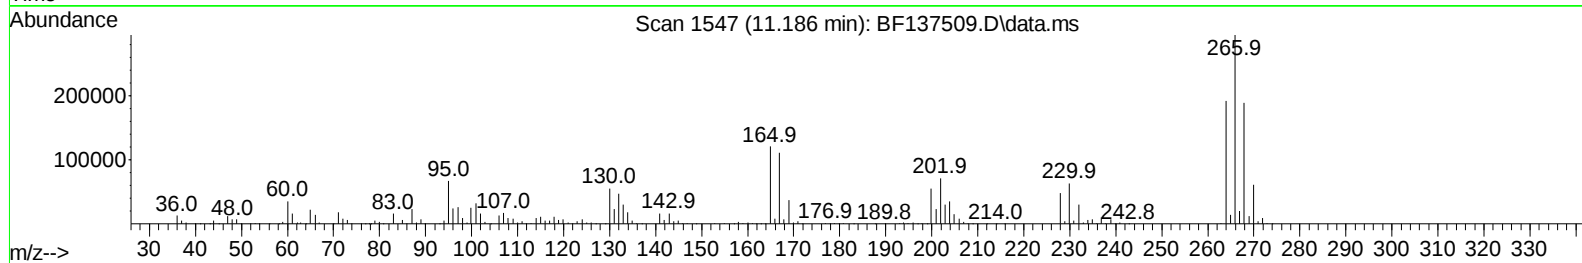


Quant Time: Mar 07 00:05:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 00:07:28 2024
Response via : Initial Calibration

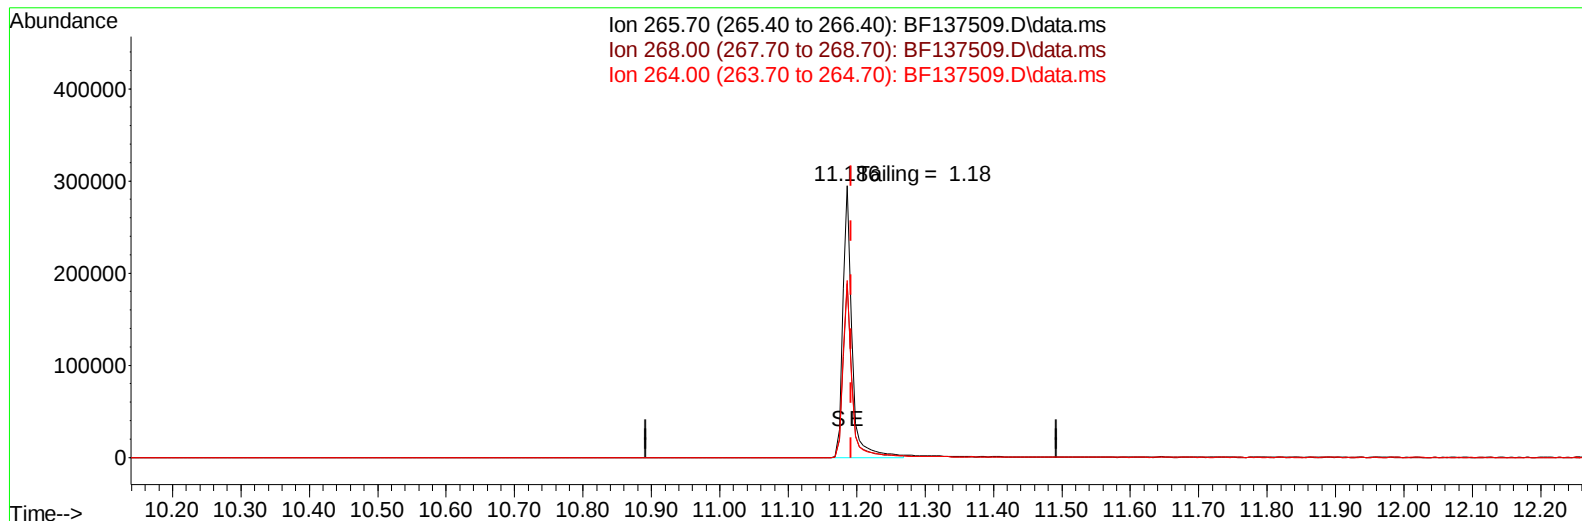

TIC: BF137509.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 300609.95 ng

response **269882**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.94
264.00	63.60	65.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
Data File : BF137509.D
Acq On : 06 Mar 2024 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 00:05:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 00:07:28 2024
Response via : Initial Calibration

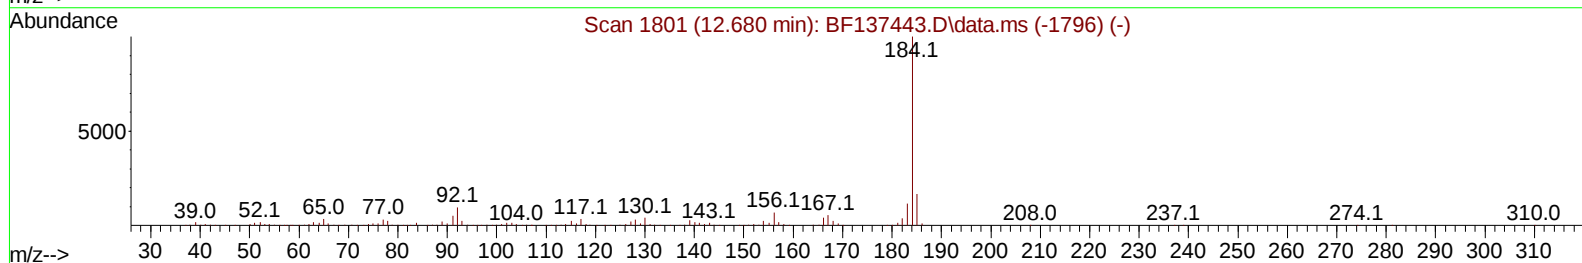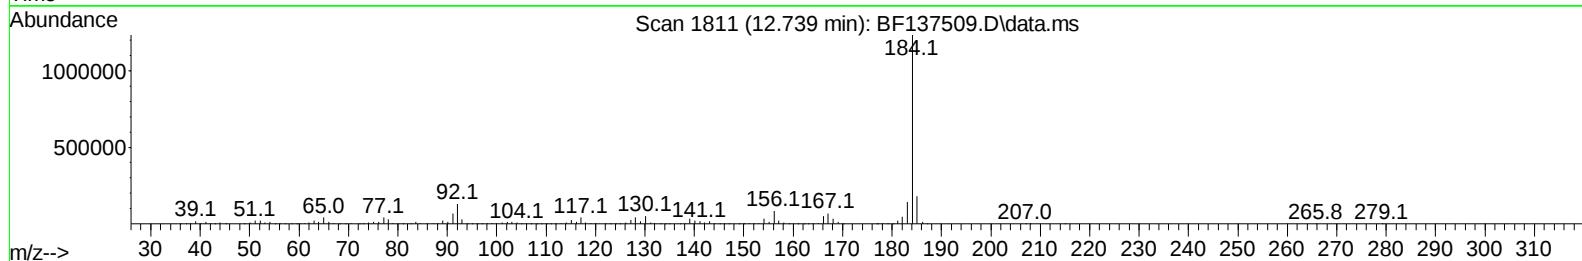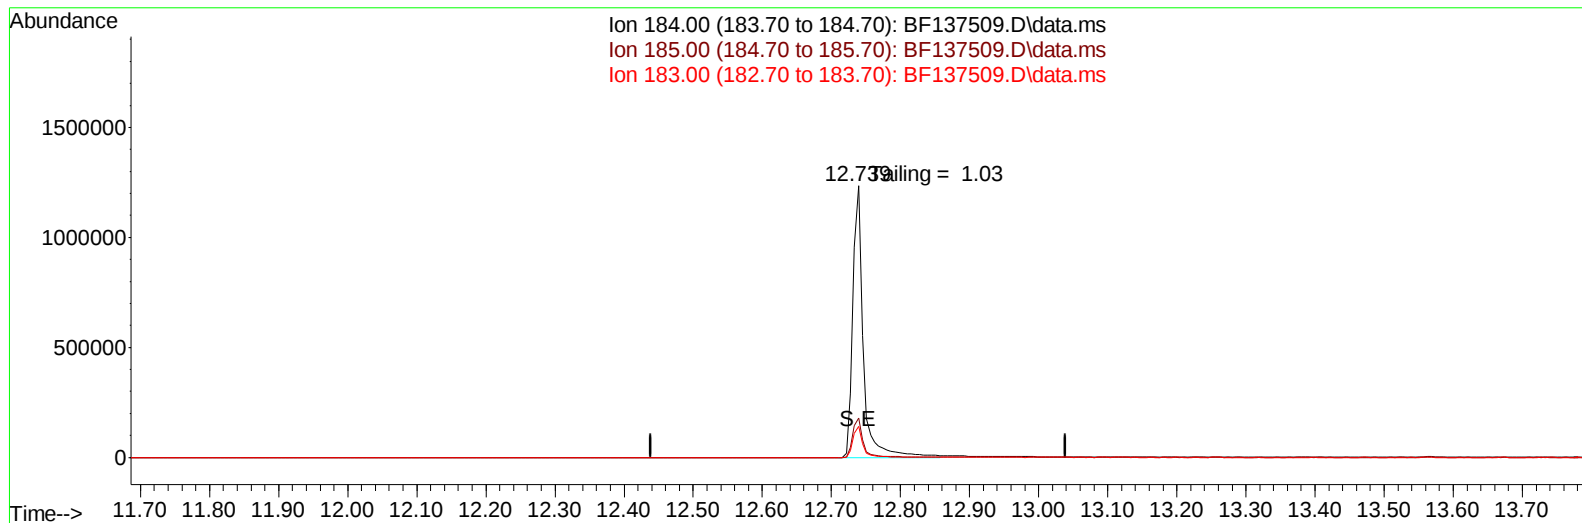

TIC: BF137509.D\data.ms

(77) Benzidine

12.739min (-12.739) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.50	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00