

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
 Data File : BF137511.D
 Acq On : 06 Mar 2024 11:23
 Operator : CG\JU
 Sample : PB159466BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB159466BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.146	517	520	533	rVB	90586	140777	1.42%	0.250%
2	5.516	578	583	586	rBV	6240563	7062910	71.06%	12.567%
3	6.498	744	750	753	rBV	6050374	7434855	74.81%	13.229%
4	6.851	807	810	828	rBV	1784539	1581262	15.91%	2.814%
5	7.416	900	906	909	rBV	4635172	4939449	49.70%	8.789%
6	8.128	1022	1027	1047	rBV	2192353	2233033	22.47%	3.973%
7	9.210	1205	1211	1214	rBV	8301942	8494225	85.47%	15.114%
8	9.886	1320	1326	1341	rBV	2921549	2642266	26.59%	4.701%
9	10.680	1456	1461	1464	rBV	4948971	4844756	48.75%	8.620%
10	11.380	1576	1580	1589	rBV	2961313	2754518	27.71%	4.901%
11	12.992	1848	1854	1857	rBV	8796003	9938817	100.00%	17.684%
12	14.039	2028	2032	2044	rBV	2052232	2075440	20.88%	3.693%
13	15.568	2286	2292	2299	rBV	1101970	1519279	15.29%	2.703%
14	15.633	2299	2303	2309	rVB	90686	139635	1.40%	0.248%
15	16.115	2380	2385	2394	rVB2	83821	150632	1.52%	0.268%
16	16.674	2475	2480	2489	rBV3	67397	147313	1.48%	0.262%
17	17.345	2590	2594	2602	rVB3	44810	101706	1.02%	0.181%




Sum of corrected areas: 56200873

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
Data File : BF137511.D
Acq On : 06 Mar 2024 11:23
Operator : CG\JU
Sample : PB159466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159466BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

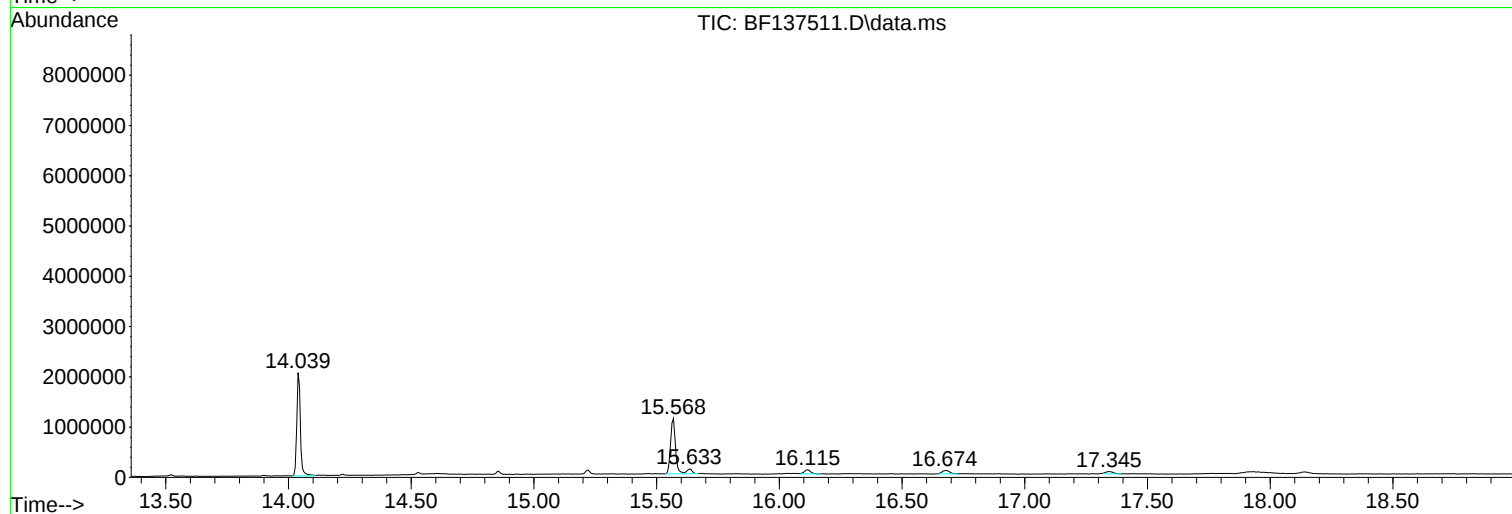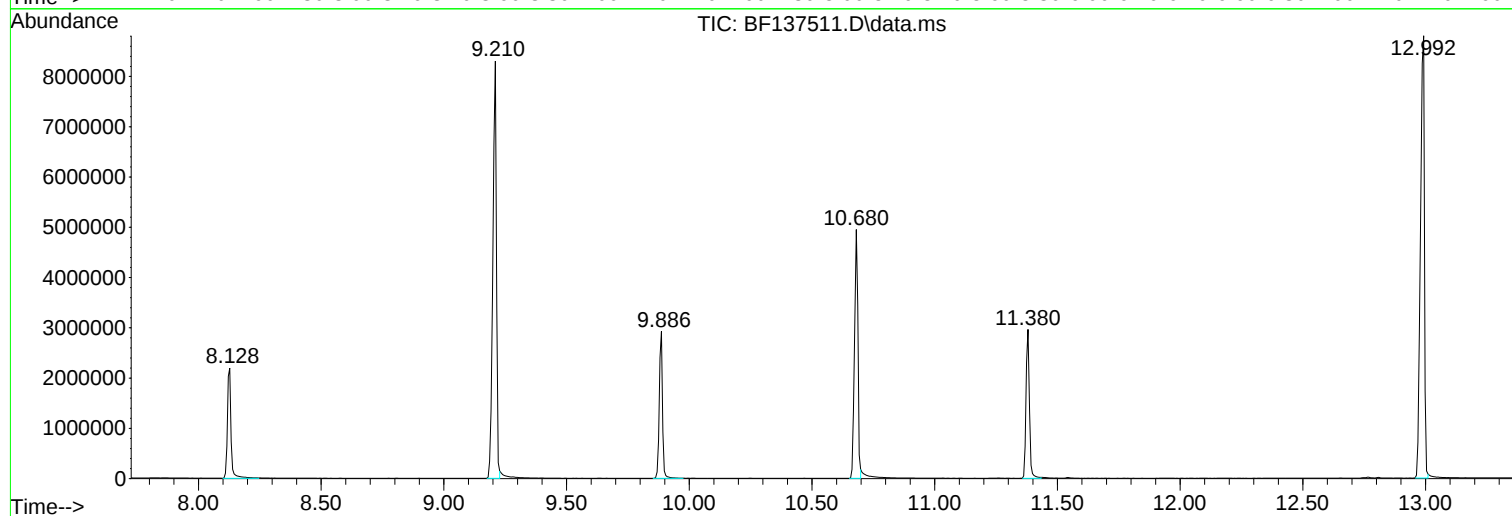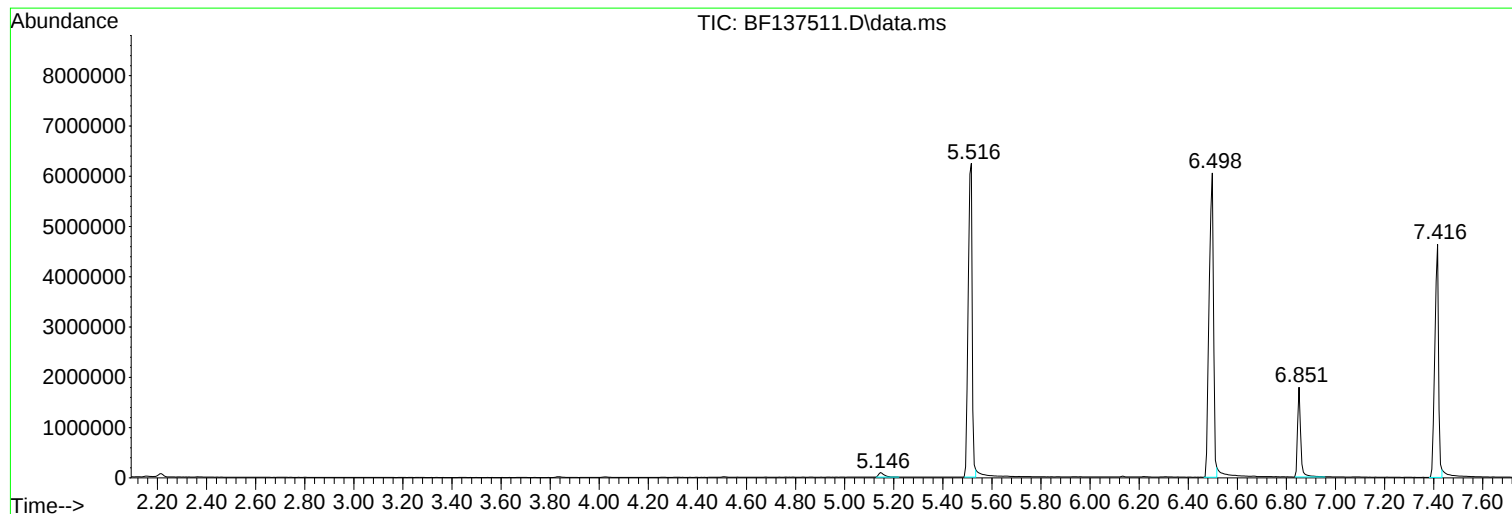

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
Data File : BF137511.D
Acq On : 06 Mar 2024 11:23
Operator : CG\JU
Sample : PB159466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159466BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
Data File : BF137511.D
Acq On : 06 Mar 2024 11:23
Operator : CG\JU
Sample : PB159466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159466BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------