


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
Data File : BF137509.D
Acq On : 06 Mar 2024 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 06 00:07:28 2024

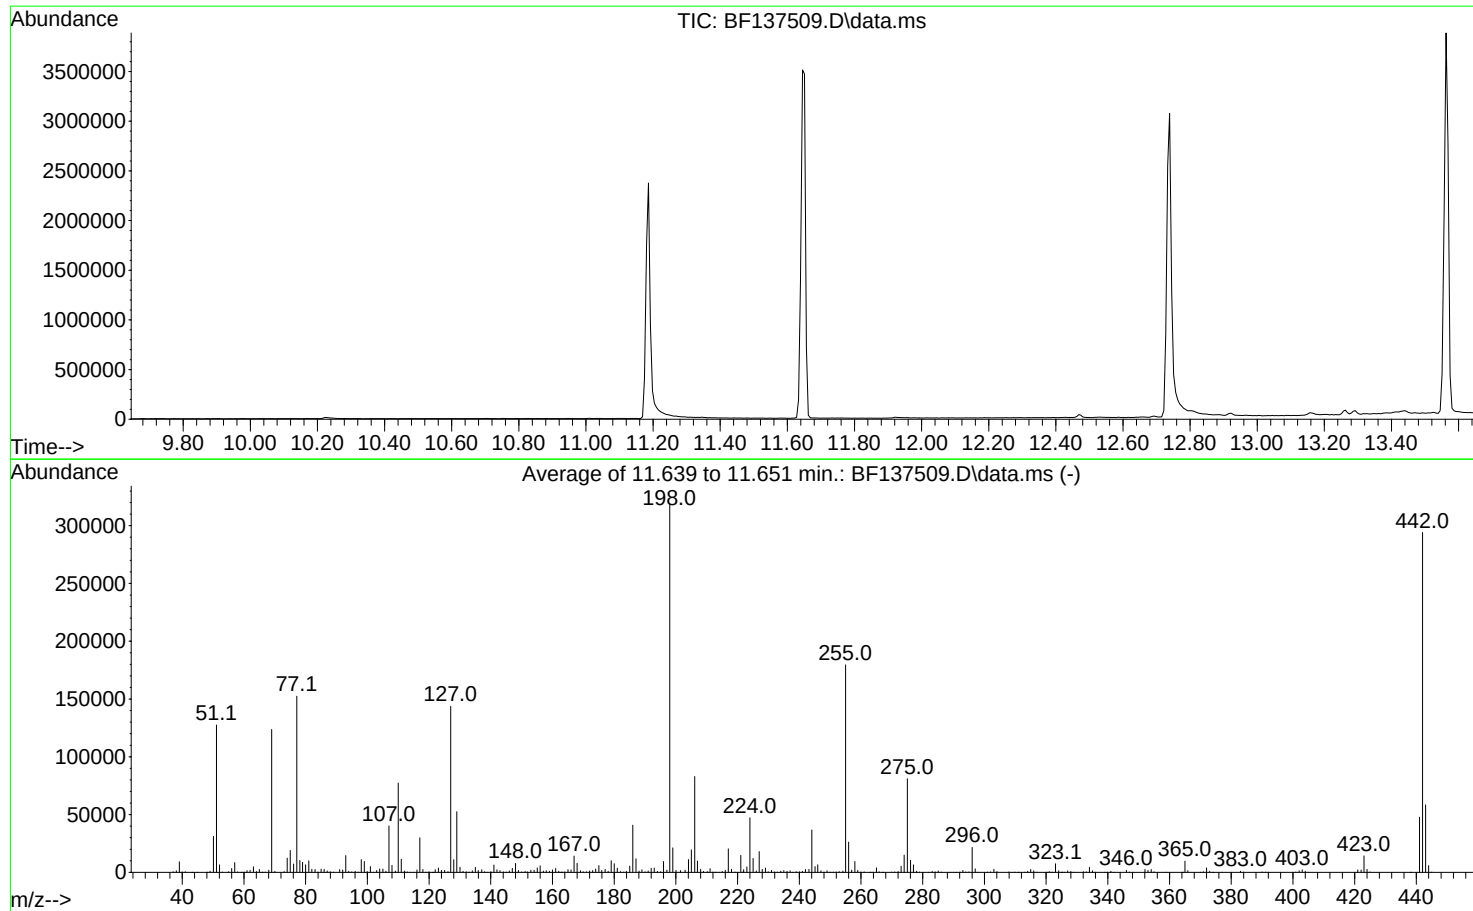




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	127587	PASS
68	69	0.00	2	1.6	2012	PASS
69	198	0.00	100	38.9	123669	PASS
70	69	0.00	2	0.6	792	PASS
127	198	10	80	45.1	143627	PASS
197	198	0.00	2	0.6	1954	PASS
198	198	100	100	100.0	318315	PASS
199	198	5	9	6.7	21235	PASS
275	198	10	60	25.5	81069	PASS
365	198	1	100	3.0	9685	PASS
441	198	0.01	100	15.0	47717	PASS
442	442	50	100	100.0	294096	PASS
443	442	15	24	19.9	58481	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
Data File : BF137509.D
Acq On : 06 Mar 2024 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 00:05:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 00:07:28 2024
Response via : Initial Calibration

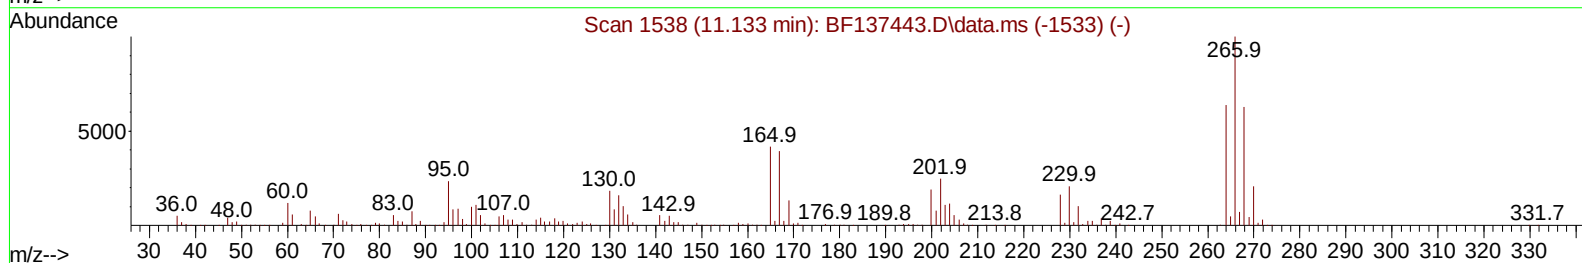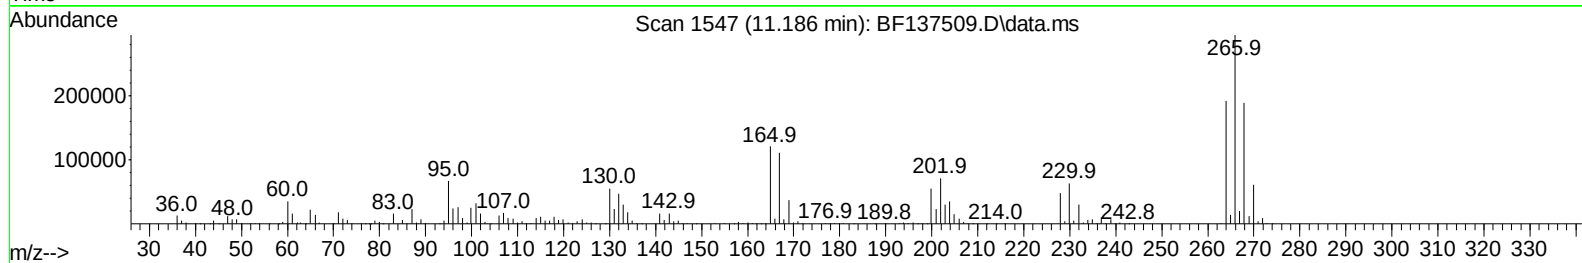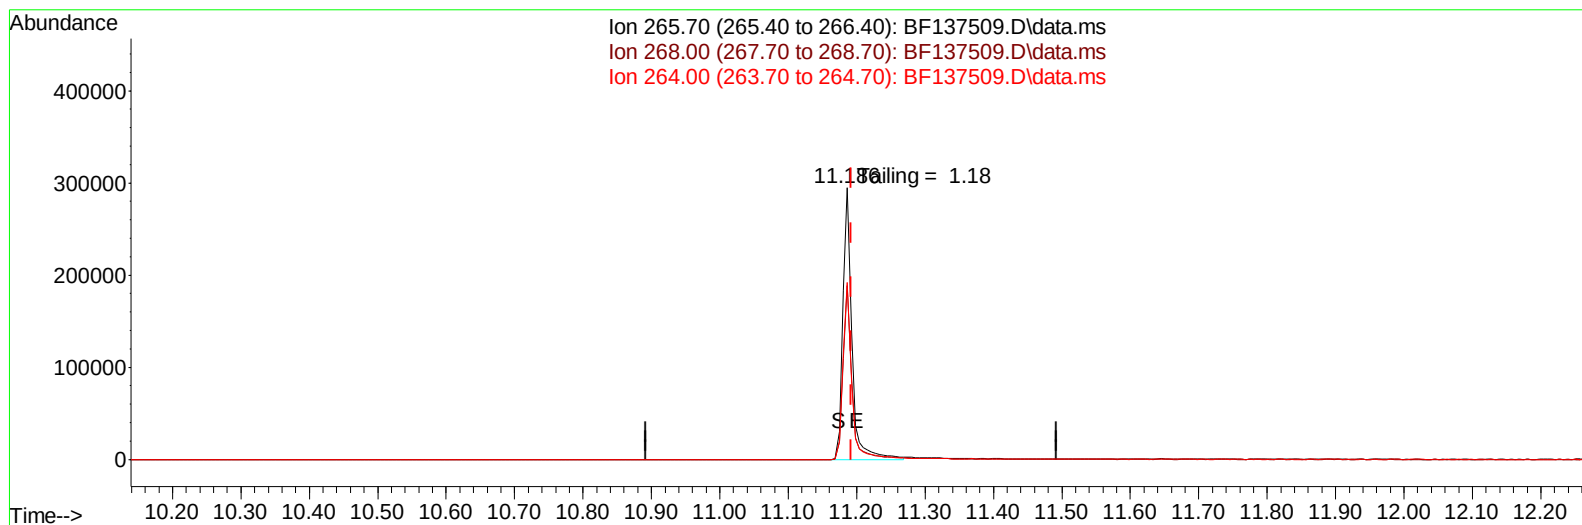

TIC: BF137509.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 300609.95 ng




response 269882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.94
264.00	63.60	65.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030624\
Data File : BF137509.D
Acq On : 06 Mar 2024 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 00:05:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 00:07:28 2024
Response via : Initial Calibration

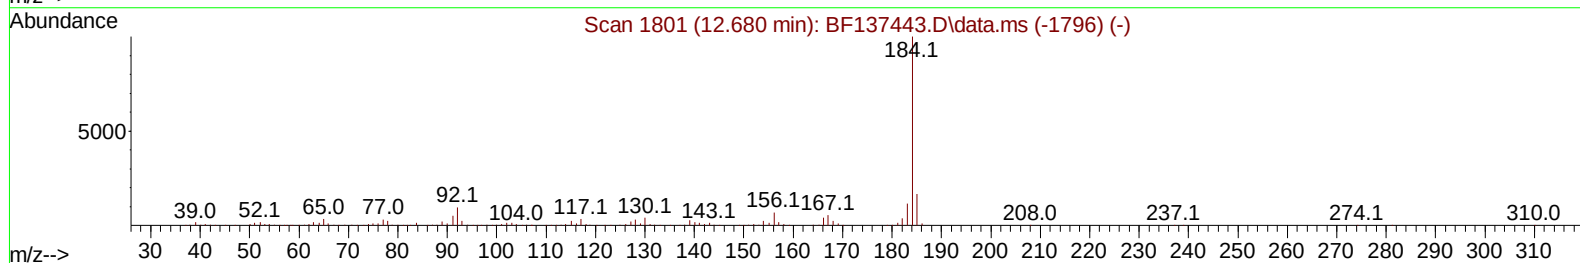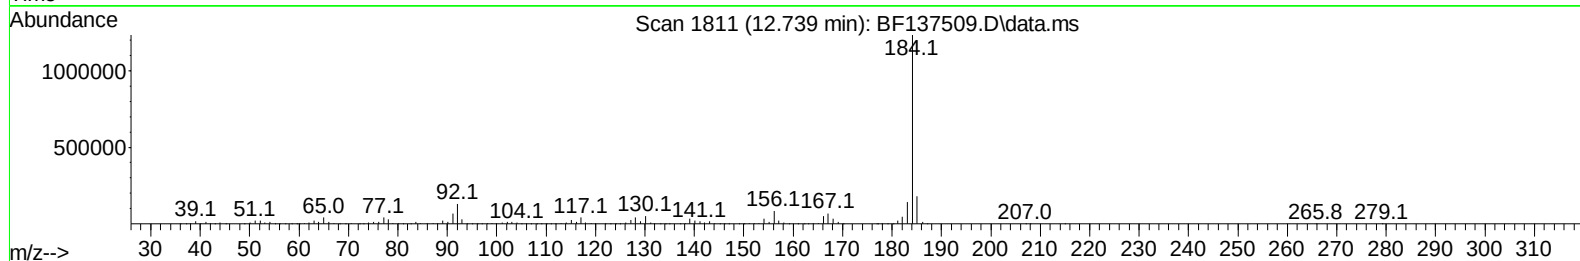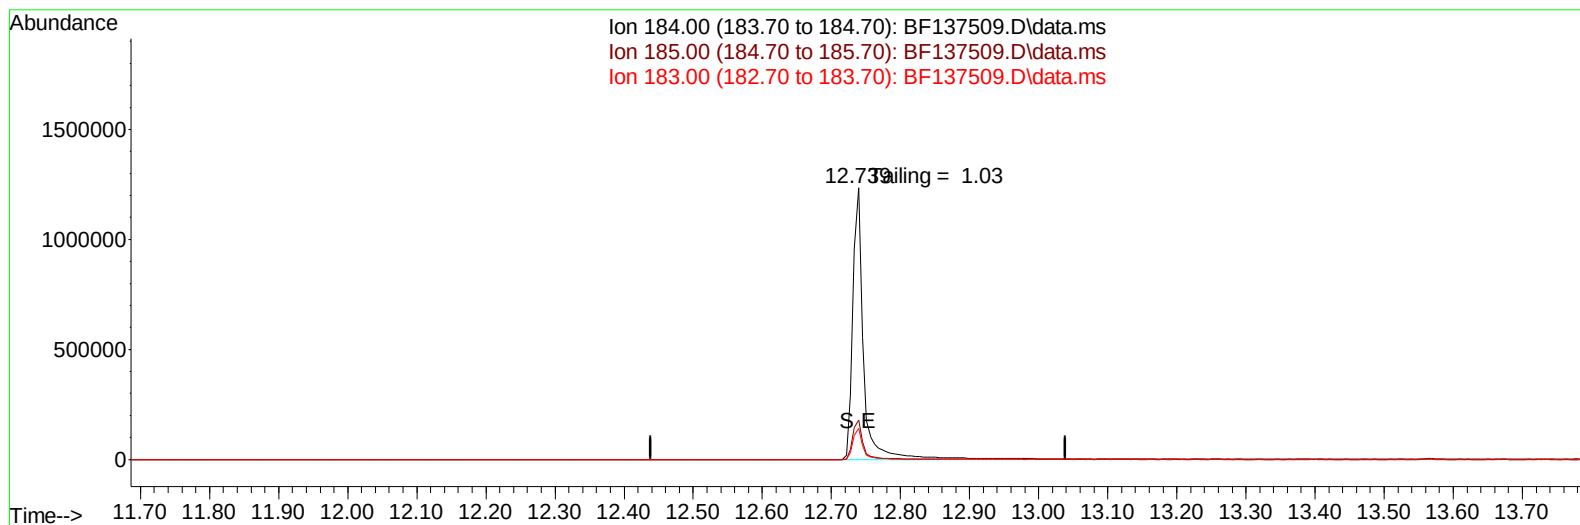

TIC: BF137509.D\data.ms

(77) Benzidine

12.739min (-12.739) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.50	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/6/2024	BNA_F	<u>BF137509.D</u>
Compound Name	Response	Retention Time
DDT	651095	13.563
DDD	14848	13.263
DDE	3030	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17878	668973	2.67

Instrument :
BNA_F
ClientSampleId :
DFTPP