
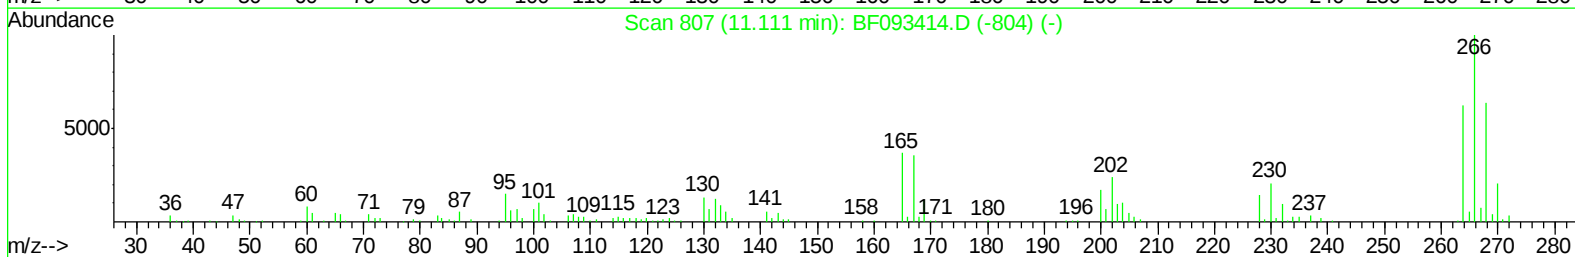
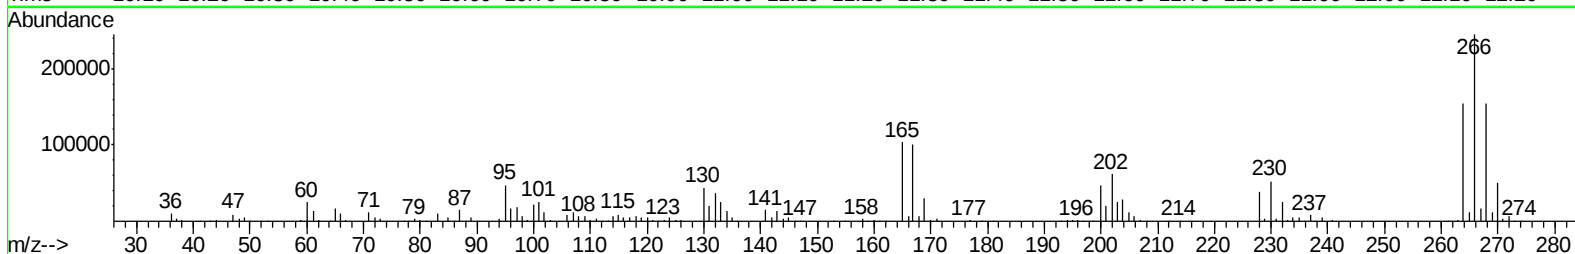


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF030717\  
Data File : BF093410.D  
Acq On : 7 Mar 2017 10:33  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 18:16:40 2017  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF030717.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 07 15:55:22 2017  
Response via : Initial Calibration

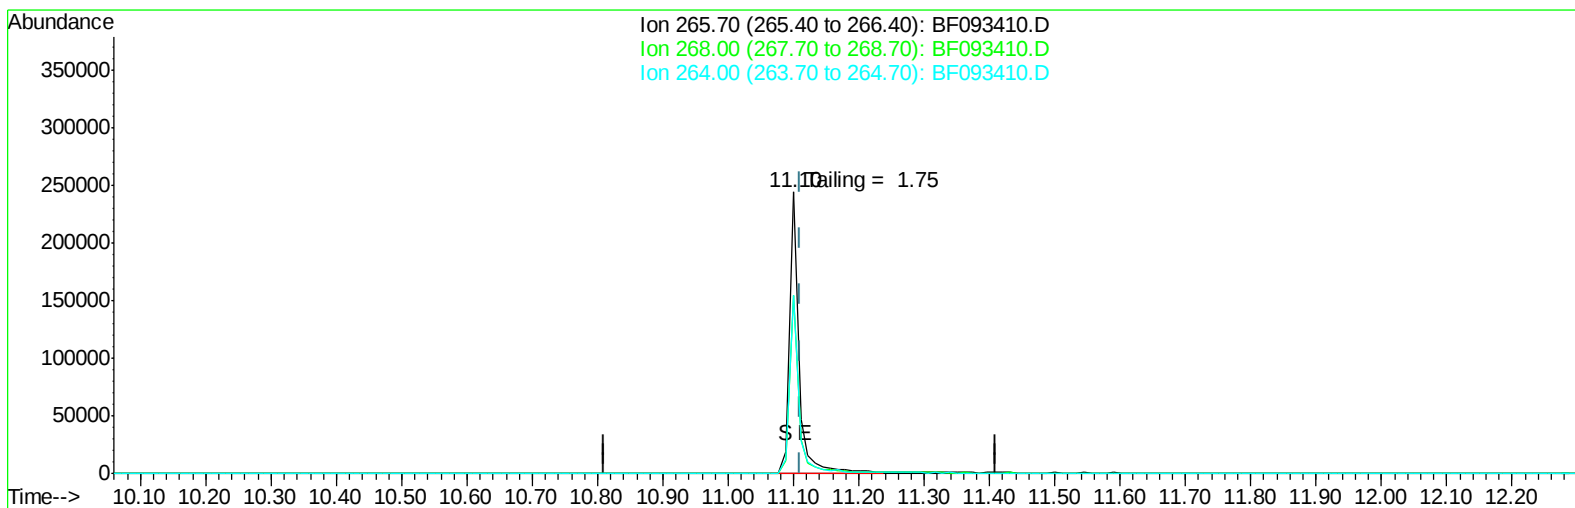

TIC: BF093410.D

(69) Pentachlorophenol (C)




11.099min (-0.011) 0.00ng

response 252769

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.60 | 63.38 |
| 264.00 | 62.90 | 63.27 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF030717\  
Data File : BF093410.D  
Acq On : 7 Mar 2017 10:33  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 18:16:40 2017  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF030717.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 07 15:55:22 2017  
Response via : Initial Calibration

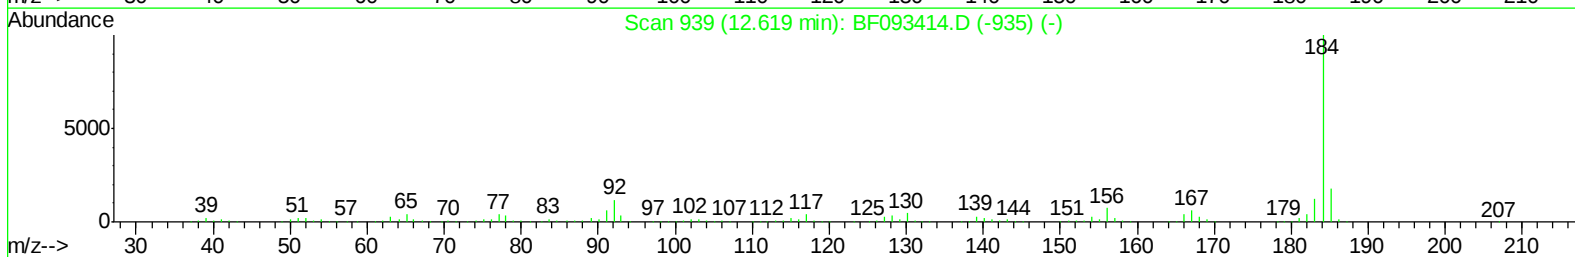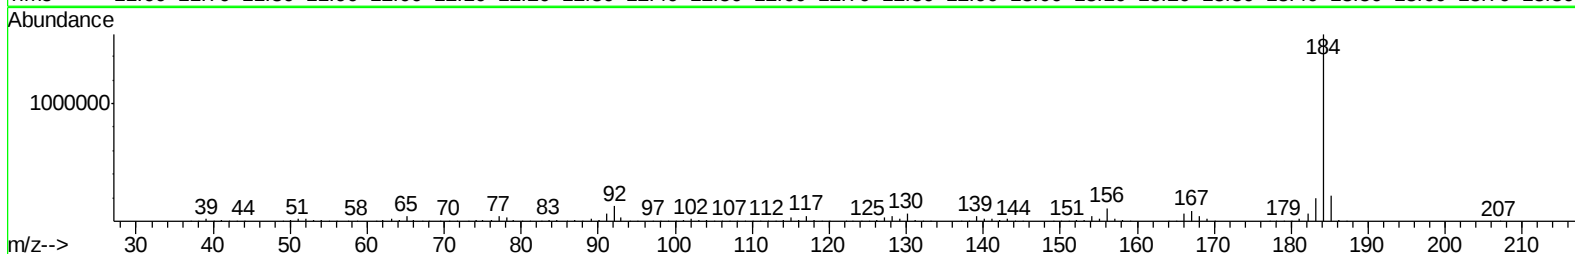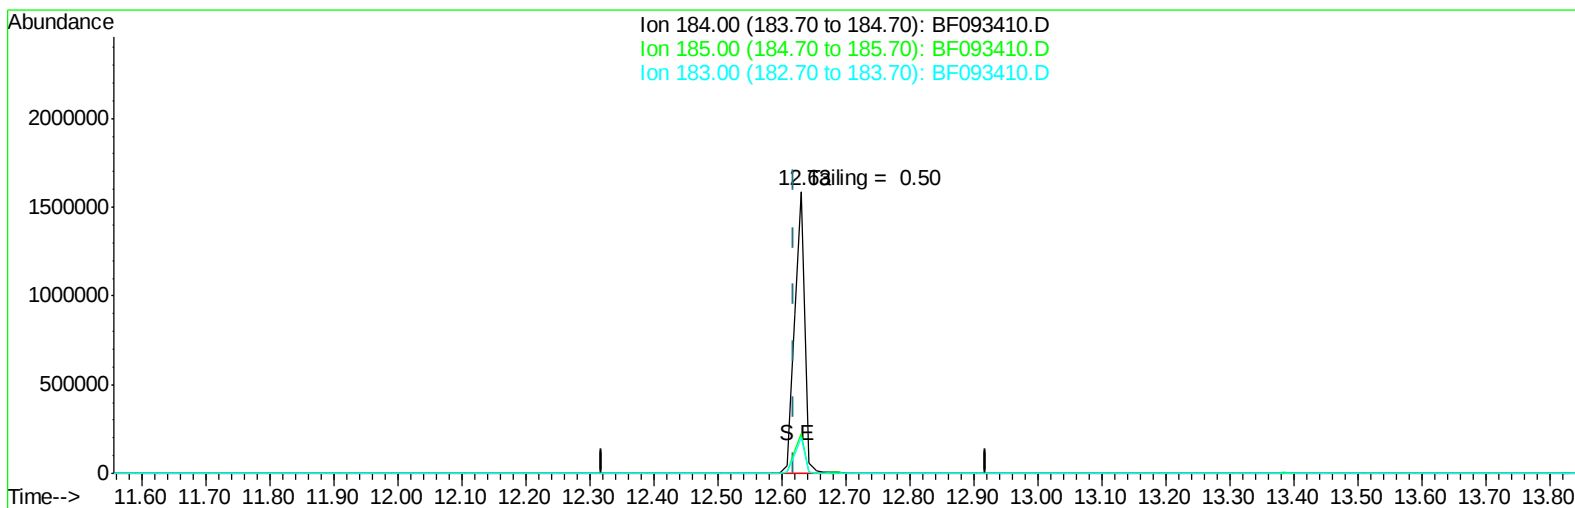

TIC: BF093410.D

(76) Benzidine

12.631min (+0.011) 0.00ng

response 1813647

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.70 | 14.02 |
| 183.00 | 11.50 | 12.67 |
| 0.00   | 0.00  | 0.00  |