
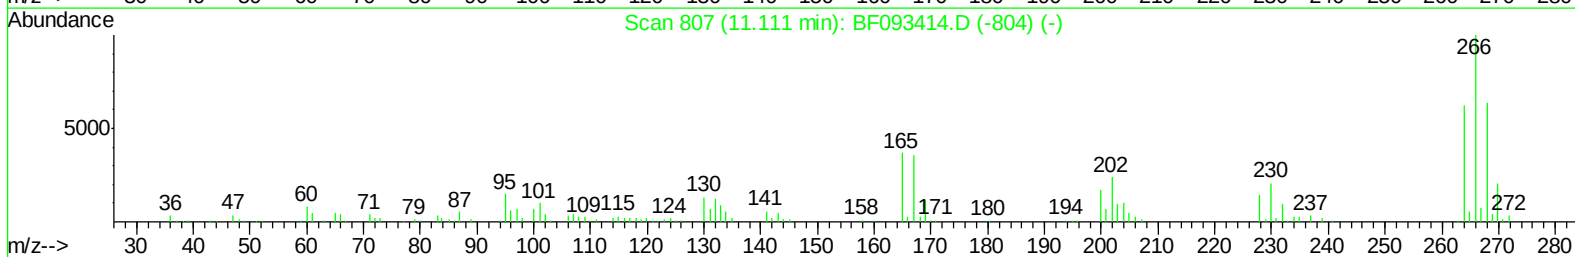
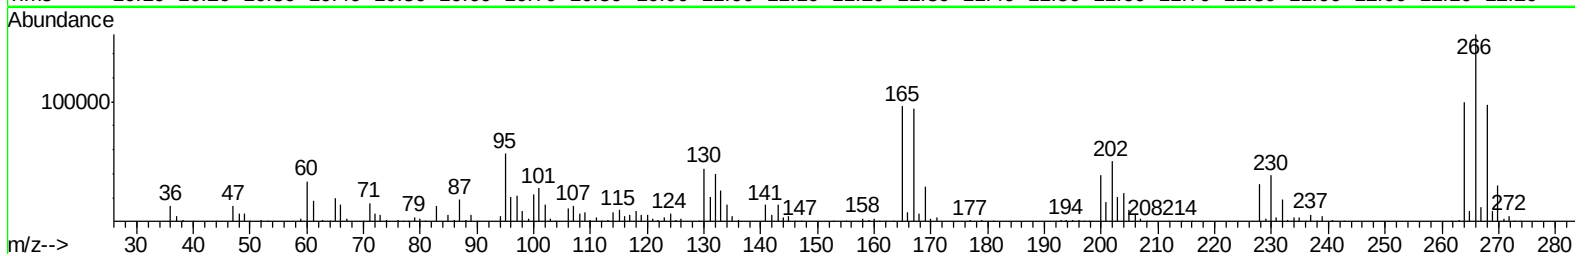


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030717\
Data File : BF093419.D
Acq On : 7 Mar 2017 15:08
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 03:53:39 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

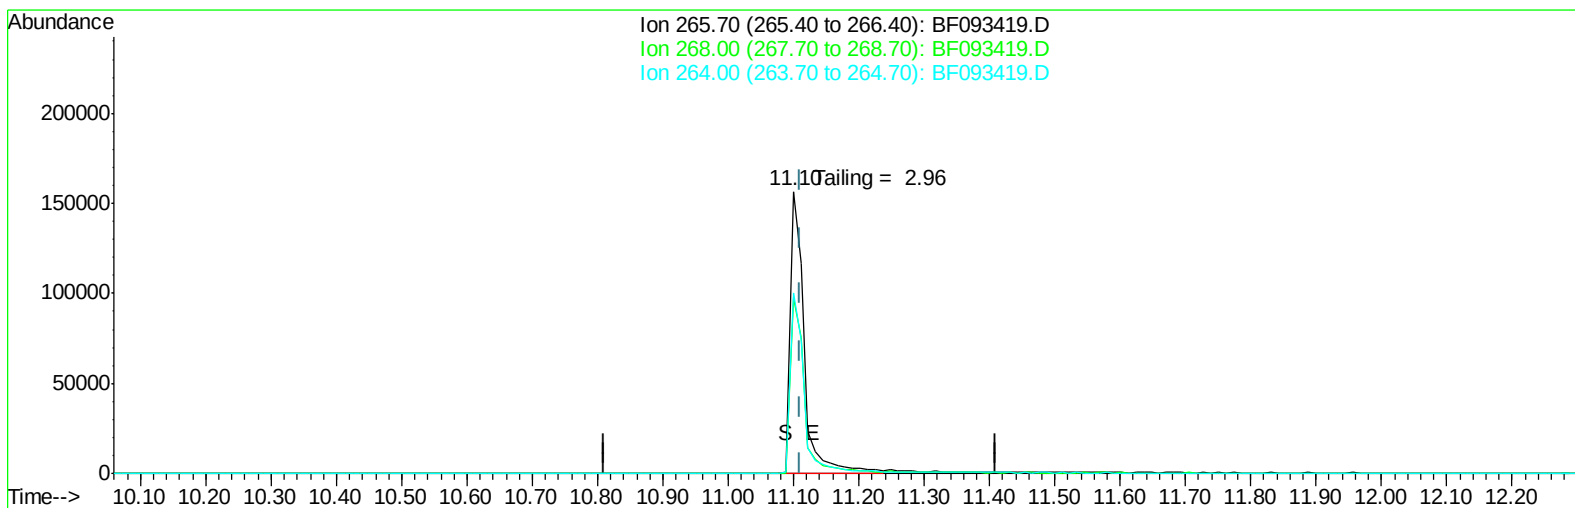

TIC: BF093419.D

(69) Pentachlorophenol (C)




11.099min (-0.011) 291290.18ng

response 238645

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.40
264.00	62.90	63.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF030717\
Data File : BF093419.D
Acq On : 7 Mar 2017 15:08
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 03:53:39 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

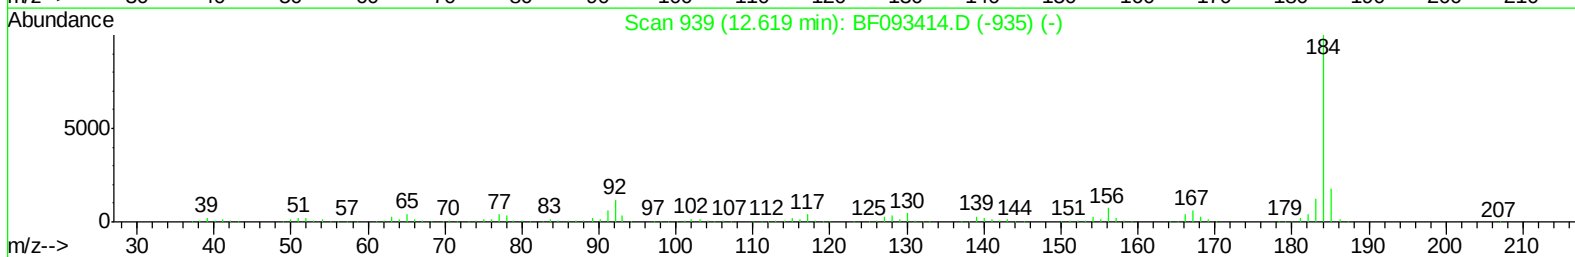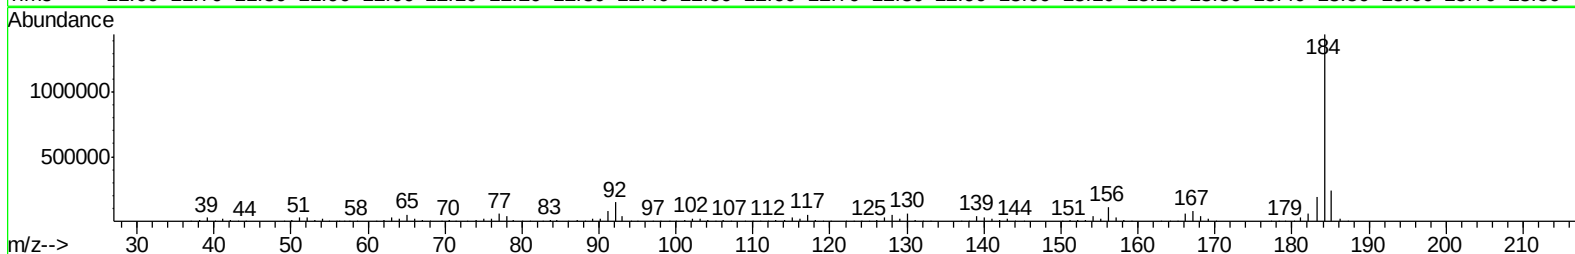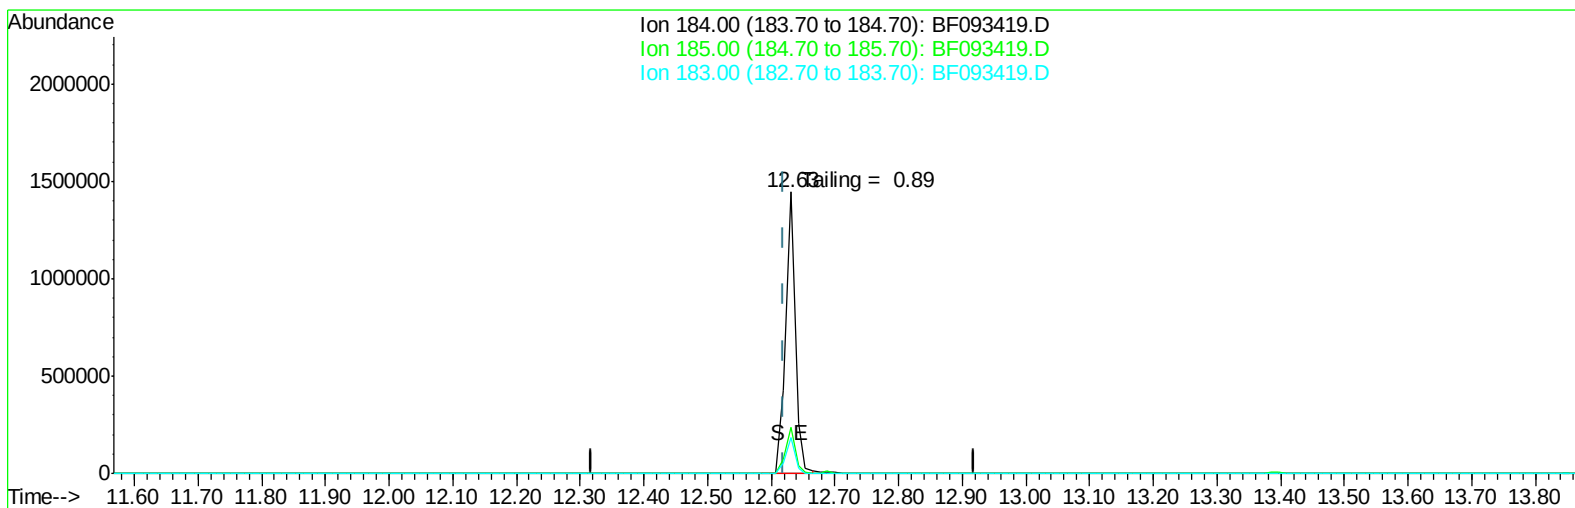

TIC: BF093419.D

(76) Benzidine

12.631min (+0.011) 0.00ng

response 1513195

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	16.60
183.00	11.50	12.84
0.00	0.00	0.00