


Data Path : Z:\HPCHEM1\BNA F\Data\BF030717\
 Data File : BF093419.D
 Acq On : 7 Mar 2017 15:08
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 07 15:55:22 2017

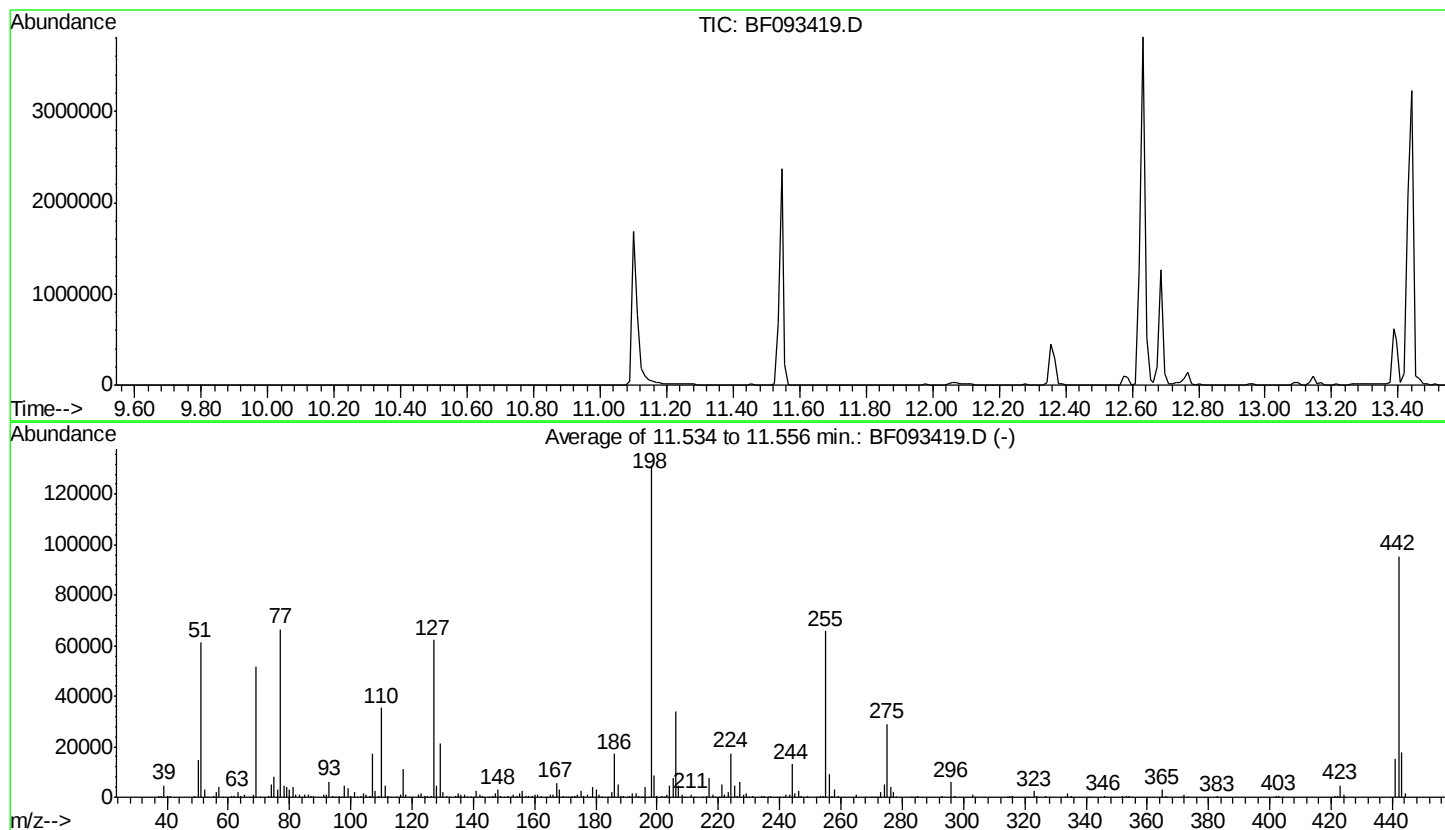

AutoFind: Scans 844, 845, 846; Background Corrected with Scan 840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	61300	PASS
68	69	0.00	2	1.8	929	PASS
69	198	0.00	100	39.5	51821	PASS
70	69	0.00	2	0.3	154	PASS
127	198	10	80	47.3	62159	PASS
197	198	0.00	2	0.2	218	PASS
198	198	100	100	100.0	131343	PASS
199	198	5	9	6.8	8884	PASS
275	198	10	60	22.1	29008	PASS
365	198	1	100	2.2	2824	PASS
441	442	0.01	24	15.8	15047	PASS
442	198	50	100	72.6	95397	PASS
443	442	15	24	18.4	17524	PASS