
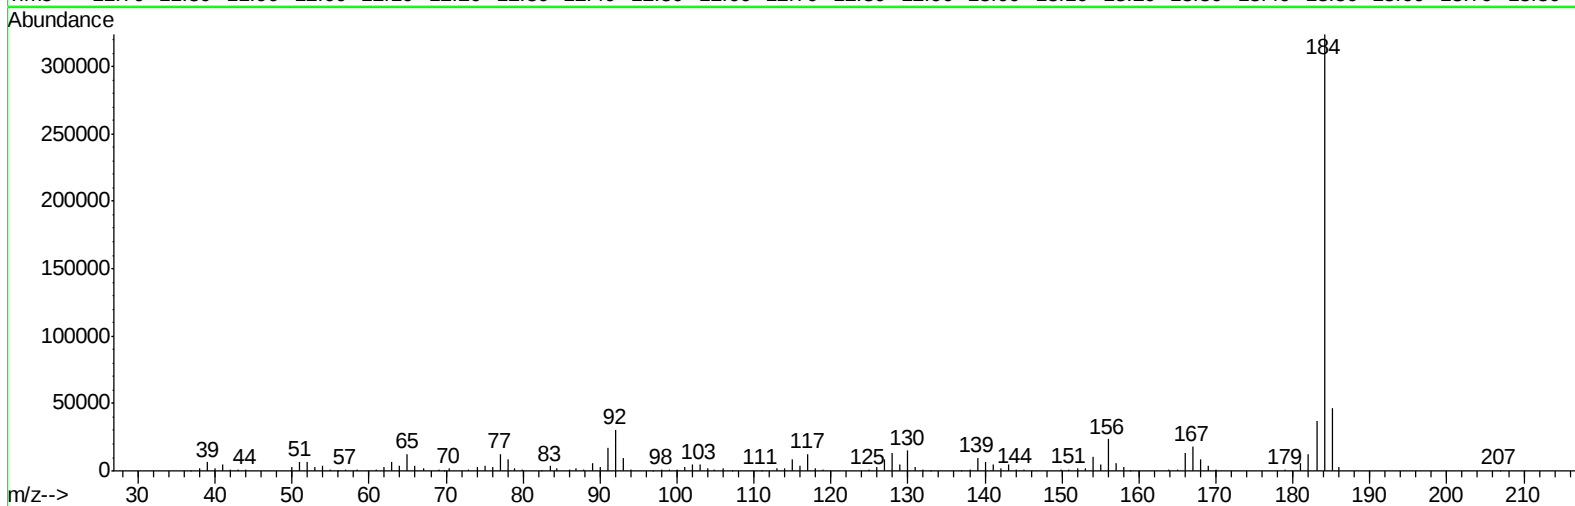


Data Path : Z:\HPCHEM1\BNA F\DATA\BF030718\
Data File : BF103490.D
Acq On : 7 Mar 2018 10:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 08:29:46 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 07 11:40:36 2018
Response via : Initial Calibration

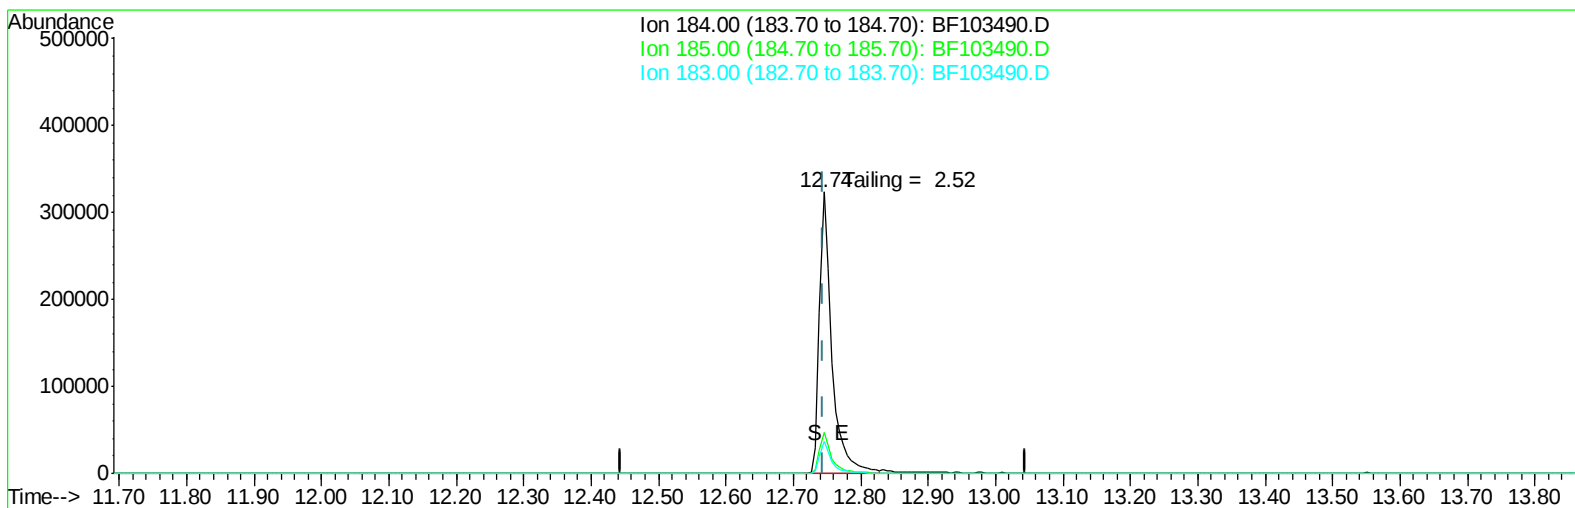

TIC: BF103490.D

(76) Benzidine



12.745min (-0.000) 14738.73ng m

response 400034

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.43
183.00	11.60	11.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030718\
Data File : BF103490.D
Acq On : 7 Mar 2018 10:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 08:29:46 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 07 11:40:36 2018
Response via : Initial Calibration

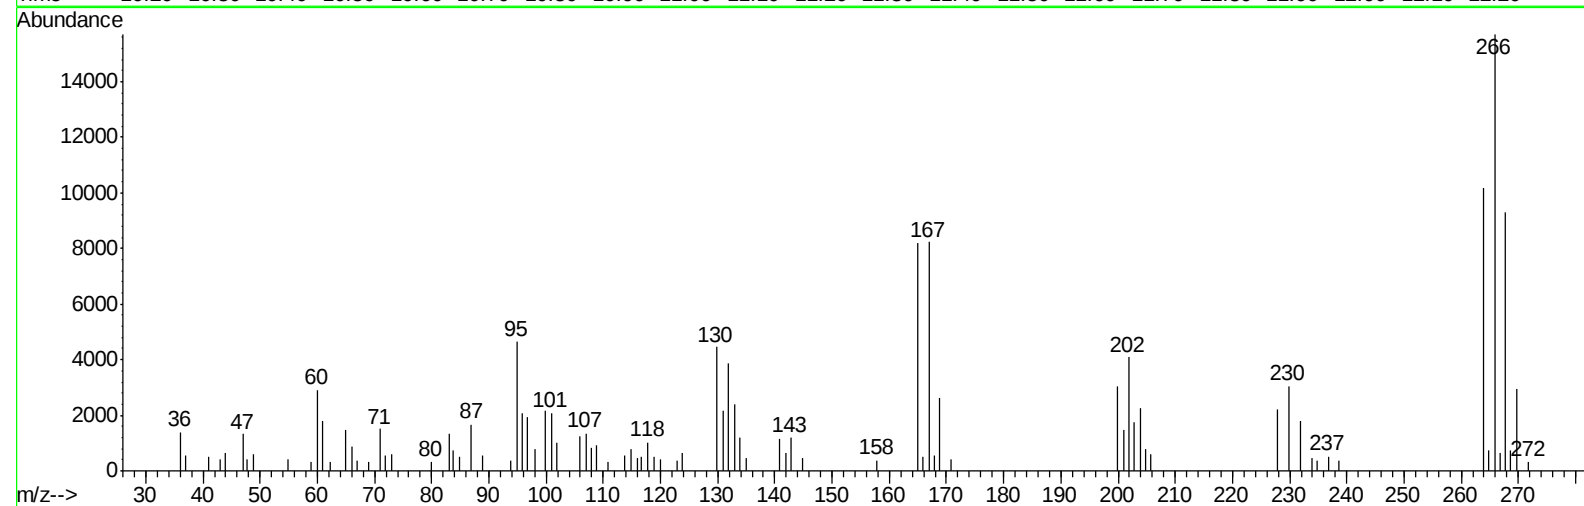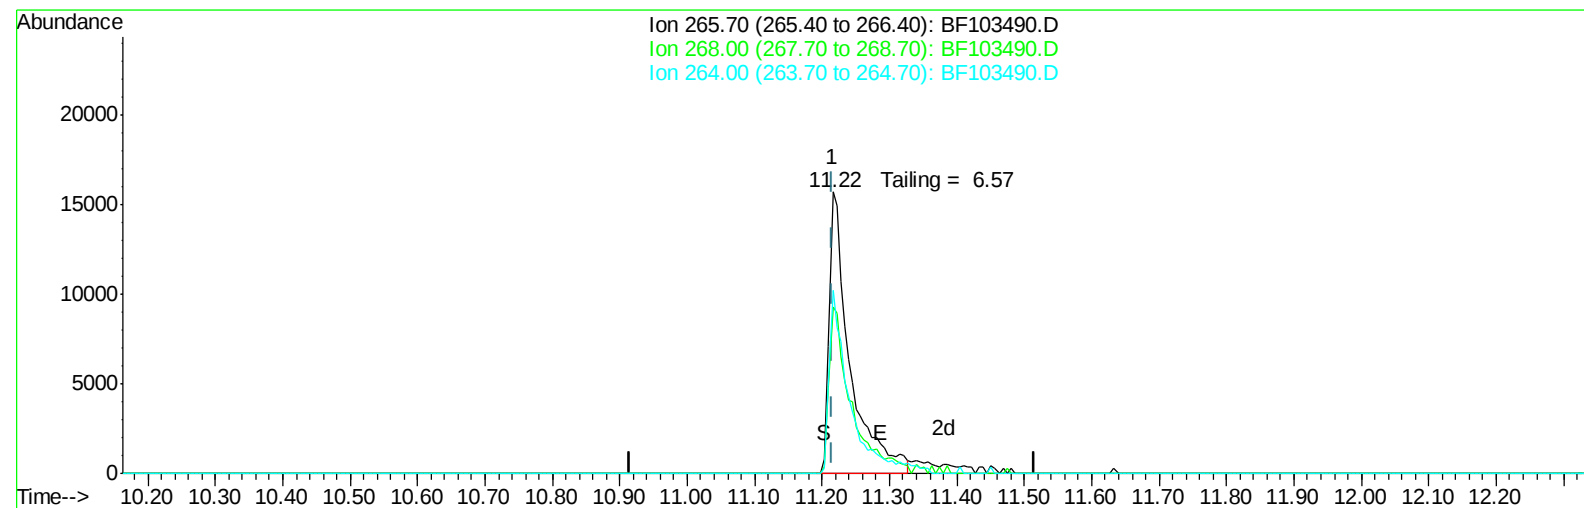

TIC: BF103490.D

(69) Pentachlorophenol (C)

11.216min (-0.000) 6645.93ng

response 33281

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.75
264.00	61.90	64.85
0.00	0.00	0.00