


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF030718\  
 Data File : BF103490.D  
 Acq On : 7 Mar 2018 10:23  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF022218.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 07 11:40:36 2018

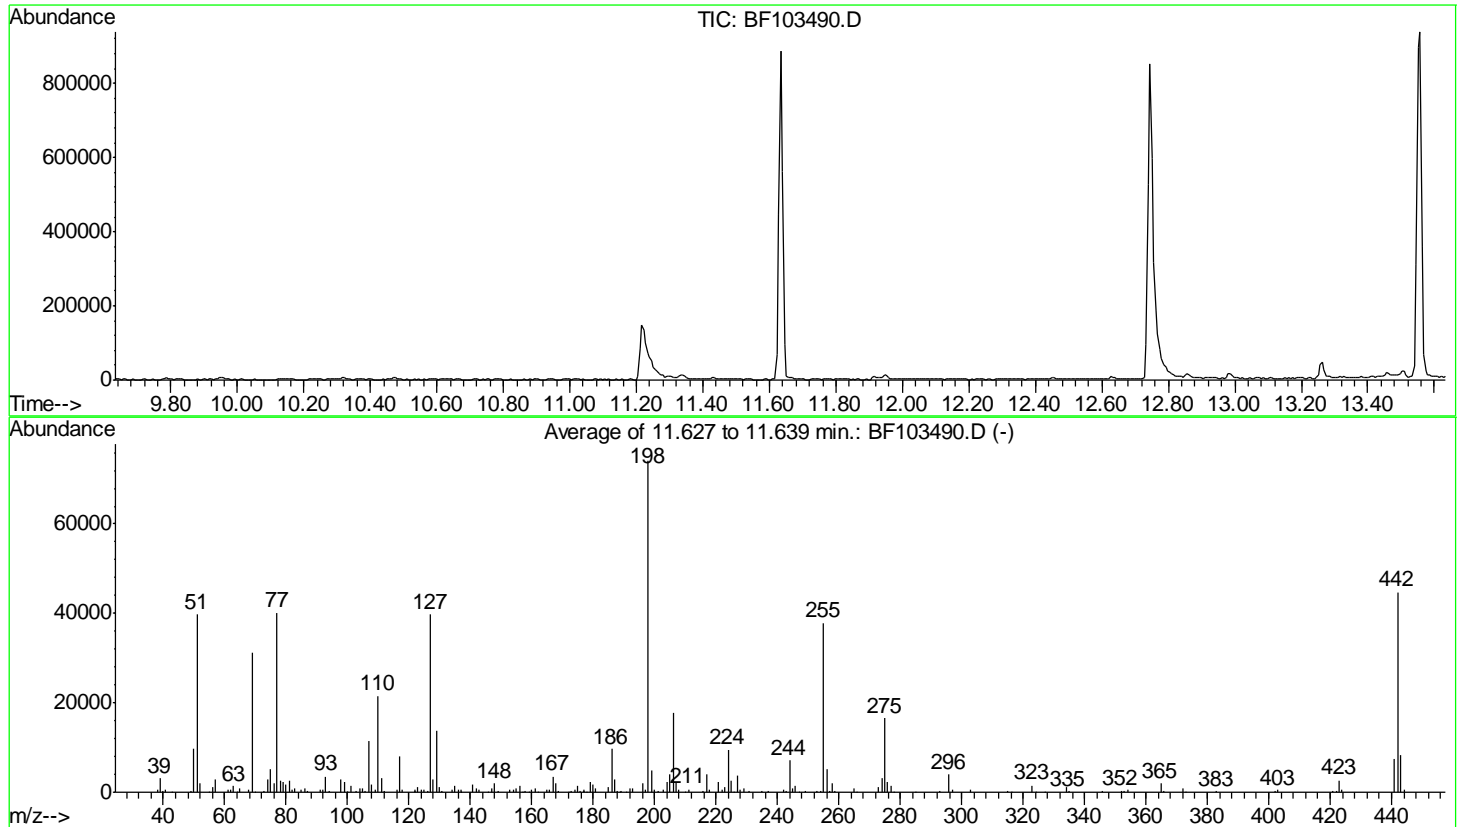

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	39722	PASS
68	69	0.00	2	1.8	560	PASS
69	198	0.00	100	42.1	31234	PASS
70	69	0.00	2	0.4	118	PASS
127	198	10	80	53.7	39800	PASS
197	198	0.00	2	0.9	657	PASS
198	198	100	100	100.0	74178	PASS
199	198	5	9	6.7	4984	PASS
275	198	10	60	22.4	16581	PASS
365	198	1	100	2.7	1997	PASS
441	443	0.01	100	89.4	7503	PASS
442	198	50	100	60.4	44823	PASS
443	442	15	24	18.7	8388	PASS