

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF030719\
 Data File : BF112919.D
 Acq On : 7 Mar 2019 14:18
 Operator : JU/SJ
 Sample : K1760-15
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 Z2-11

Quant Time: Mar 08 00:43:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 01 15:40:43 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	160048	20.00	ng	-0.01
21) Naphthalene-d8	8.01	136	634168	20.00	ng	-0.01
39) Acenaphthene-d10	9.76	164	314268	20.00	ng	0.00
64) Phenanthrene-d10	11.24	188	665096	20.00	ng	0.00
76) Chrysene-d12	13.86	240	650659	20.00	ng	-0.01
87) Perylene-d12	15.27	264	622057	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	722763	70.25	ng	-0.01
7) Phenol-d6	6.36	99	964662	74.64	ng	0.00
23) Nitrobenzene-d5	7.29	82	565489	53.36	ng	-0.02
42) 2,4,6-Tribromophenol	10.55	330	323959	97.10	ng	-0.01
45) 2-Fluorobiphenyl	9.09	172	1123471	53.73	ng	-0.01
79) Terphenyl-d14	12.82	244	1314390	39.16	ng	-0.01
Target Compounds						
50) Dimethylphthalate	9.48	163	95331	4.114	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF030719\
Data File : BF112919.D
Acq On : 7 Mar 2019 14:18
Operator : JU/SJ
Sample : K1760-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z2-11

Quant Time: Mar 08 00:43:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 15:40:43 2019
Response via : Initial Calibration

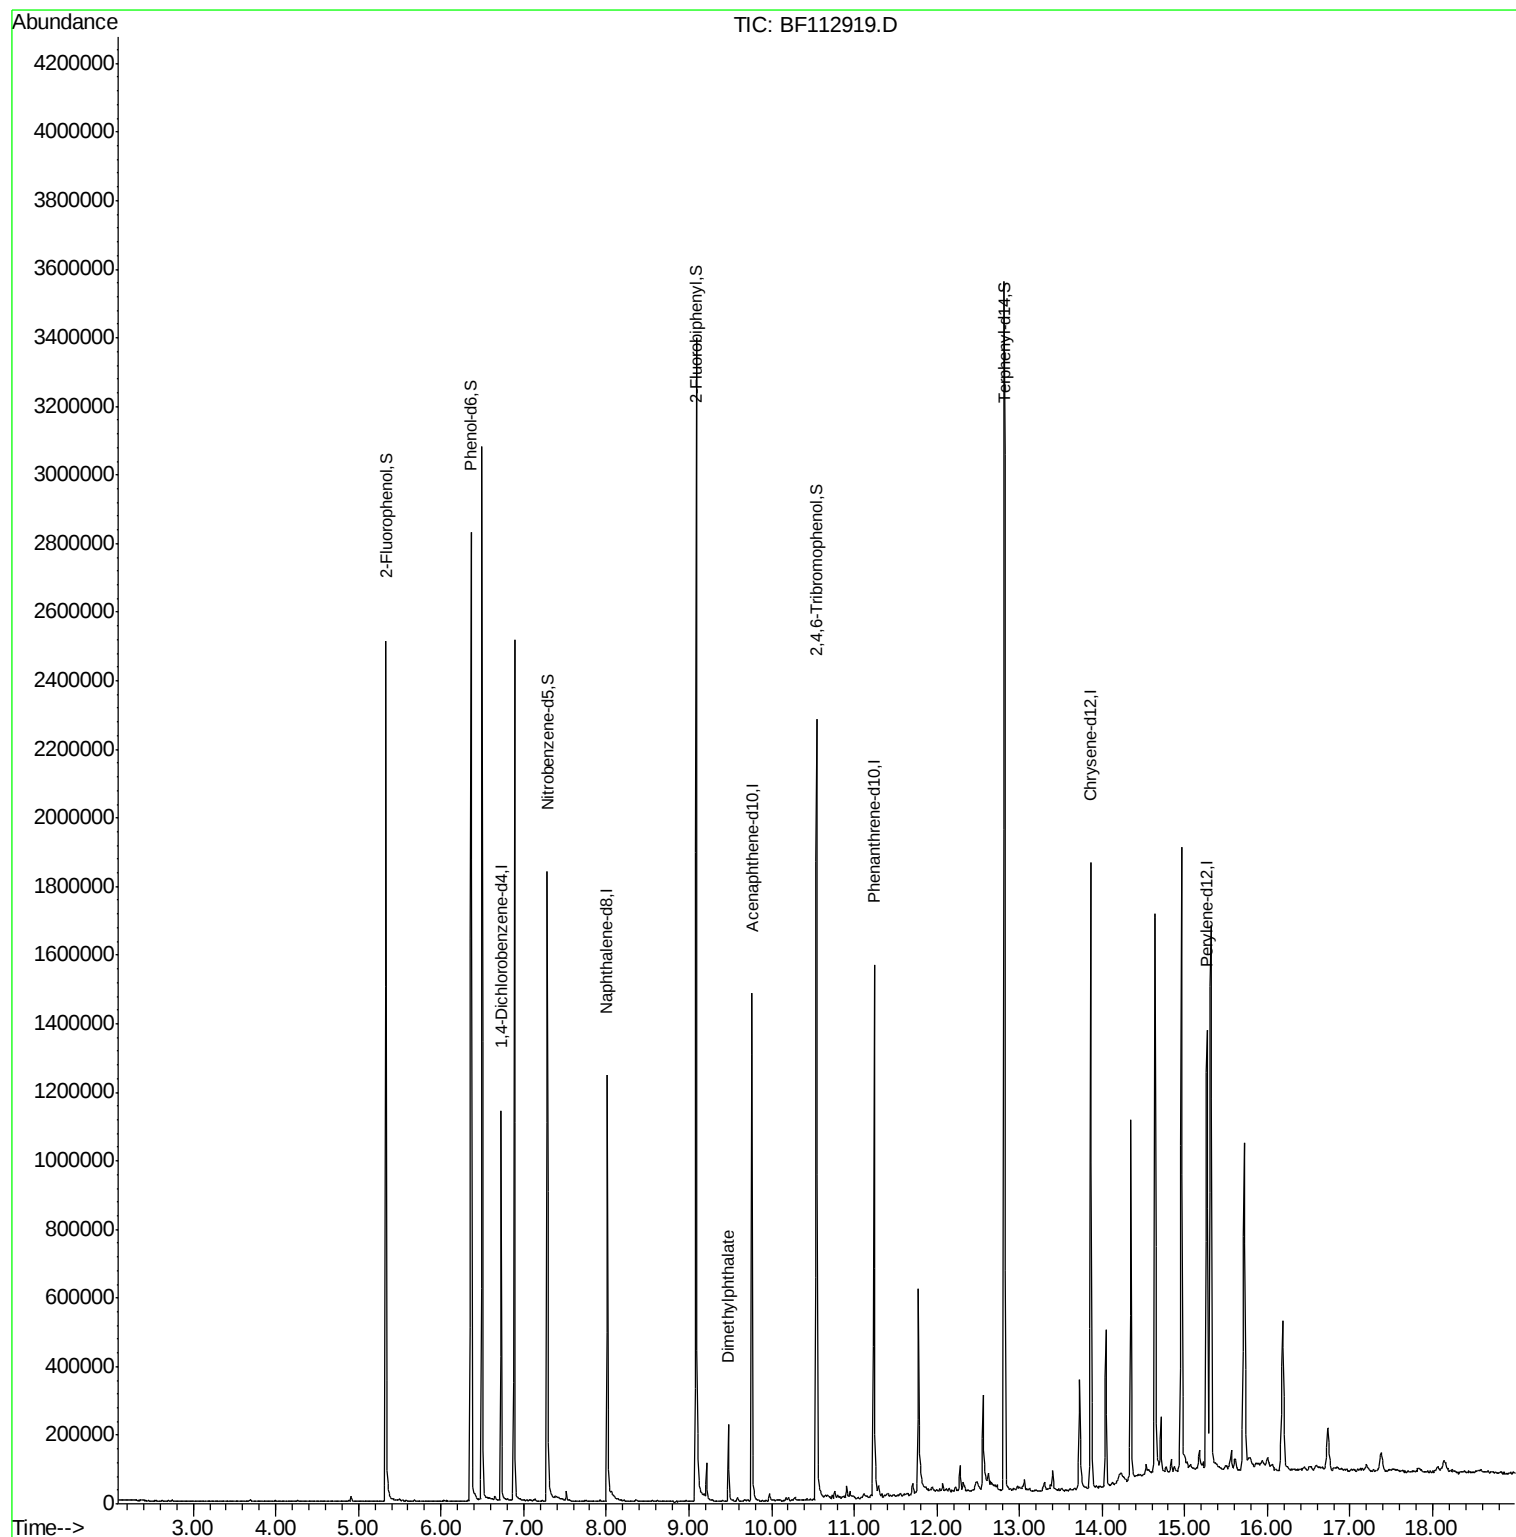

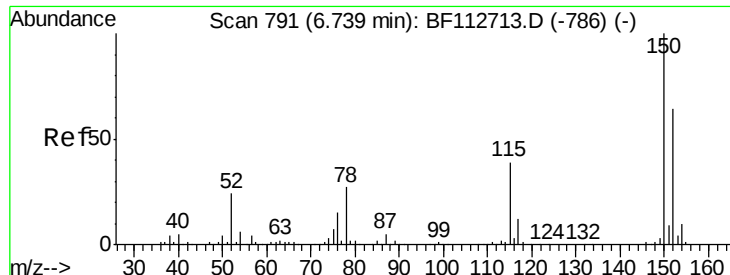


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18

Instrument :
BNA_F
ClientSampleId :
Z2-11

Tot Ion:152 Resp: 160048
Ion Ratio Lower Upper
152 100
150 156.4 124.2 186.2
115 61.3 48.2 72.4

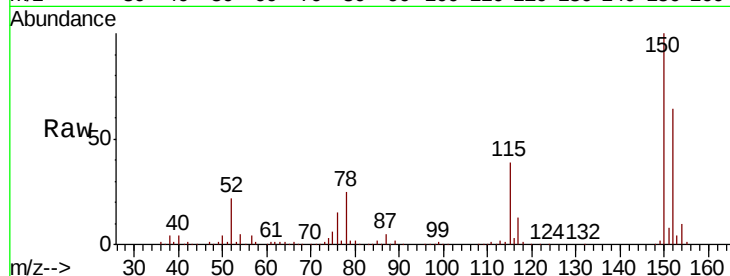


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

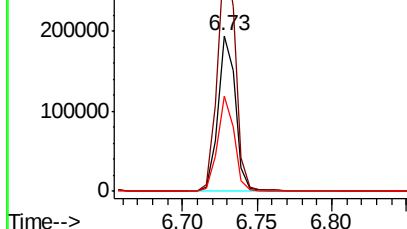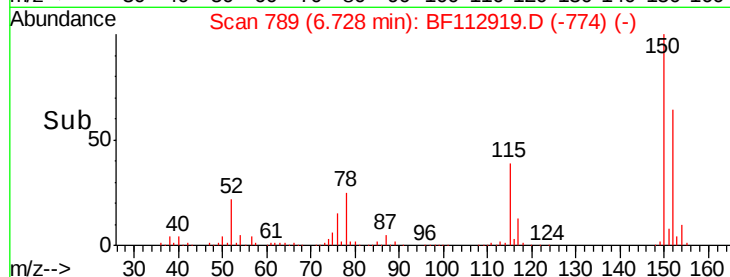



#5


2-Fluorophenol
Concen: 70.247 ng
RT: 5.33 min Scan# 552
Delta R.T. -0.01 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18

Tgt Ion:112 Resp: 722763
Ion Ratio Lower Upper
112 100
64 59.7 47.6 71.4
63 29.9 24.4 36.6

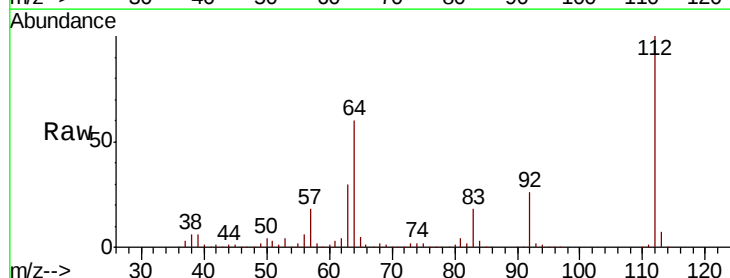

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

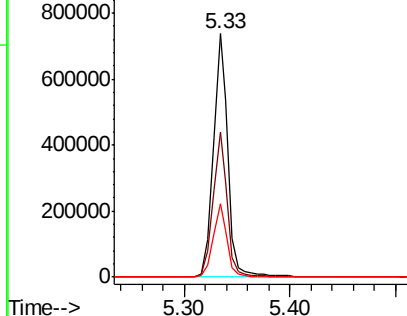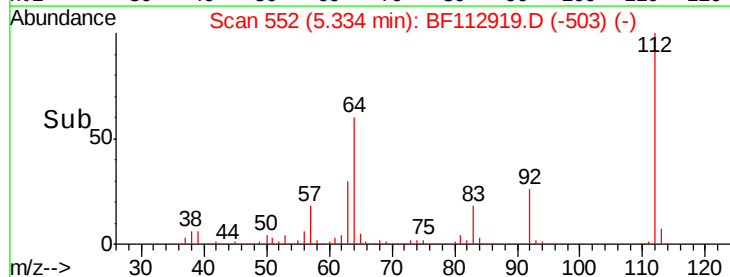

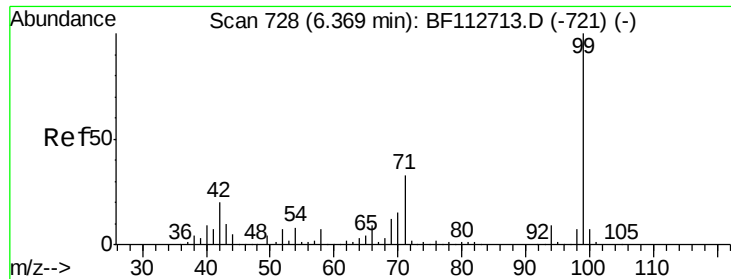

#7

Phenol-d6

Concen: 74.638 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF112919.D

Acq: 7 Mar 2019 14:18

Instrument :

BNA_F

ClientSampled :

Z2-11


Tot Ion: 99 Resp: 964662

Ion Ratio Lower Upper




99 100

42 17.9 16.3 24.5

71 31.2 26.2 39.4

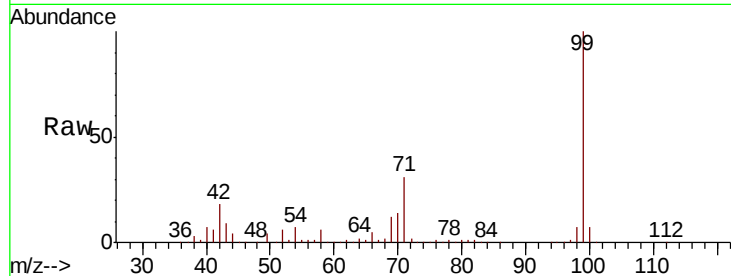

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

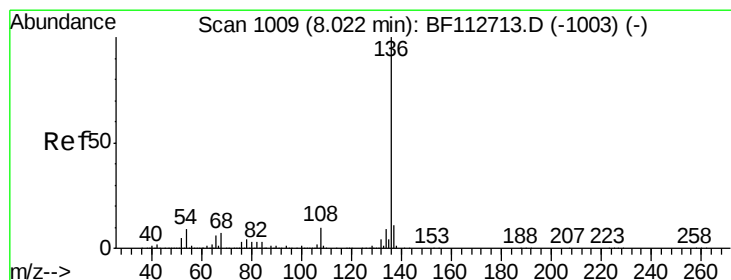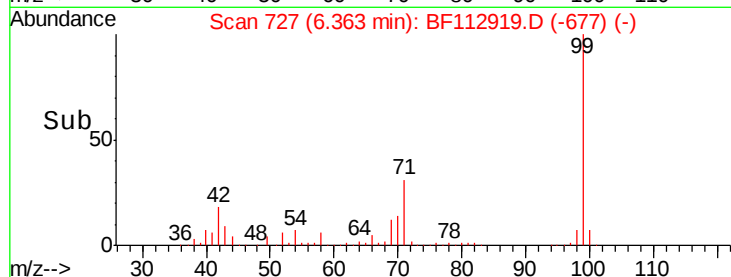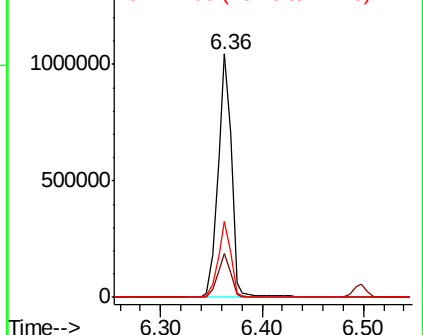

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.01 min

Lab File: BF112919.D

Acq: 7 Mar 2019 14:18

Tgt Ion: 136 Resp: 634168


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 8.4 7.3 10.9

68 6.5 5.4 8.2

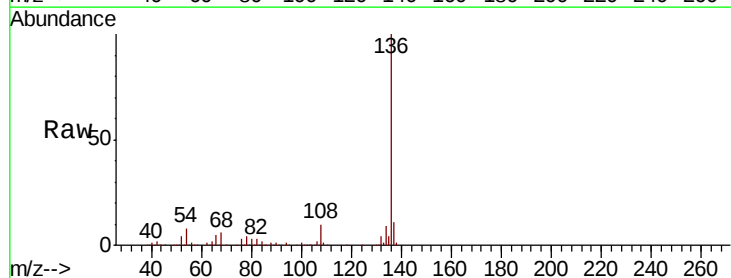

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



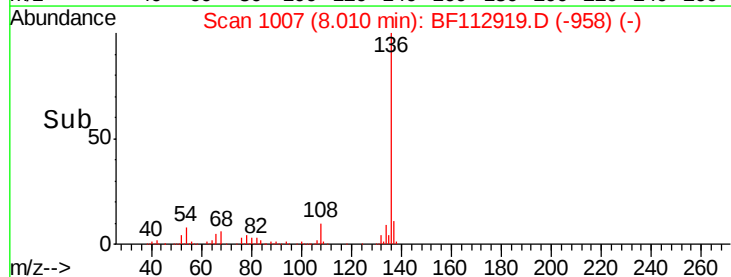
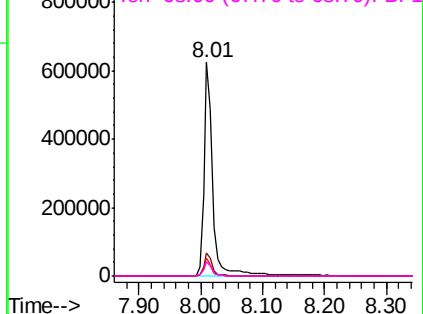


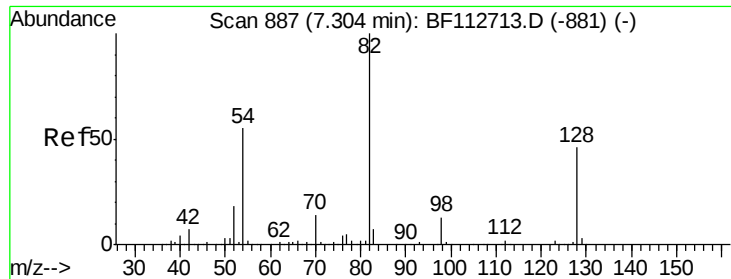

#23
Nitrobenzene-d5
Concen: 53.358 ng
RT: 7.29 min Scan# 884
Delta R.T. -0.02 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18




Instrument :
BNA_F
ClientSampleId :
Z2-11


Tot Ion: 82 Resp: 565489
Ion Ratio Lower Upper
82 100
128 47.0 36.3 54.5
54 51.8 43.7 65.5

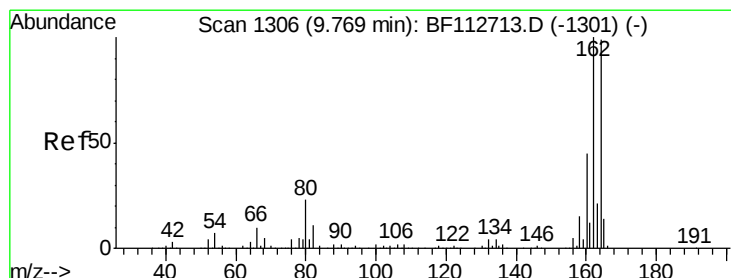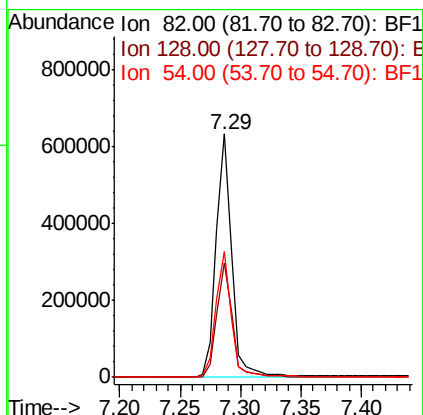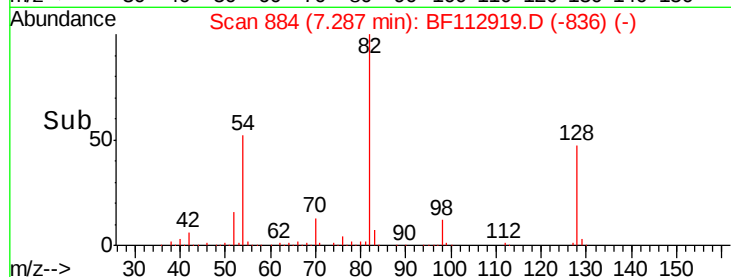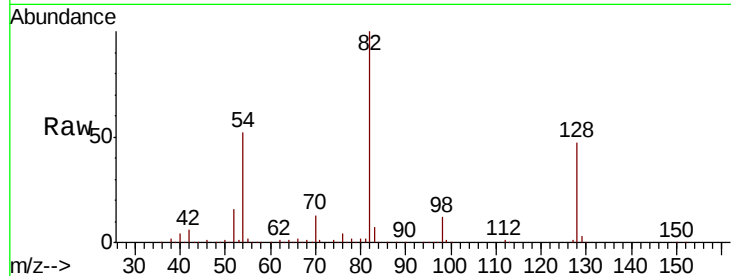

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.76 min Scan# 1305
Delta R.T. -0.01 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18

Tgt Ion:164 Resp: 314268
Ion Ratio Lower Upper
164 100
162 101.5 80.6 120.8
160 45.7 36.0 54.0

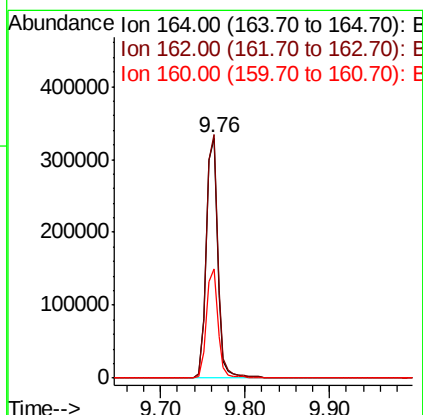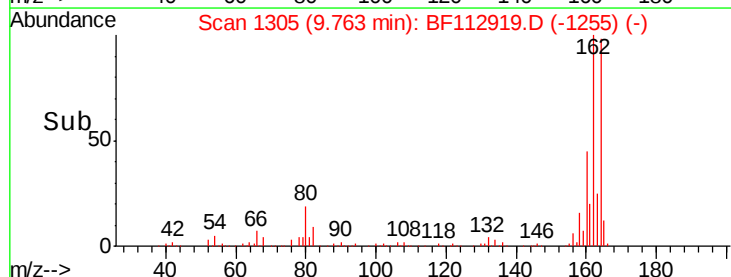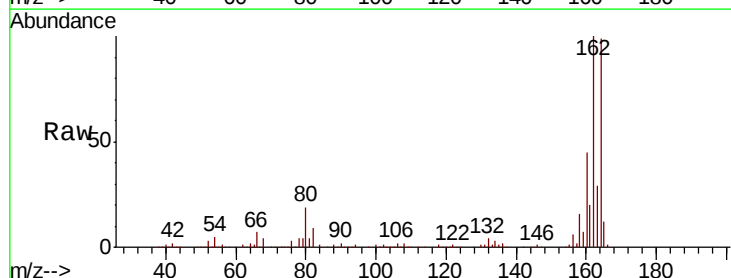


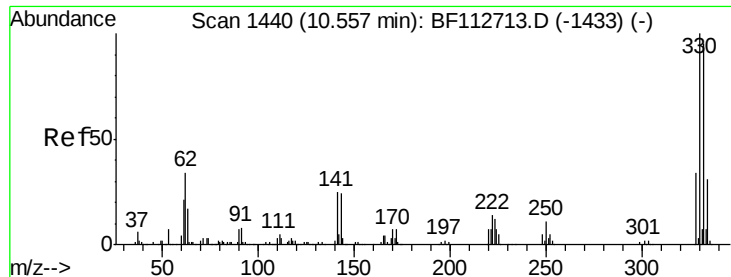




#42
 2,4,6-Tribromophenol
 Concen: 97.100 ng
 RT: 10.55 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF112919.D
 Acq: 7 Mar 2019 14:18

Instrument :
 BNA_F
 ClientSampleId :
 Z2-11

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	76.2	114.4
141	28.2	27.0	40.6

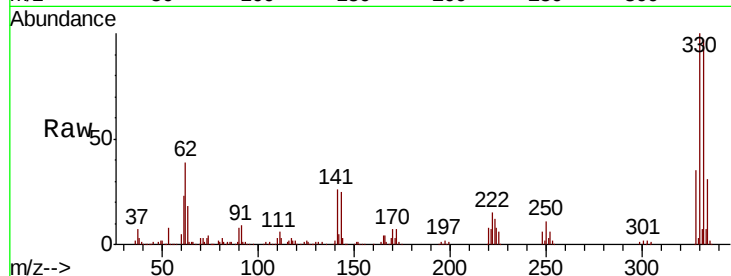


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

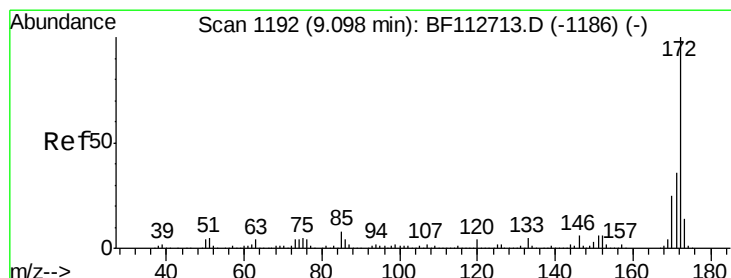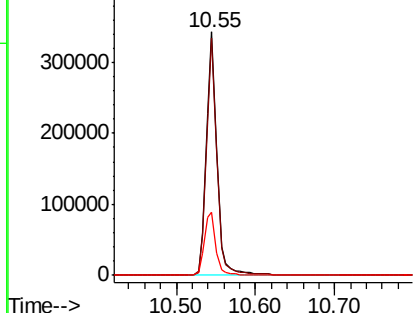
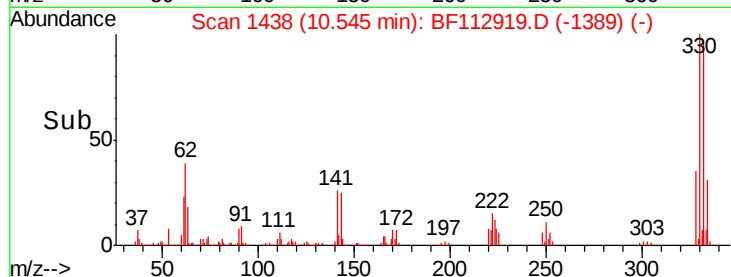



#45
 2-Fluorobiphenyl
 Concen: 53.735 ng
 RT: 9.09 min Scan# 1190
 Delta R.T. -0.01 min
 Lab File: BF112919.D
 Acq: 7 Mar 2019 14:18

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.6	29.0	43.4
170	24.3	20.0	30.0

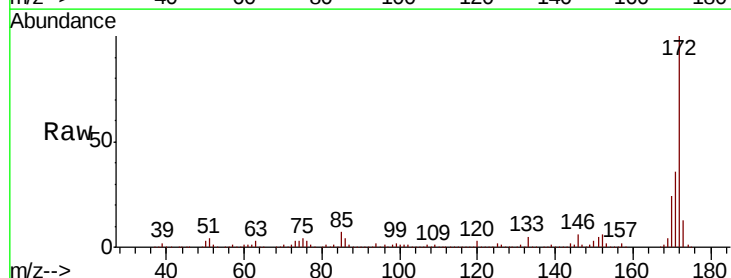

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

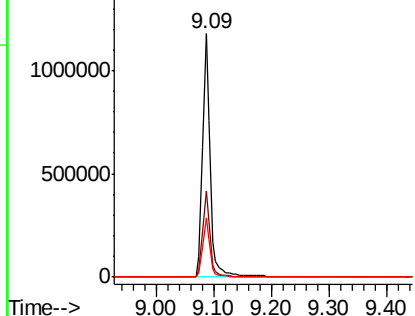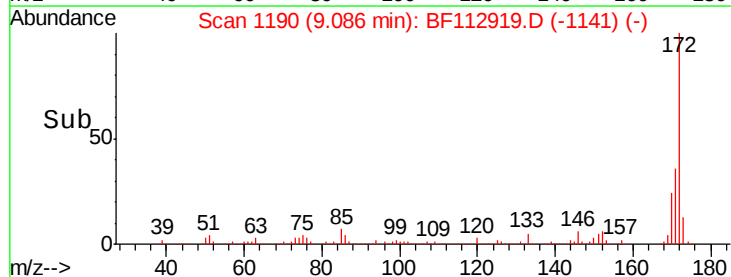


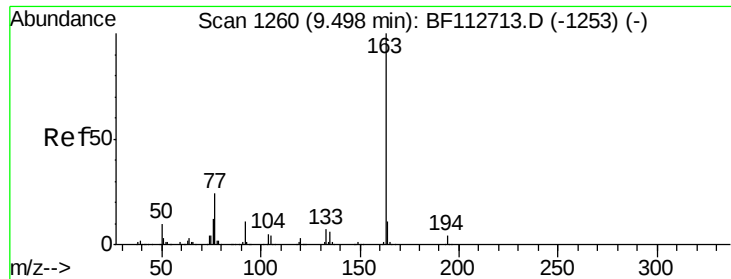

#50
Dimethylphthalate
Concen: 4.114 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.02 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18

Instrument :
BNA_F
ClientSampleId :
Z2-11

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.0	4.4
164	9.7	8.4	12.6



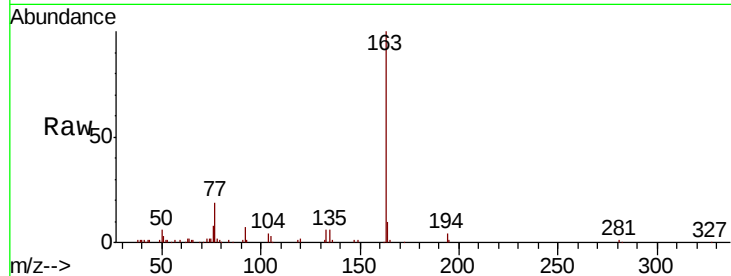


Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

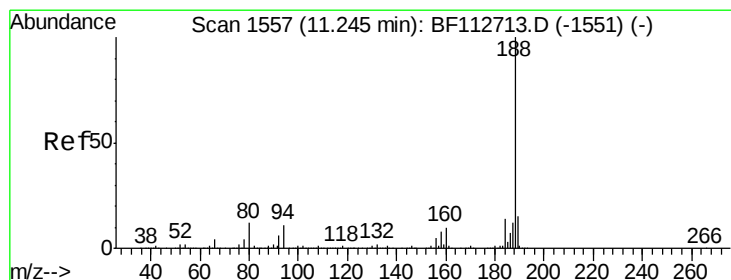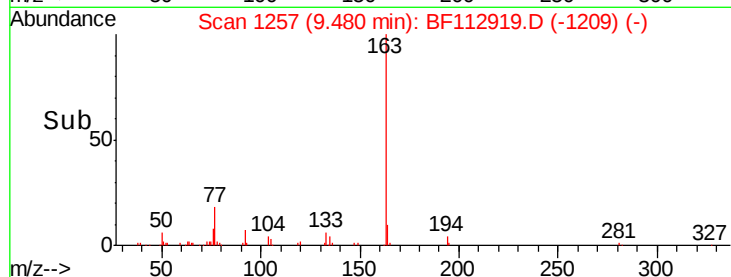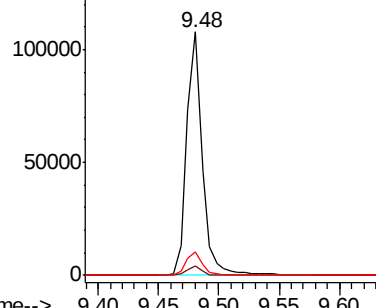

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.4	9.0	13.4
80	9.7	9.2	13.8


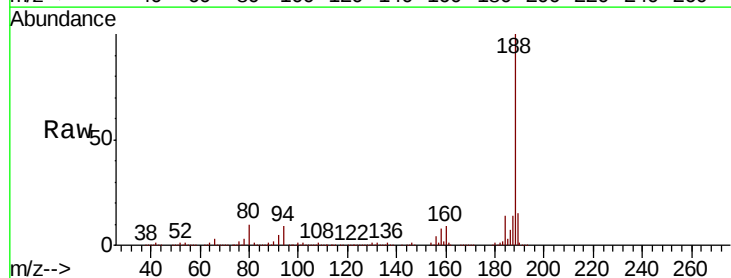



Abundance

Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

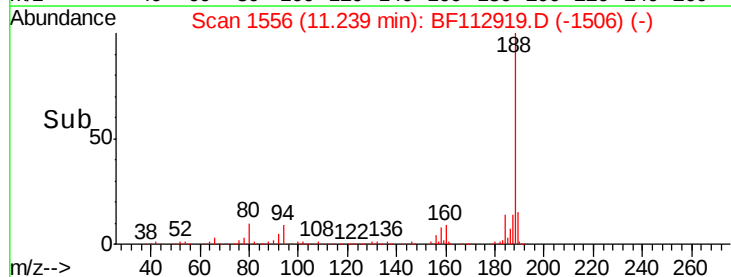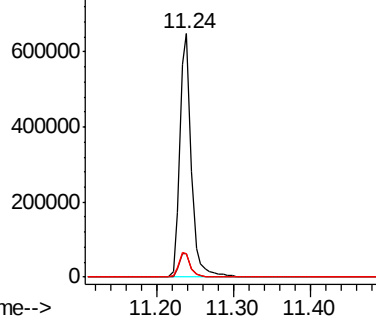


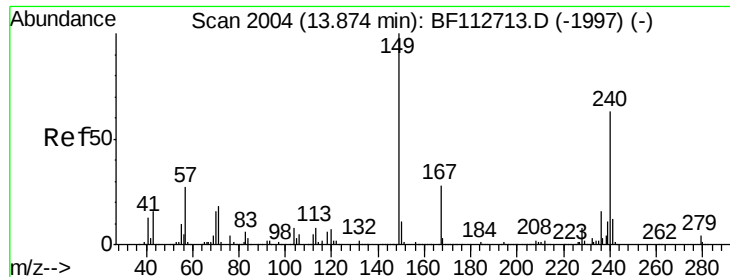




#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.86 min Scan# 2002
Delta R.T. -0.01 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18

Instrument :
BNA_F
ClientSampleId :
Z2-11

Tot Ion:240 Resp: 650659
Ion Ratio Lower Upper
240 100
120 11.5 8.9 13.3
236 26.3 20.7 31.1

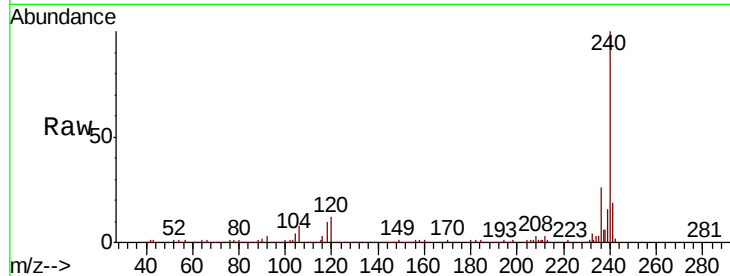


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

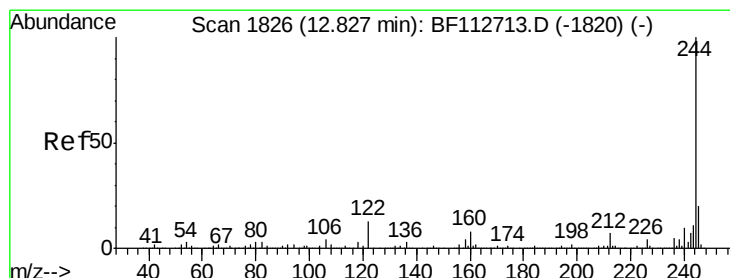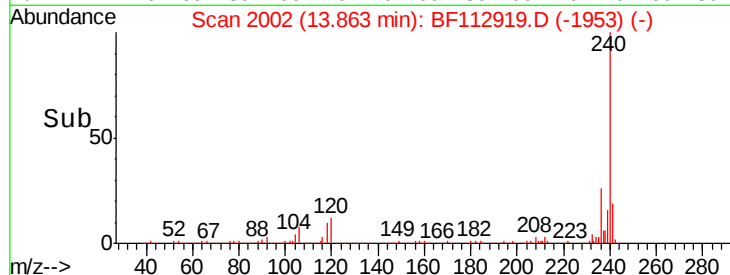
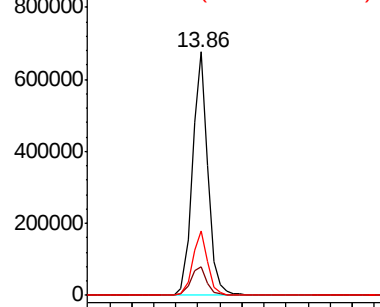



#79
Terphenyl-d14
Concen: 39.159 ng
RT: 12.82 min Scan# 1824
Delta R.T. -0.01 min
Lab File: BF112919.D
Acq: 7 Mar 2019 14:18

Tgt Ion:244 Resp: 1314390
Ion Ratio Lower Upper
244 100
212 6.8 5.6 8.4
122 11.9 10.5 15.7

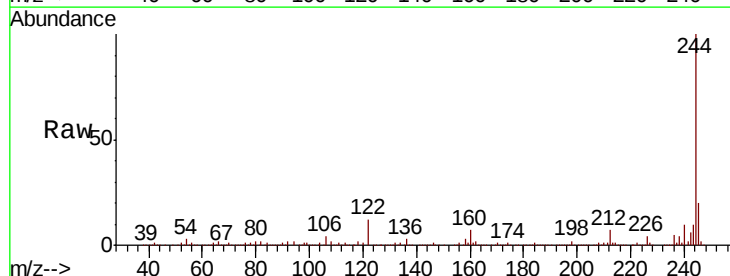

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

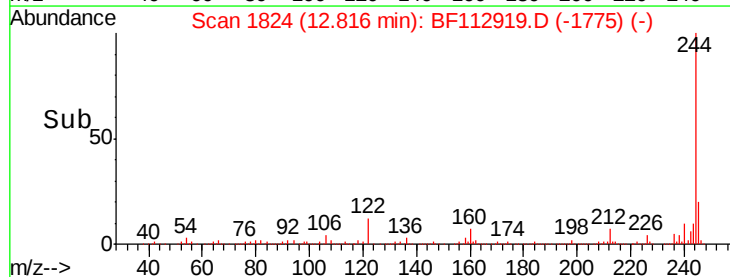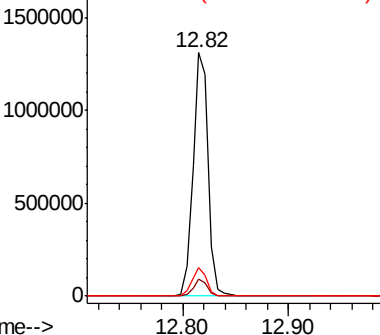

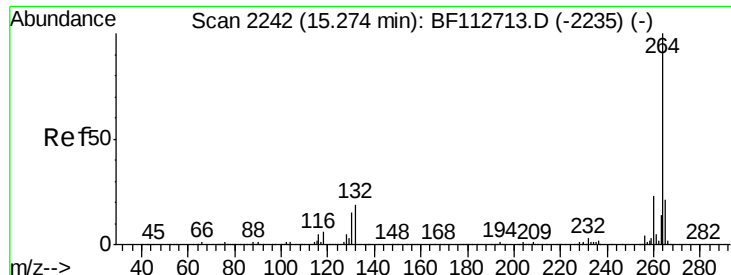

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.27 min Scan# 2241
 Delta R.T. -0.01 min
 Lab File: BF112919.D
 Acq: 7 Mar 2019 14:18

Instrument :
 BNA_F
 ClientSampleId :
 Z2-11

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.2	18.7	28.1
265	21.6	17.2	25.8

