


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030719\
 Data File : BF112916.D
 Acq On : 7 Mar 2019 12:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

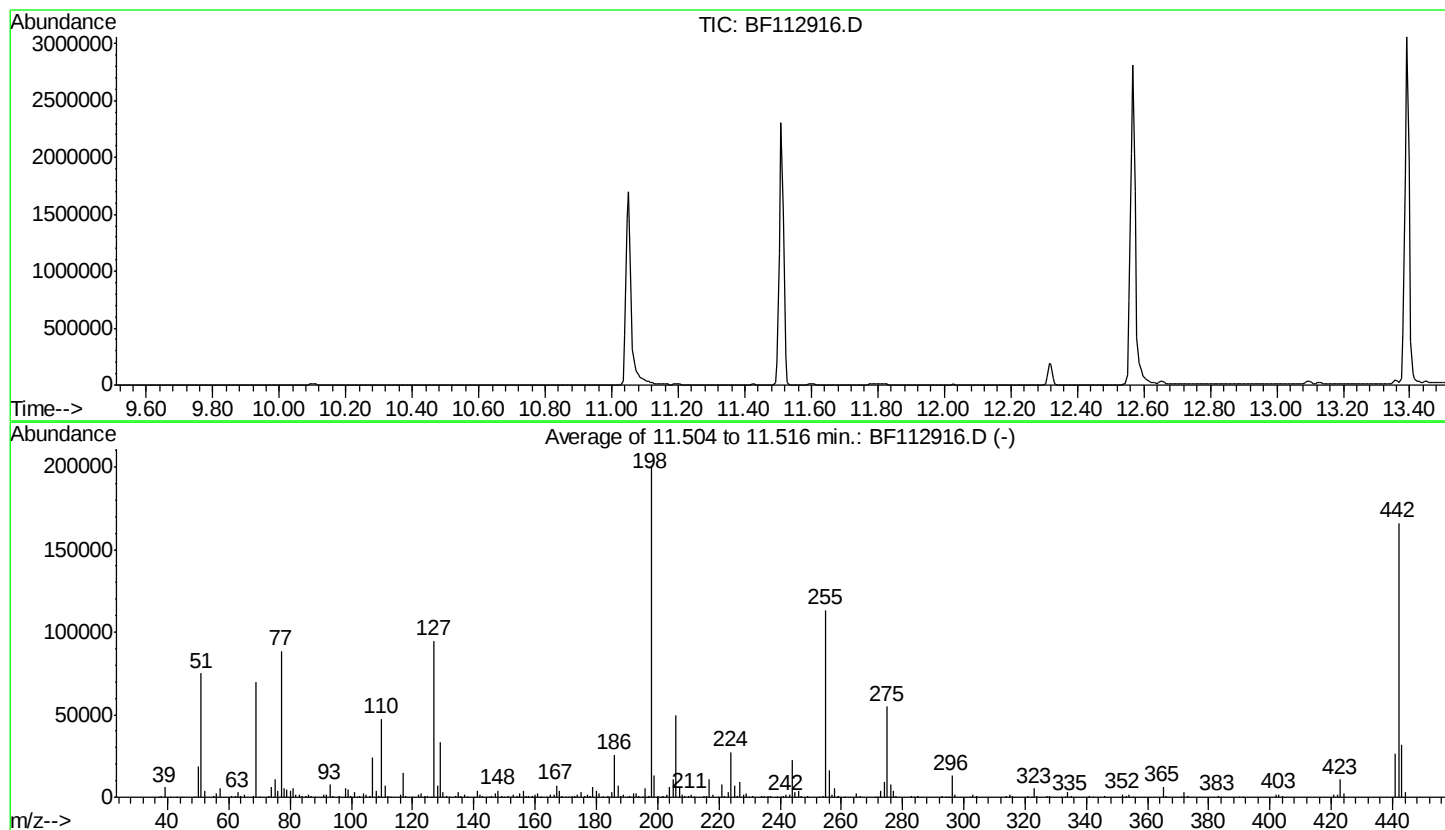

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	75106	PASS
68	69	0.00	2	1.6	1094	PASS
69	198	0.00	100	34.6	69512	PASS
70	69	0.00	2	0.2	143	PASS
127	198	10	80	47.3	94922	PASS
197	198	0.00	2	0.4	854	PASS
198	198	100	100	100.0	200874	PASS
199	198	5	9	6.5	13083	PASS
275	198	10	60	27.3	54776	PASS
365	198	1	100	3.2	6453	PASS
441	198	0.01	100	13.2	26510	PASS
442	198	50	100	82.7	166221	PASS
443	442	15	24	19.2	31842	PASS