
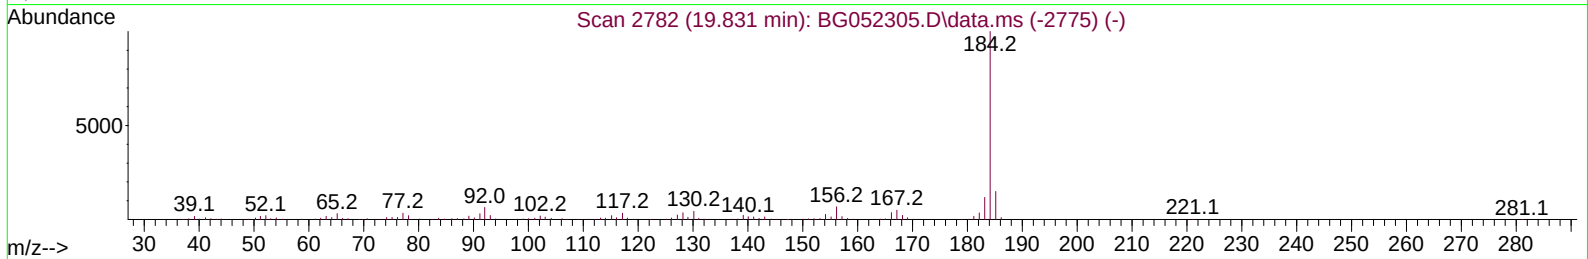
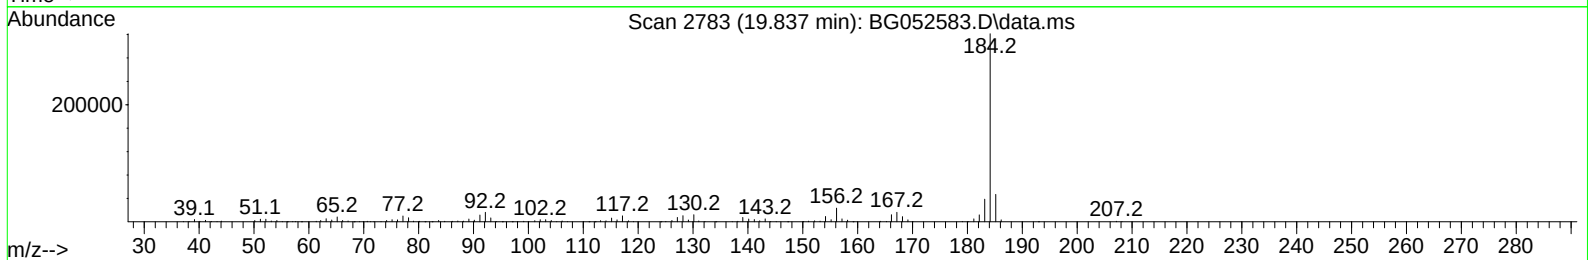


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030722\
 Data File : BG052583.D
 Acq On : 7 Mar 2022 9:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 11:29:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 07 11:25:10 2022
 Response via : Initial Calibration

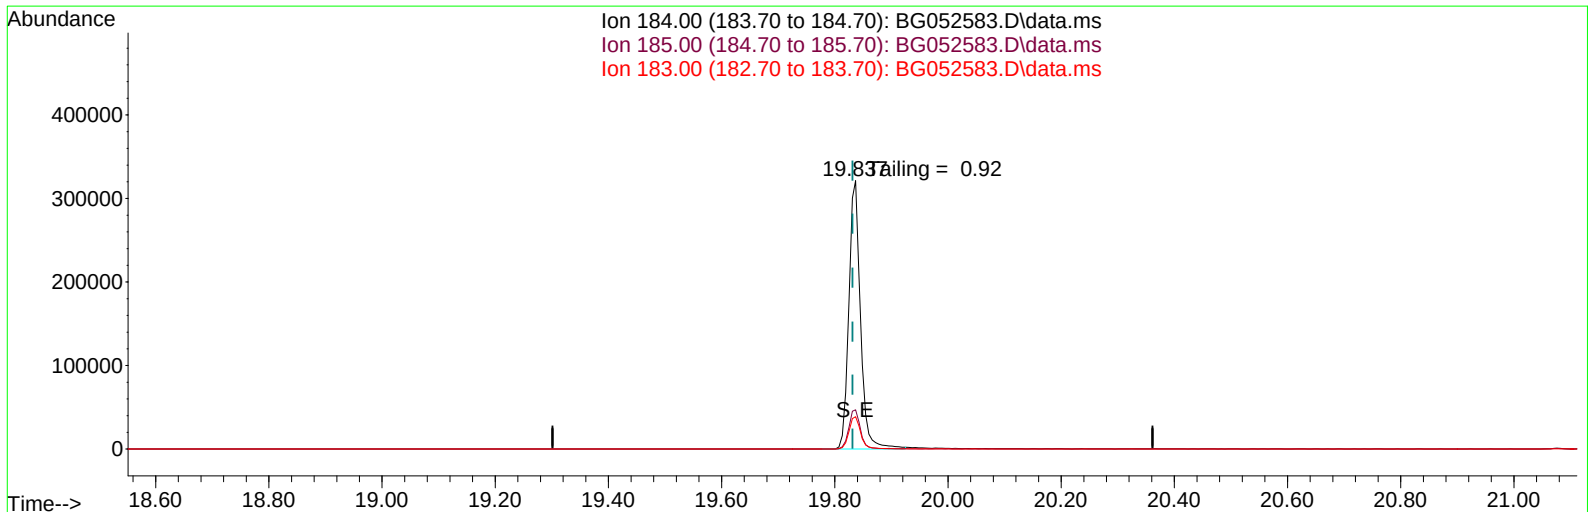

TIC: BG052583.D\data.ms

(77) Benzidine**19.837min (+ 0.006) 44930.32 ng****response 463709**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.64
183.00	12.20	12.07
0.00	0.00	0.00