
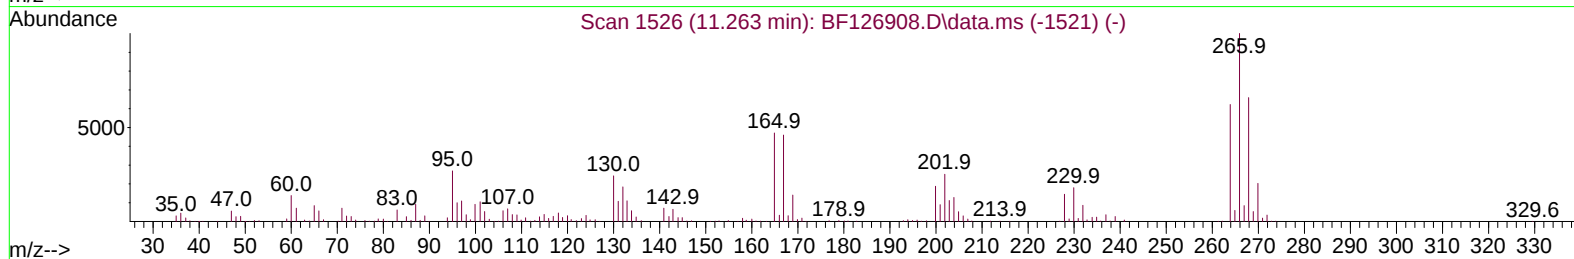
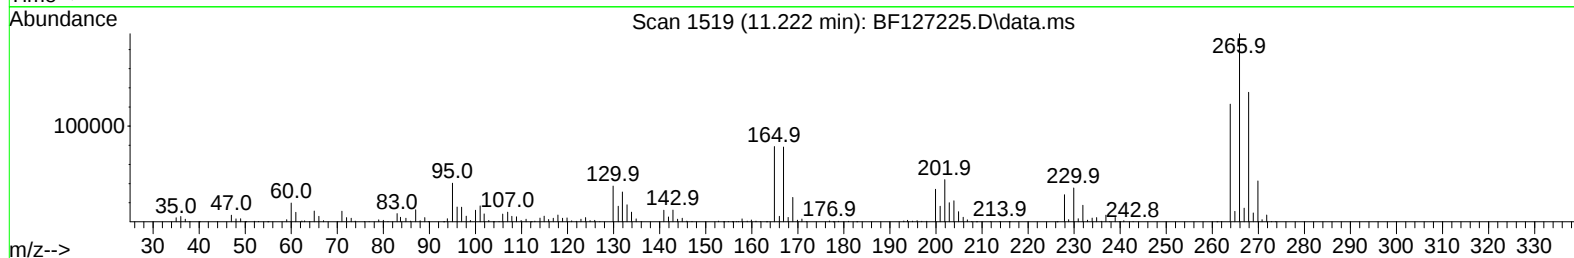


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127225.D
 Acq On : 07 Mar 2022 17:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 05:20:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 02:16:58 2022
 Response via : Initial Calibration

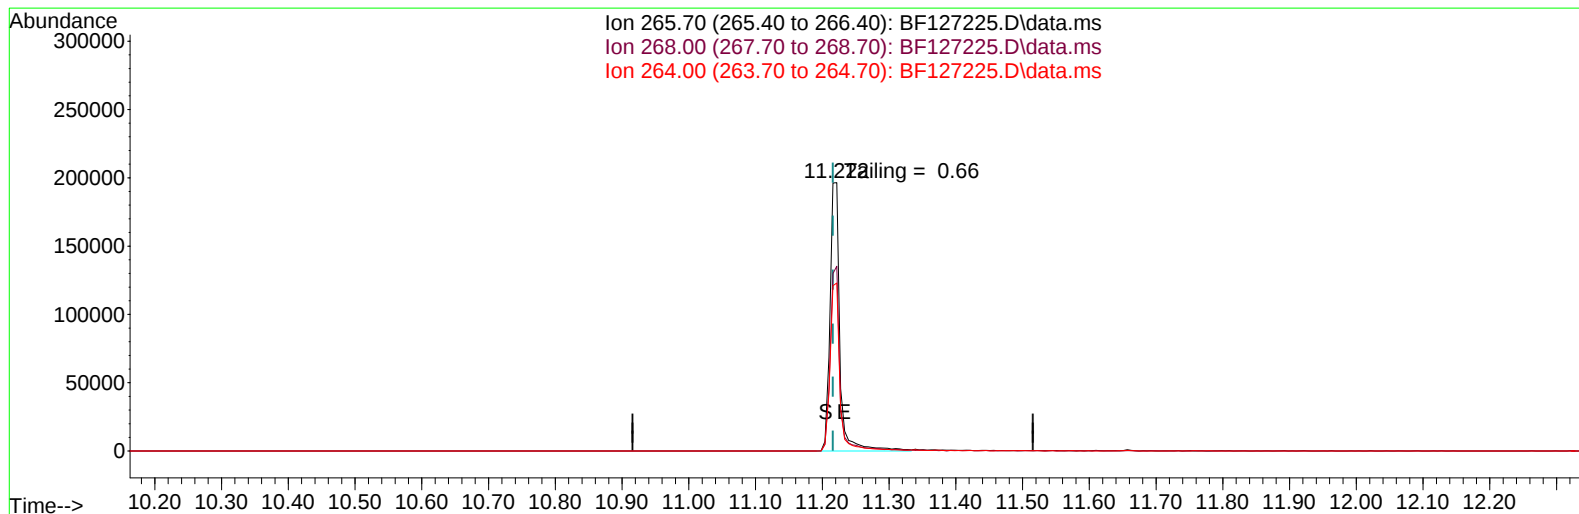

TIC: BF127225.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.006) 26546.32 ng

response 204108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	68.89
264.00	63.00	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127225.D
Acq On : 07 Mar 2022 17:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 05:20:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 02:16:58 2022
Response via : Initial Calibration

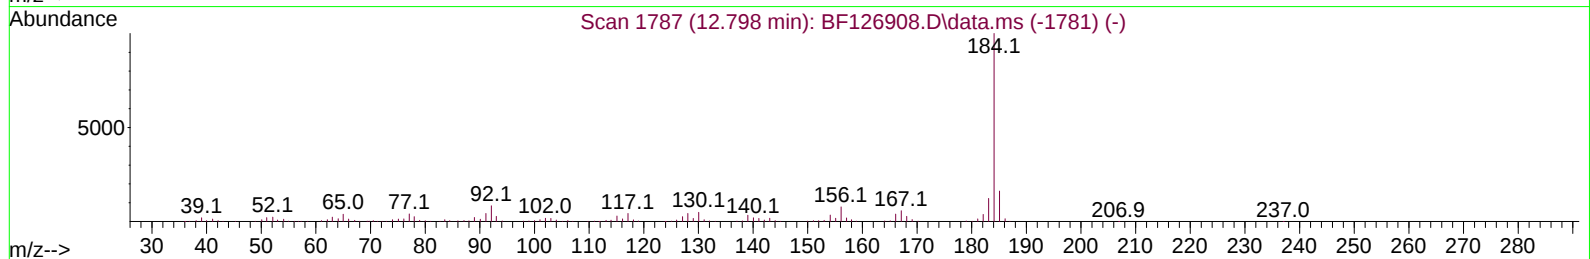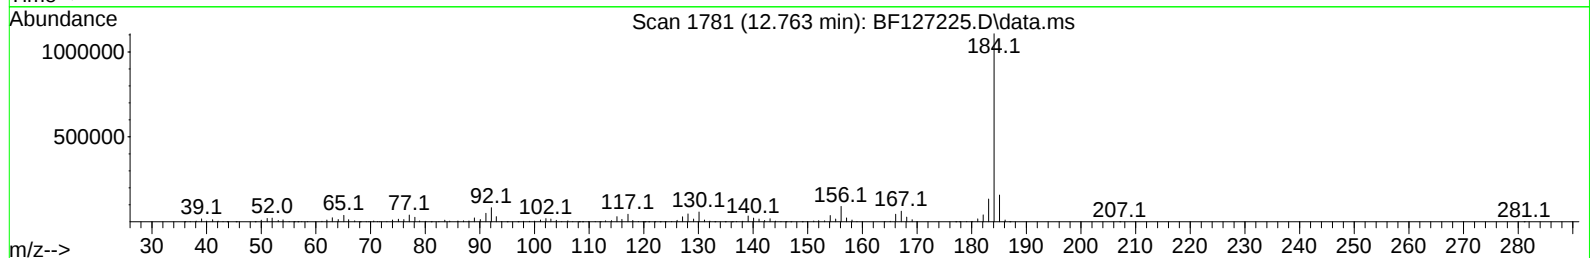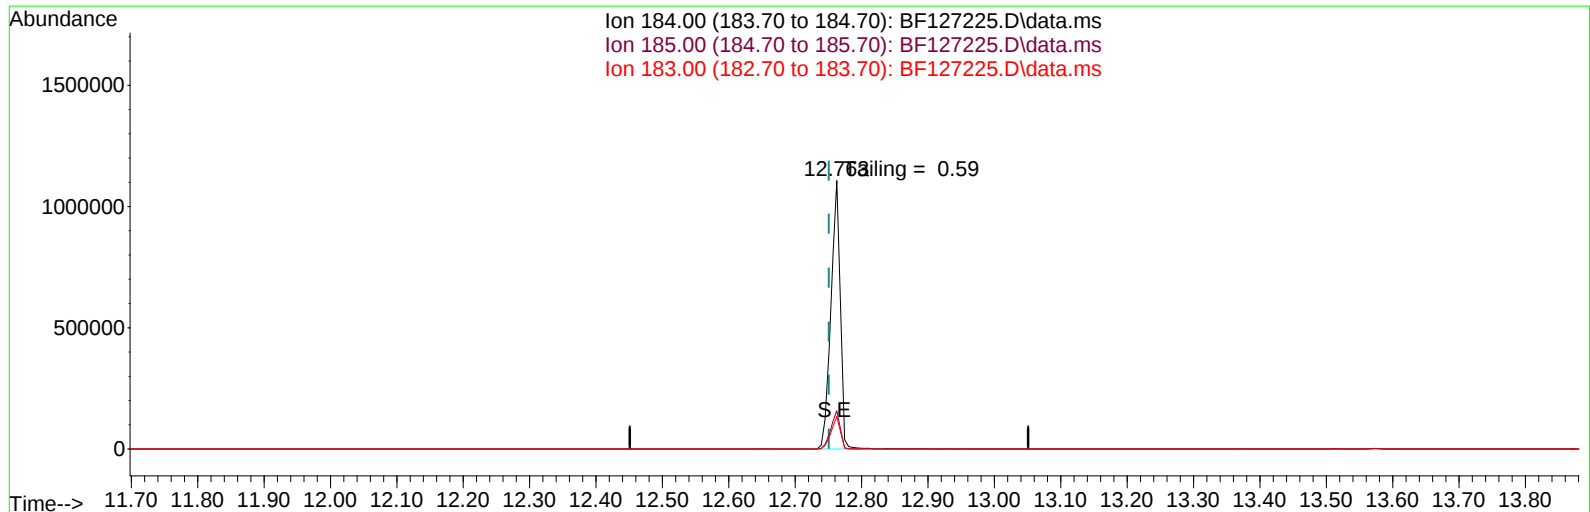

TIC: BF127225.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng

response 1091214

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.25
183.00	10.20	12.11
0.00	0.00	0.00