

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127216.D
 Acq On : 07 Mar 2022 11:20
 Operator : CG\JU
 Sample : PB143066BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143066BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	543	548	551	rBV	2976629	2896528	72.12%	12.380%
2	6.516	713	719	721	rBV	2678221	3040372	75.71%	12.995%
3	6.875	777	780	784	rBV	711410	594844	14.81%	2.542%
4	7.445	871	877	880	rBV	1971866	2047965	50.99%	8.753%
5	8.157	994	998	1002	rBV	818978	807165	20.10%	3.450%
6	9.239	1176	1182	1185	rBV	4098493	3734844	93.00%	15.963%
7	9.922	1292	1298	1301	rBV	1039076	924102	23.01%	3.950%
8	10.716	1428	1433	1436	rBV	2869587	2492965	62.08%	10.655%
9	11.410	1547	1551	1555	rBV	1178758	1009263	25.13%	4.314%
10	13.004	1817	1822	1825	rBV	4445019	4016047	100.00%	17.165%
11	13.845	1959	1965	1968	rBV	33329	46429	1.16%	0.198%
12	13.921	1974	1978	1983	rVB	106862	106958	2.66%	0.457%
13	14.057	1997	2001	2005	rBV	761303	659721	16.43%	2.820%
14	14.151	2011	2017	2023	rBV	54526	74400	1.85%	0.318%
15	15.162	2186	2189	2194	rVB2	45545	52419	1.31%	0.224%
16	15.551	2249	2255	2262	rBV	447186	585807	14.59%	2.504%
17	15.998	2325	2331	2336	rBV	45736	71266	1.77%	0.305%
18	16.515	2414	2419	2429	rVB3	43717	77763	1.94%	0.332%
19	17.127	2515	2523	2531	rVB2	28124	68088	1.70%	0.291%
20	17.298	2542	2552	2553	rBV3	43639	90201	2.25%	0.386%




Sum of corrected areas: 23397147

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127216.D
Acq On : 07 Mar 2022 11:20
Operator : CG\JU
Sample : PB143066BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143066BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

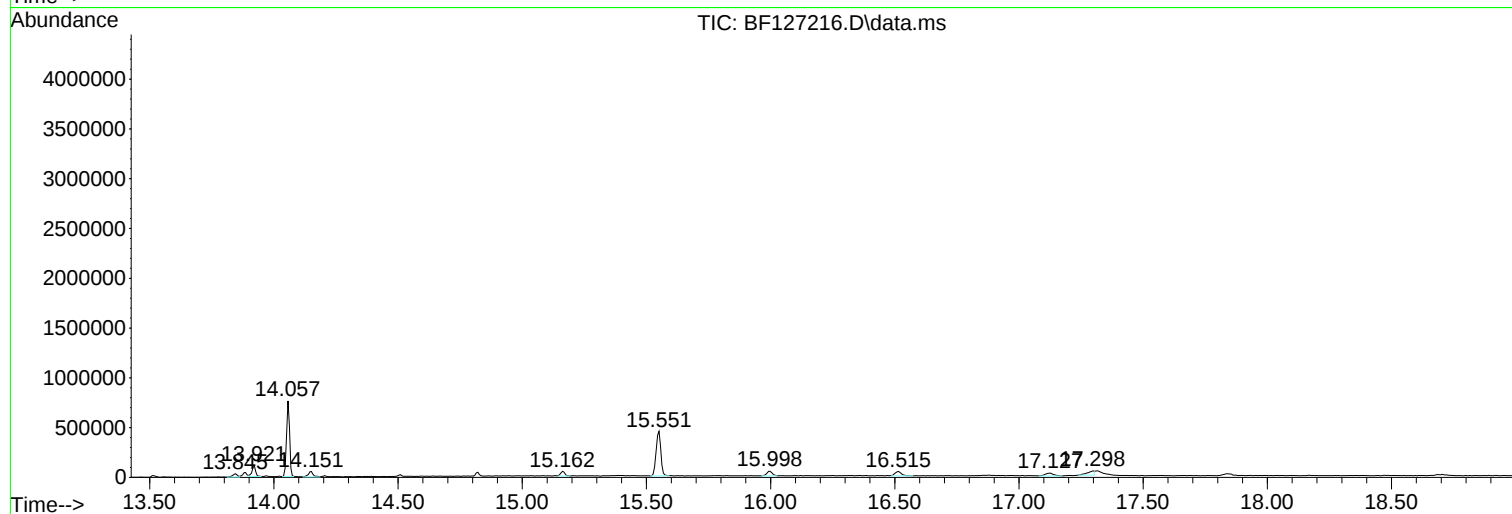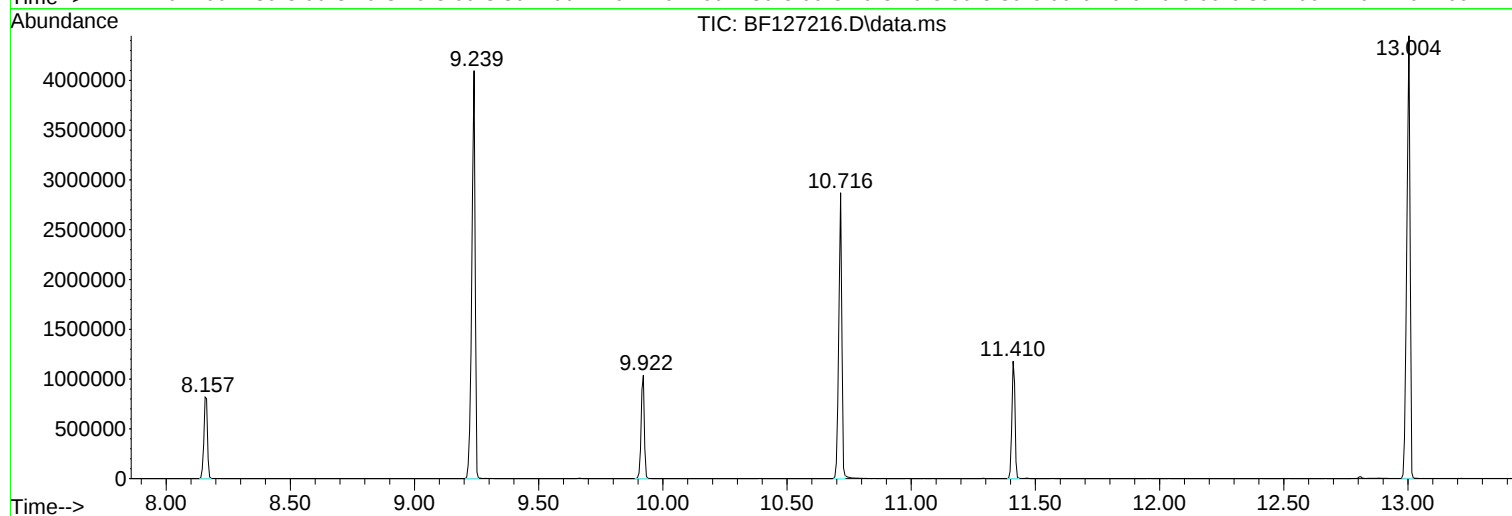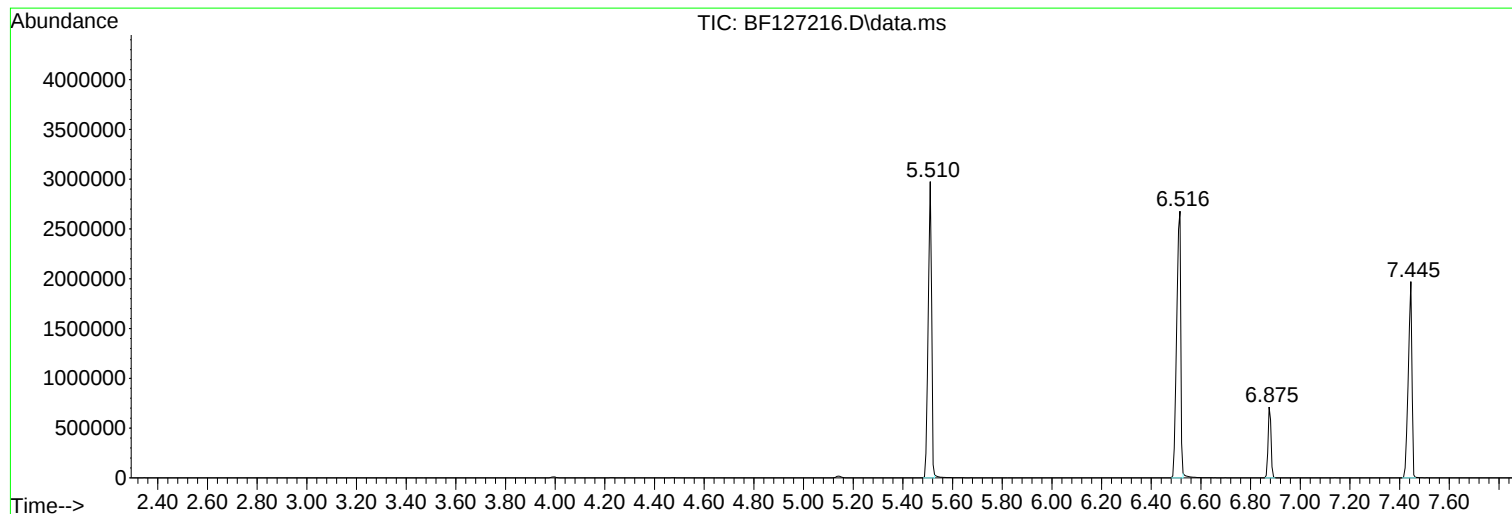

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127216.D
Acq On : 07 Mar 2022 11:20
Operator : CG\JU
Sample : PB143066BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143066BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127216.D
Acq On : 07 Mar 2022 11:20
Operator : CG\JU
Sample : PB143066BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143066BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------