

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127229.D
 Acq On : 07 Mar 2022 19:18
 Operator : CG\JU
 Sample : N1730-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 13-14-SAMPLE-LOCATION-7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	542	547	550	rBV	2256704	2153639	86.34%	11.917%
2	6.510	713	718	721	rBV	2252229	2133528	85.53%	11.805%
3	6.875	777	780	784	rBV	699226	558637	22.40%	3.091%
4	7.440	871	876	879	rBV	1444460	1439950	57.73%	7.968%
5	8.063	978	982	990	rBV2	21524	50726	2.03%	0.281%
6	8.157	995	998	1002	rVV	877250	740685	29.69%	4.098%
7	9.239	1176	1182	1185	rBV	2689995	2494357	100.00%	13.802%
8	9.304	1189	1193	1197	rVB	38759	33720	1.35%	0.187%
9	9.628	1243	1248	1250	rBV	41115	39114	1.57%	0.216%
10	9.839	1280	1284	1288	rVB	44888	41408	1.66%	0.229%
11	9.916	1294	1297	1301	rVB	988459	895520	35.90%	4.955%
12	10.316	1362	1365	1366	rBV	35240	31225	1.25%	0.173%
13	10.339	1366	1369	1372	rVB2	73060	66736	2.68%	0.369%
14	10.557	1399	1406	1408	rBV3	29580	36367	1.46%	0.201%
15	10.710	1428	1432	1436	rBV	1948372	1805940	72.40%	9.993%
16	10.810	1444	1449	1454	rVB2	68255	80360	3.22%	0.445%
17	11.263	1521	1526	1528	rBV	62170	61325	2.46%	0.339%
18	11.286	1528	1530	1536	rVB2	31859	39120	1.57%	0.216%
19	11.351	1538	1541	1544	rVB	67449	56796	2.28%	0.314%
20	11.410	1547	1551	1554	rBV	1183656	946723	37.95%	5.238%
21	11.569	1575	1578	1583	rBV2	49939	54627	2.19%	0.302%
22	11.686	1595	1598	1601	rBV	52771	42401	1.70%	0.235%
23	11.963	1640	1645	1647	rBV	50278	42823	1.72%	0.237%
24	12.098	1665	1668	1671	rBV	41803	38136	1.53%	0.211%
25	12.480	1730	1733	1735	rBV3	45516	45315	1.82%	0.251%
26	12.998	1817	1821	1824	rBV	2951156	2489435	99.80%	13.775%
27	13.845	1960	1965	1968	rBV	32869	46338	1.86%	0.256%
28	13.886	1968	1972	1974	rVV	46058	48213	1.93%	0.267%
29	13.922	1974	1978	1981	rVV	130750	120414	4.83%	0.666%
30	14.057	1997	2001	2005	rVB	859448	732843	29.38%	4.055%
31	14.151	2013	2017	2022	rVB	38953	40641	1.63%	0.225%
32	14.669	2103	2105	2110	rVB2	30957	31531	1.26%	0.174%
33	14.804	2125	2128	2134	rBV5	20671	33856	1.36%	0.187%
34	15.545	2249	2254	2260	rBV2	489529	600137	24.06%	3.321%

Sum of corrected areas: 18072586

Instrument :

BNA_F

ClientSampleId :




13-14-SAMPLE-LOCATION-7

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127229.D
Acq On : 07 Mar 2022 19:18
Operator : CG\JU
Sample : N1730-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
13-14-SAMPLE-LOCATION-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

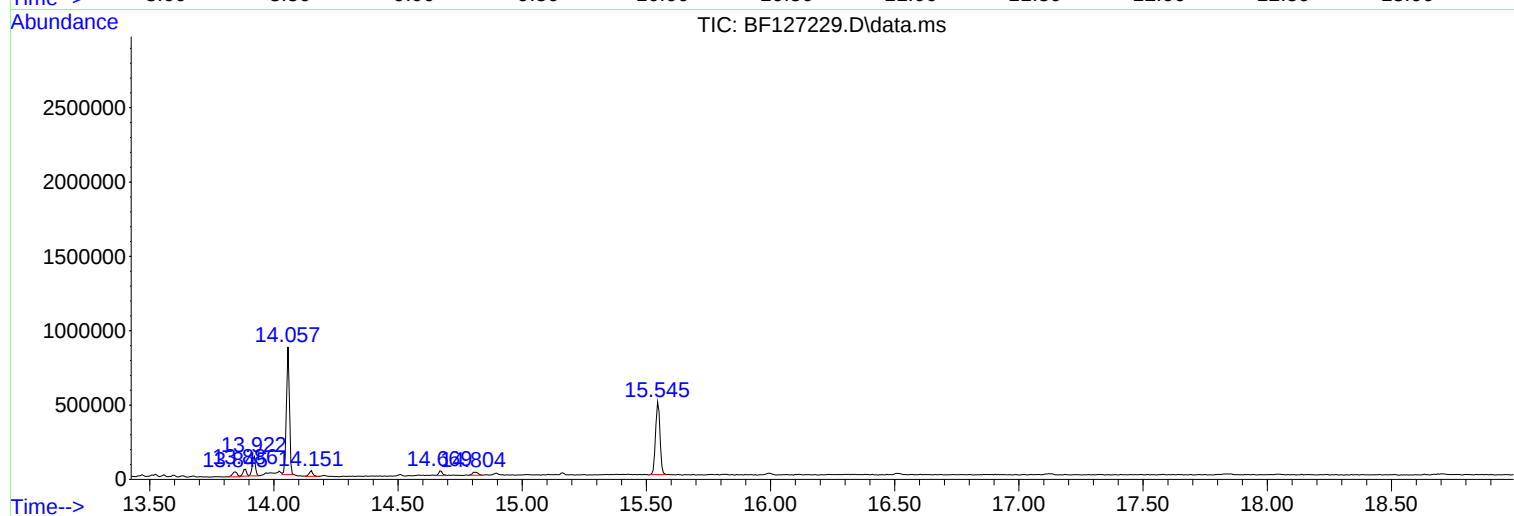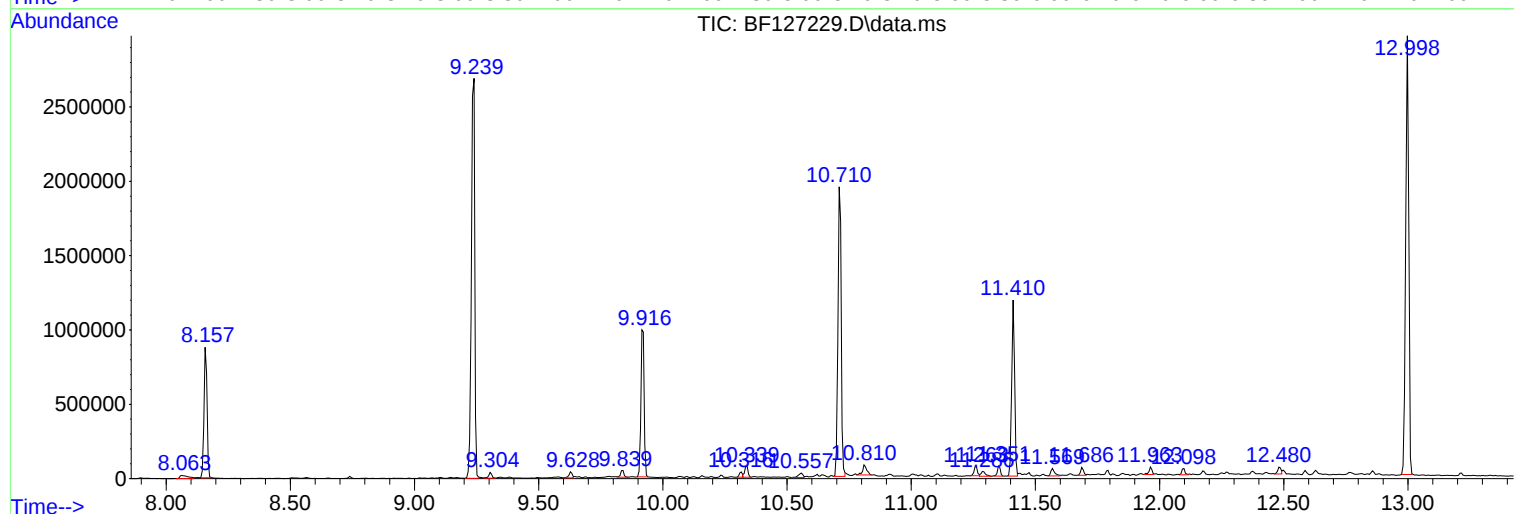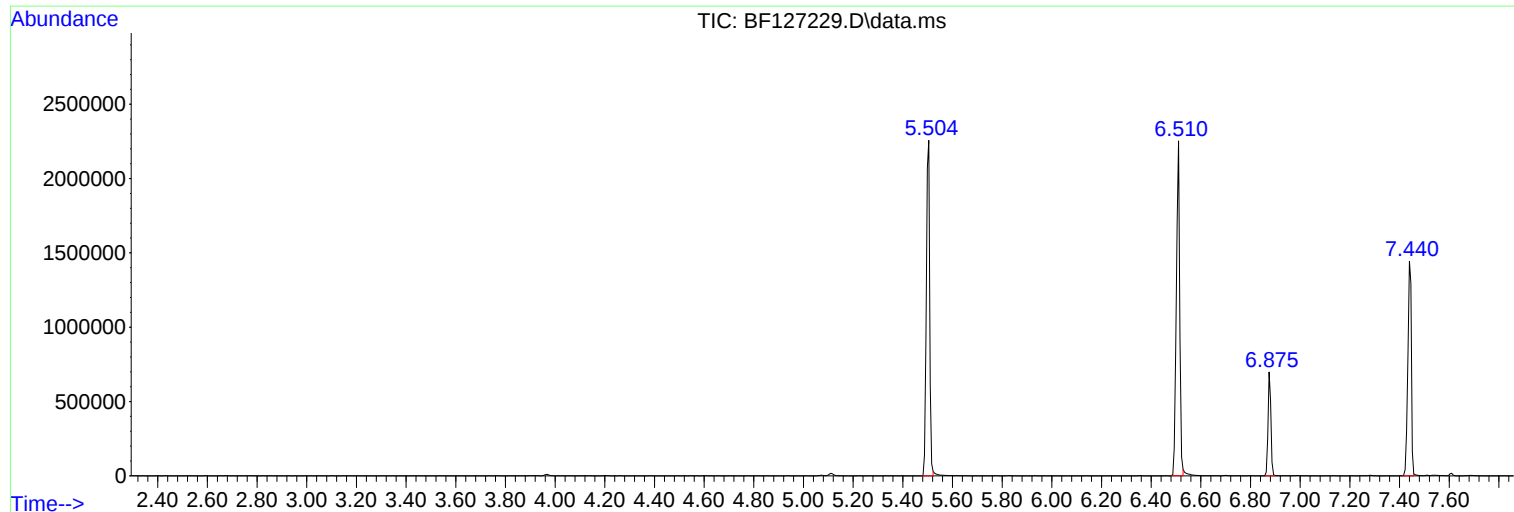

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127229.D
Acq On : 07 Mar 2022 19:18
Operator : CG\JU
Sample : N1730-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
13-14-SAMPLE-LOCATION-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127229.D
Acq On : 07 Mar 2022 19:18
Operator : CG\JU
Sample : N1730-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
13-14-SAMPLE-LOCATION-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc