

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127236.D
 Acq On : 07 Mar 2022 22:52
 Operator : CG\JU
 Sample : N1806-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUM-25

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	477	480	488	rVB	29397	36097	1.24%	0.189%
2	5.504	542	547	550	rBV	2568563	2331471	80.04%	12.213%
3	6.510	713	718	721	rBV	2480425	2440479	83.78%	12.784%
4	6.875	777	780	784	rBV	722991	578903	19.87%	3.032%
5	7.445	871	877	880	rBV	1687133	1692232	58.10%	8.865%
6	8.157	994	998	1002	rBV	888570	796287	27.34%	4.171%
7	9.239	1176	1182	1185	rBV	3136462	2912798	100.00%	15.258%
8	9.916	1294	1297	1301	rBV	1010858	884290	30.36%	4.632%
9	10.710	1428	1432	1436	rBV	2145769	1992024	68.39%	10.435%
10	11.410	1547	1551	1554	rBV	1096534	912667	31.33%	4.781%
11	11.433	1554	1555	1558	rVB	88972	45129	1.55%	0.236%
12	12.627	1754	1758	1761	rBV	149973	137467	4.72%	0.720%
13	12.857	1794	1797	1800	rVB	113271	94147	3.23%	0.493%
14	12.998	1816	1821	1824	rBV	3055867	2705782	92.89%	14.174%
15	13.845	1960	1965	1968	rBV3	26586	41269	1.42%	0.216%
16	13.880	1968	1971	1974	rVV	31348	31888	1.09%	0.167%
17	13.921	1974	1978	1981	rVB	94243	89473	3.07%	0.469%
18	13.974	1981	1987	1990	rBV5	24550	51145	1.76%	0.268%
19	14.057	1997	2001	2004	rBV	626834	566204	19.44%	2.966%
20	14.080	2004	2005	2012	rVB	59671	44285	1.52%	0.232%
21	14.151	2013	2017	2023	rVB2	26361	32203	1.11%	0.169%
22	15.104	2176	2179	2183	rBV	39447	62310	2.14%	0.326%
23	15.415	2229	2232	2237	rVB	22317	33134	1.14%	0.174%
24	15.480	2239	2243	2247	rVV	27994	35377	1.21%	0.185%
25	15.545	2249	2254	2263	rVV	398942	511153	17.55%	2.678%
26	17.045	2505	2509	2517	rBV3	18917	31763	1.09%	0.166%




Sum of corrected areas: 19089977

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127236.D
Acq On : 07 Mar 2022 22:52
Operator : CG\JU
Sample : N1806-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUM-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

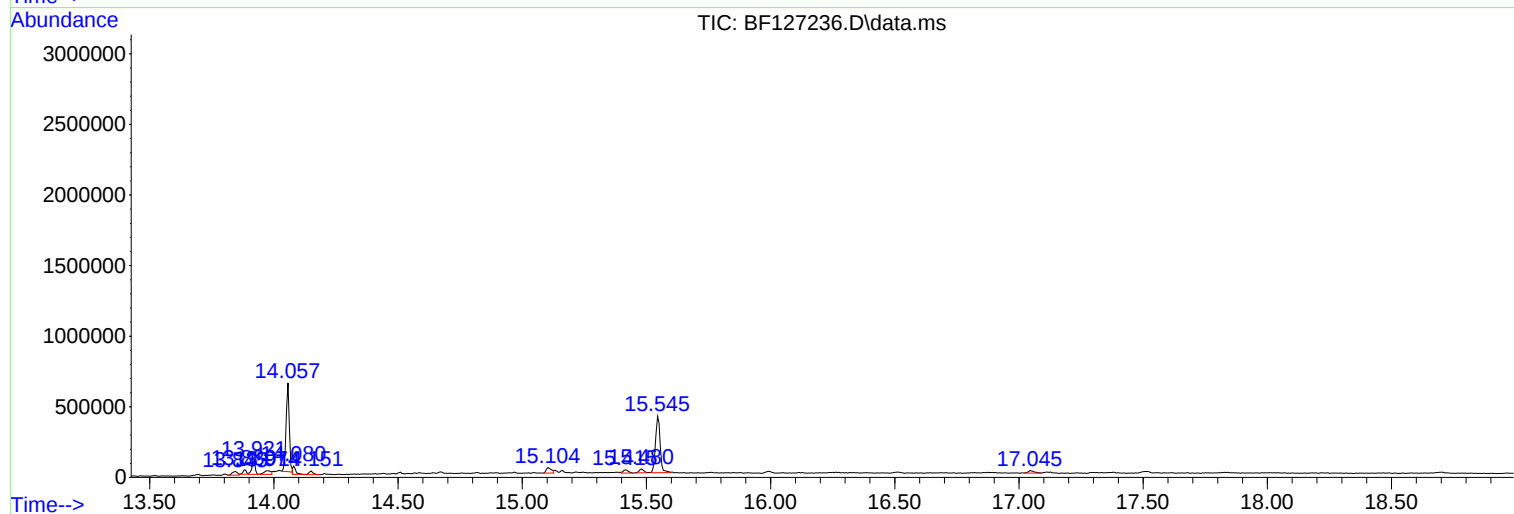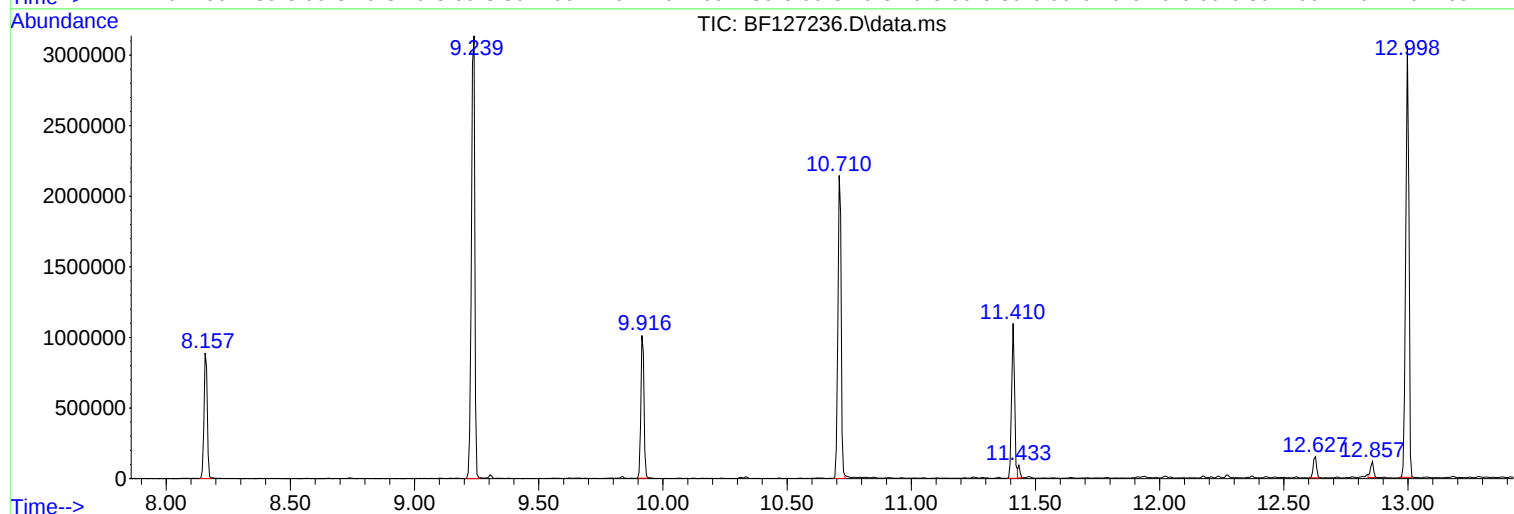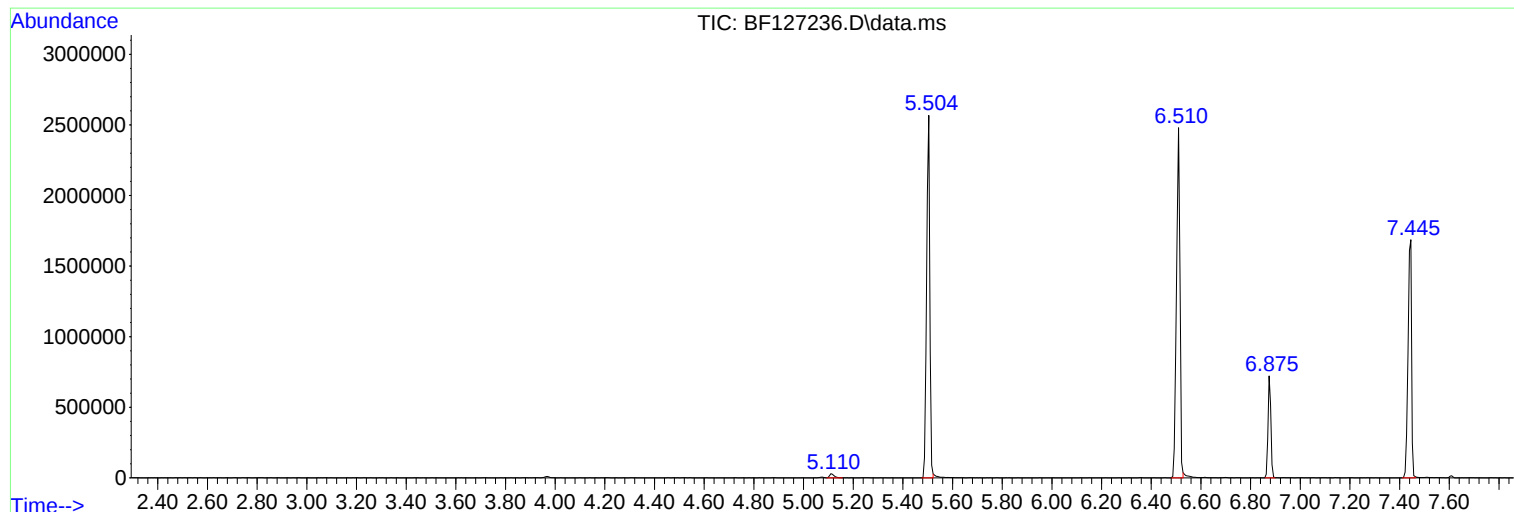

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127236.D
Acq On : 07 Mar 2022 22:52
Operator : CG\JU
Sample : N1806-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUM-25










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.921	3.16 ng	89473	Chrysene-d12	14.057

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	83
2			2,2'-(Ethane-1,2-diylbis(oxy))bi...	358	C20H22O6	1000366-99-4	72
3			1,3-Dioxolane, 2-(methoxymethyl)...	194	C11H14O3	1000156-71-2	64
4			2,3-Dimethyl-4a,8a-diphenyl-hexa...	326	C20H22O4	1000297-07-0	43
5			Benzeneacetic acid, .alpha.-oxo-...	178	C10H10O3	001603-79-8	38

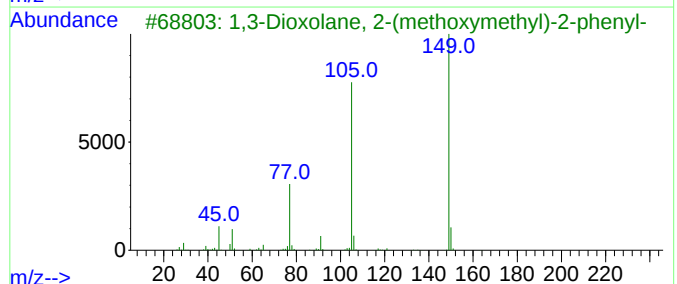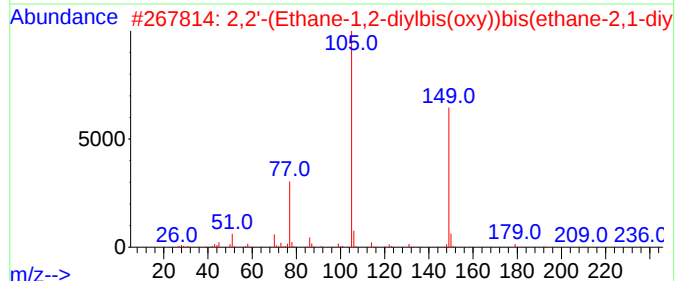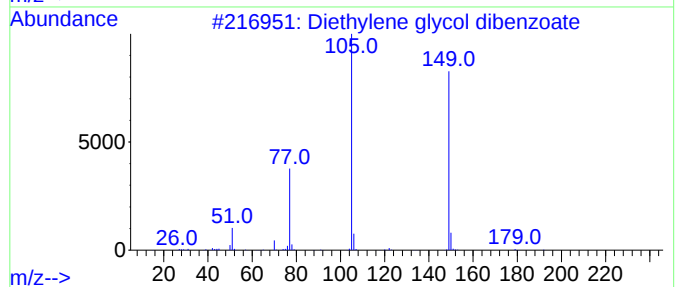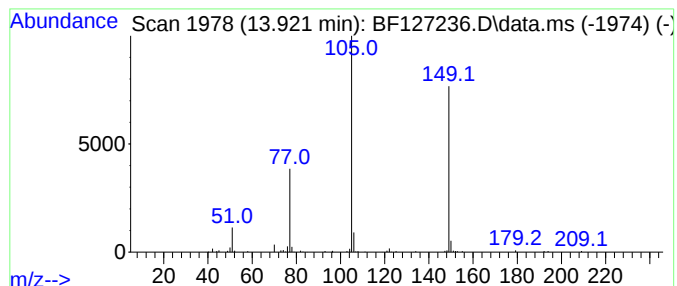

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127236.D
Acq On : 07 Mar 2022 22:52
Operator : CG\JU
Sample : N1806-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUM-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glyc...	13.921	3.2	ng	89473	5	14.057	566204	20.0