

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127247.D
 Acq On : 08 Mar 2022 04:14
 Operator : CG\JU
 Sample : N1808-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-030422

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.940	277	281	287	rVB2	8718	11782	1.25%	0.169%
2	5.493	541	545	557	rBV	527520	463529	49.35%	6.643%
3	6.504	714	717	730	rBV	581146	473355	50.39%	6.784%
4	6.875	777	780	784	rBV	851277	721893	76.85%	10.345%
5	7.440	872	876	879	rBV	396216	315470	33.58%	4.521%
6	8.163	995	999	1002	rBV	1140534	939352	100.00%	13.462%
7	9.234	1177	1181	1184	rBV	768655	563136	59.95%	8.070%
8	9.922	1294	1298	1301	rBV	1076952	901855	96.01%	12.924%
9	10.710	1428	1432	1438	rBV	308632	265776	28.29%	3.809%
10	10.822	1447	1451	1455	rVB5	14740	18441	1.96%	0.264%
11	11.292	1527	1531	1533	rVB2	12393	11205	1.19%	0.161%
12	11.410	1547	1551	1554	rBV	856809	726002	77.29%	10.404%
13	11.433	1554	1555	1558	rVB	18218	12776	1.36%	0.183%
14	11.792	1613	1616	1618	rVB	21373	16511	1.76%	0.237%
15	12.480	1728	1733	1735	rBV4	41688	53020	5.64%	0.760%
16	12.498	1735	1736	1739	rVB3	36652	25751	2.74%	0.369%
17	12.586	1749	1751	1755	rVB4	18502	18717	1.99%	0.268%
18	12.627	1755	1758	1762	rBV	34236	38978	4.15%	0.559%
19	12.857	1794	1797	1801	rBV	46590	46365	4.94%	0.664%
20	12.992	1817	1820	1827	rVB	389416	358206	38.13%	5.133%
21	14.057	1998	2001	2005	rBV	550940	516507	54.99%	7.402%
22	15.557	2252	2256	2263	rVB	382299	479337	51.03%	6.869%




Sum of corrected areas: 6977964

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127247.D
Acq On : 08 Mar 2022 04:14
Operator : CG\JU
Sample : N1808-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-030422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

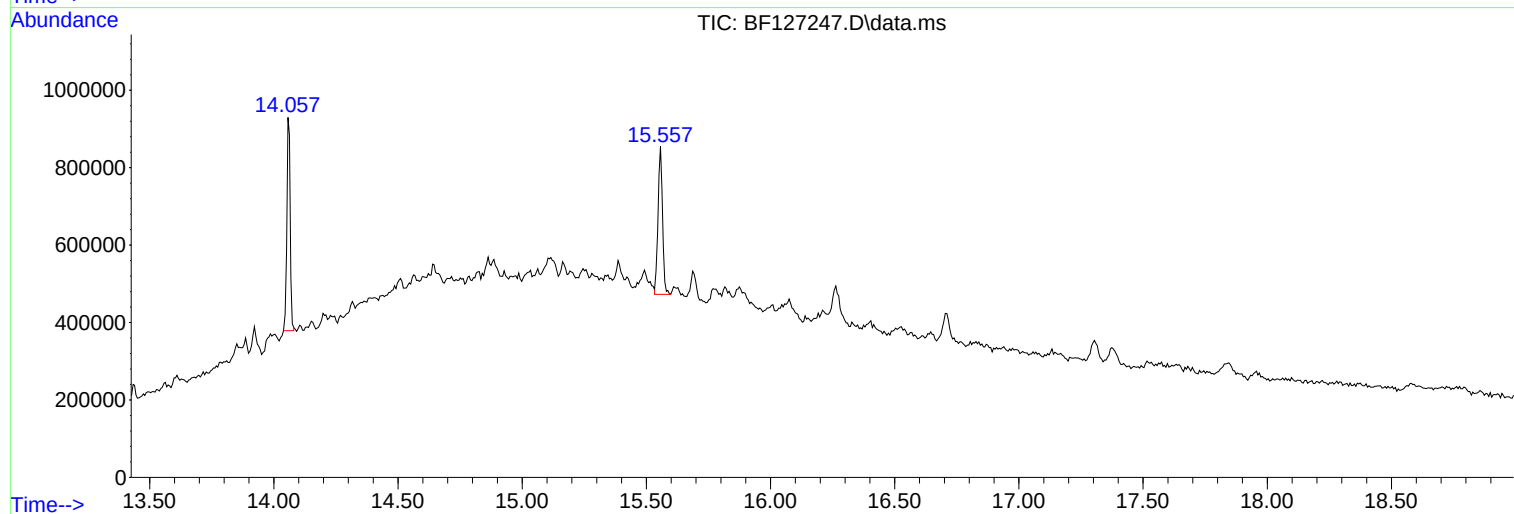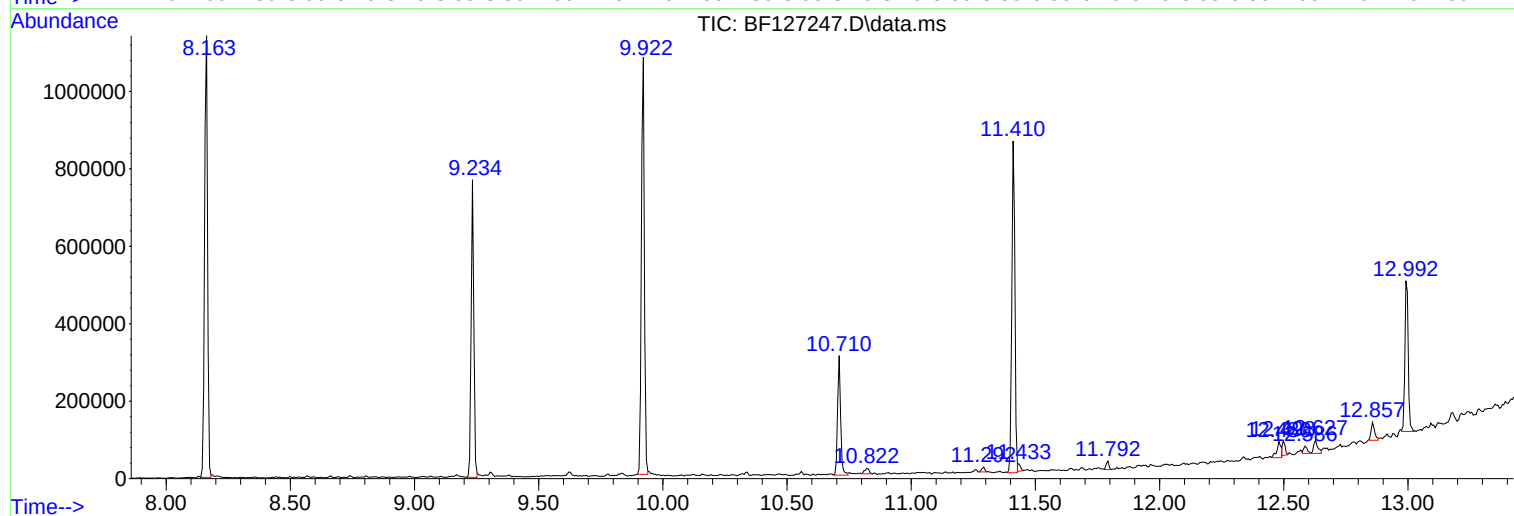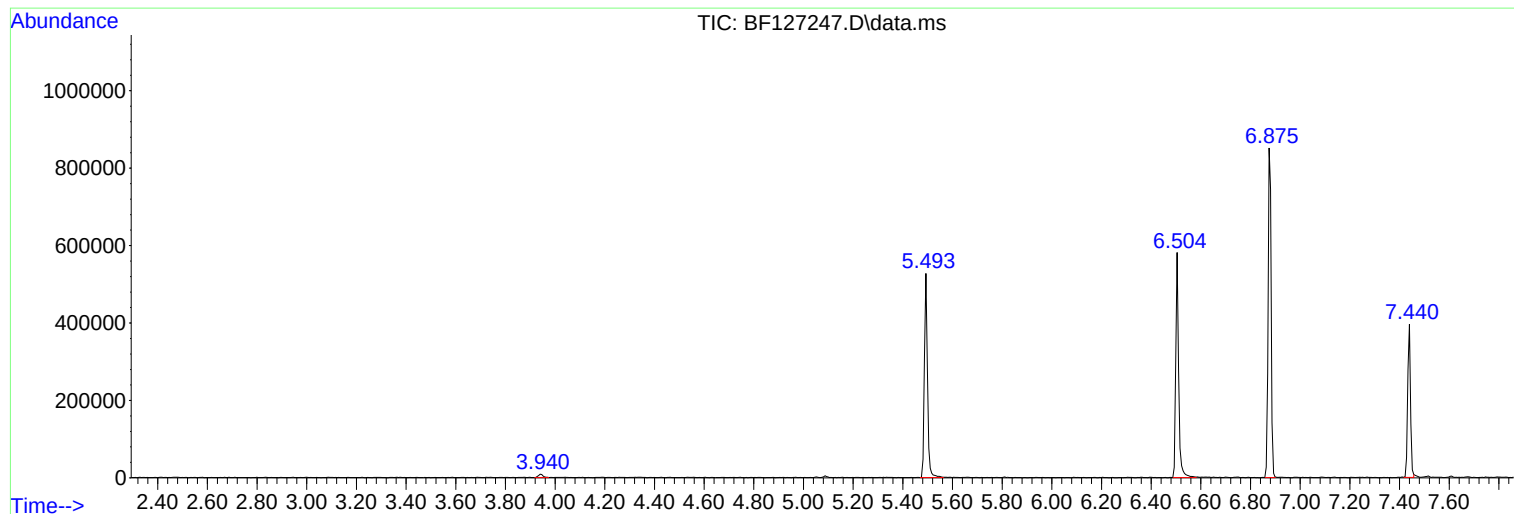

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127247.D
Acq On : 08 Mar 2022 04:14
Operator : CG\JU
Sample : N1808-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-030422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127247.D
Acq On : 08 Mar 2022 04:14
Operator : CG\JU
Sample : N1808-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-030422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------