
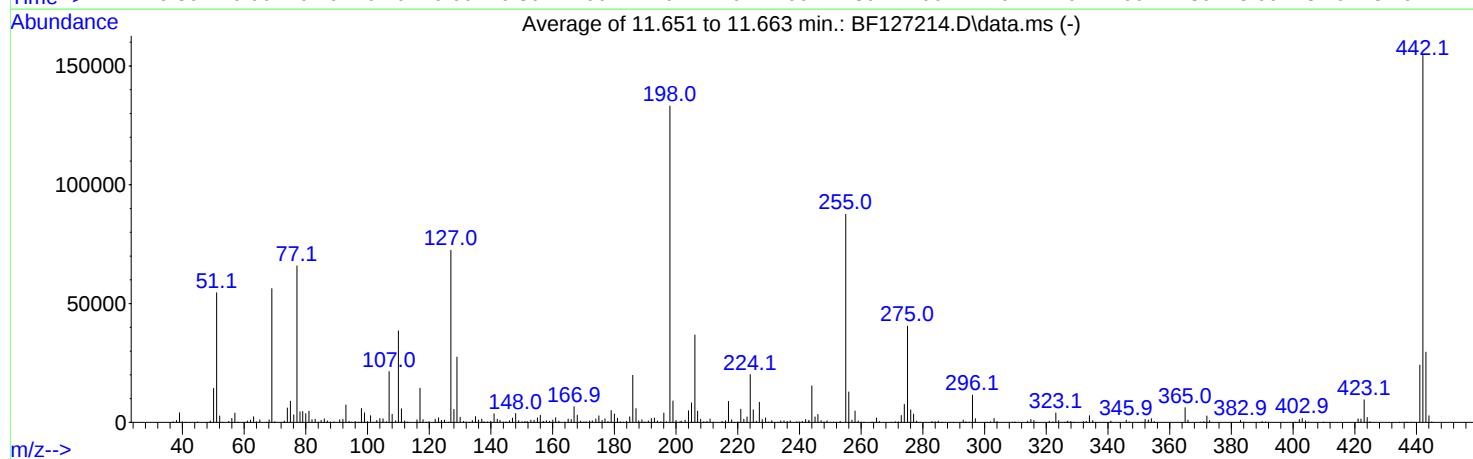


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127214.D
 Acq On : 07 Mar 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 02:16:58 2022

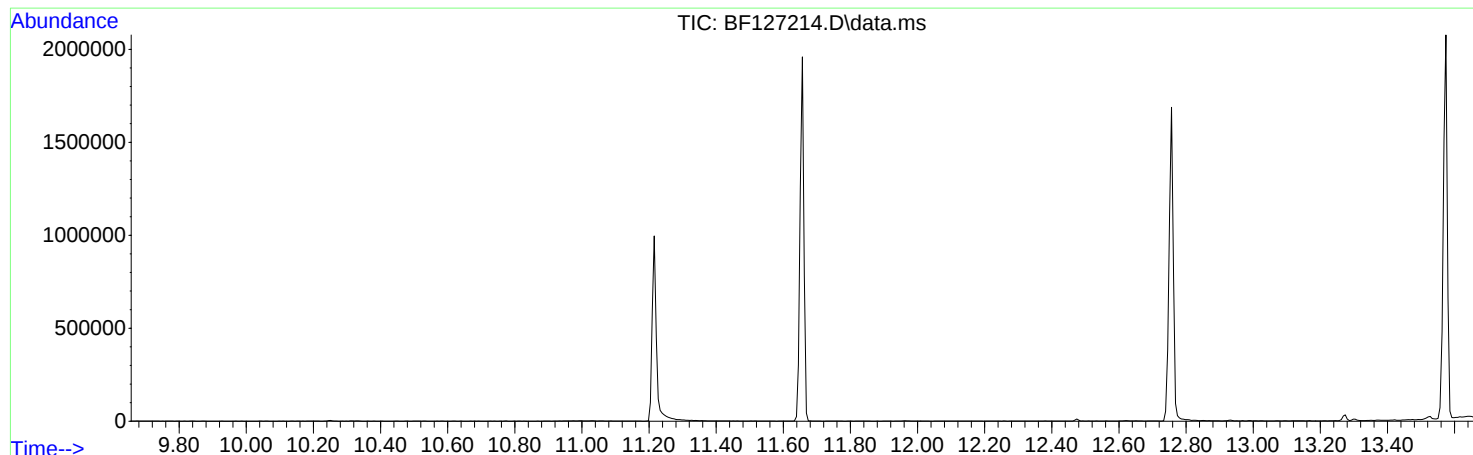




AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	54576	PASS
68	69	0.00	2	1.9	1072	PASS
69	198	0.00	100	42.3	56339	PASS
70	69	0.00	2	0.5	306	PASS
127	198	10	80	54.4	72485	PASS
197	198	0.00	2	0.2	263	PASS
198	198	100	100	100.0	133144	PASS
199	198	5	9	6.8	9000	PASS
275	198	10	60	30.4	40499	PASS
365	198	1	100	4.7	6195	PASS
441	198	0.01	100	18.1	24128	PASS
442	442	50	100	100.0	154840	PASS
443	442	15	24	19.1	29561	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127214.D
Acq On : 07 Mar 2022 09:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 16:31:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 02:16:58 2022
Response via : Initial Calibration

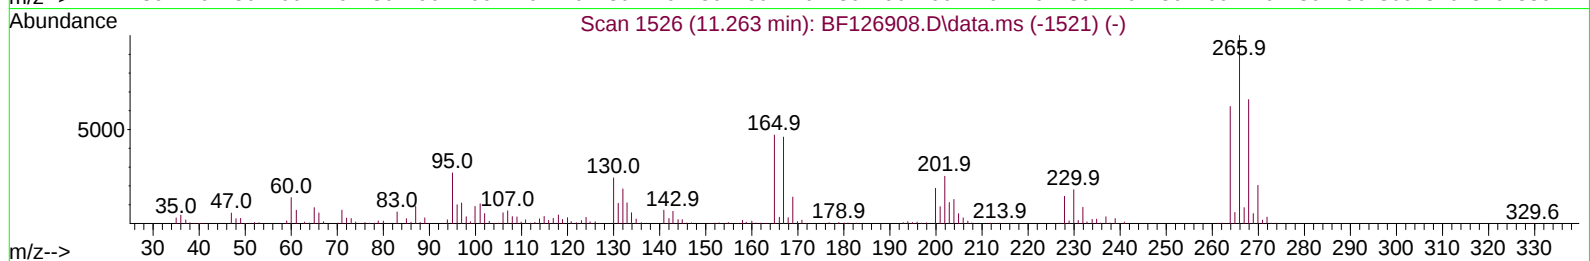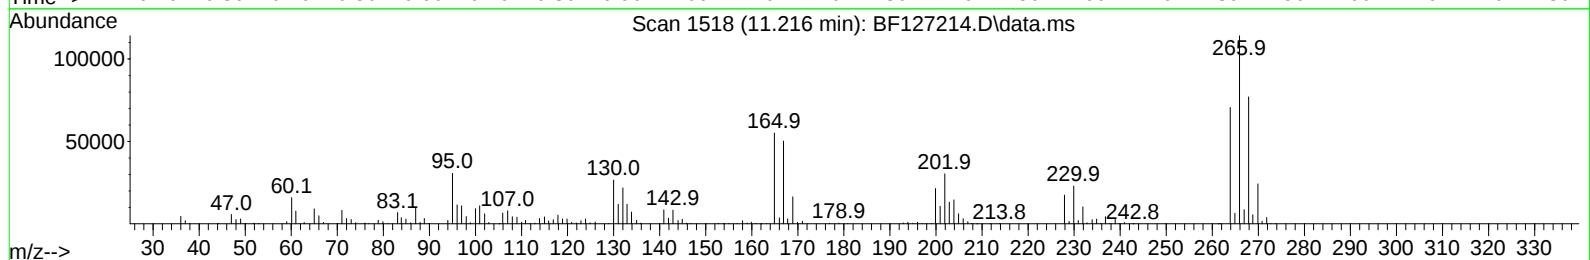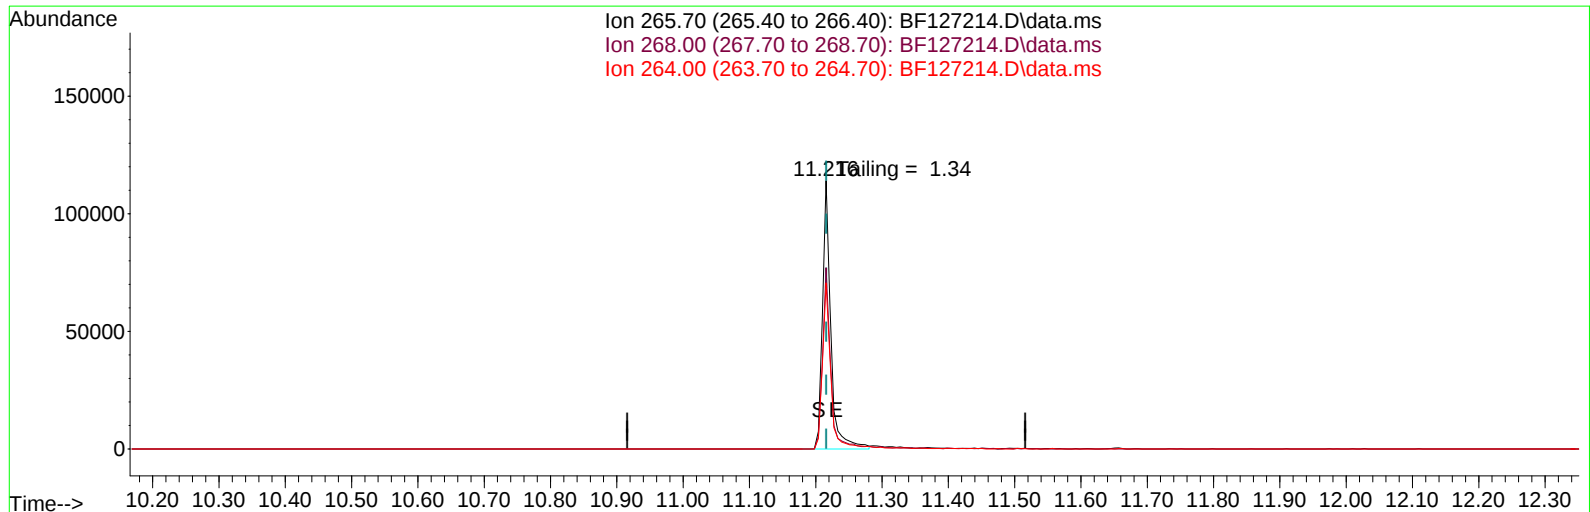

TIC: BF127214.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 18920.19 ng




response 103980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	67.50
264.00	63.00	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127214.D
 Acq On : 07 Mar 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 07 16:31:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 02:16:58 2022
 Response via : Initial Calibration

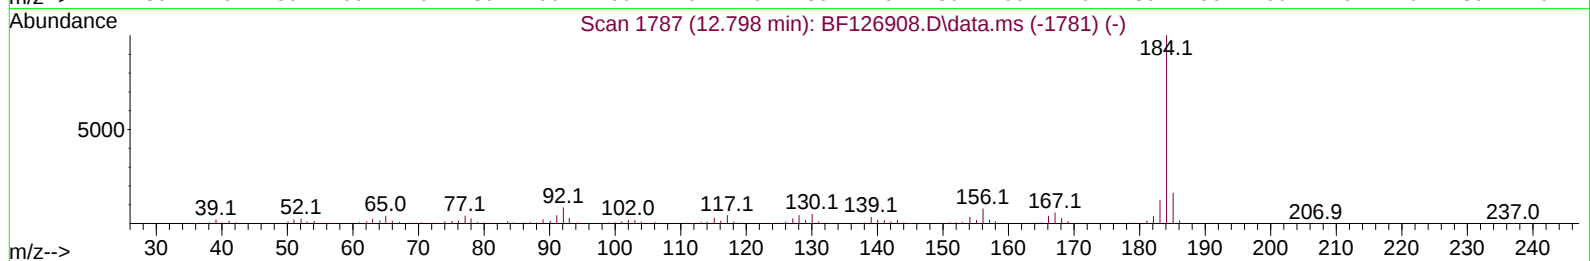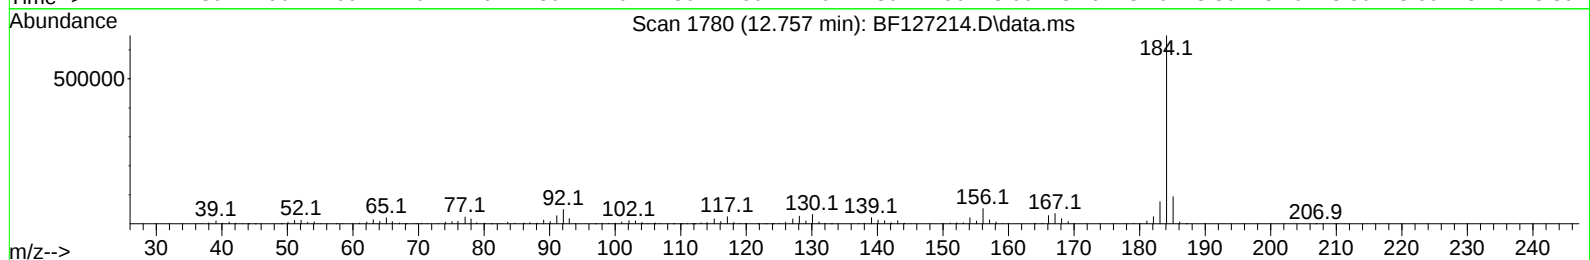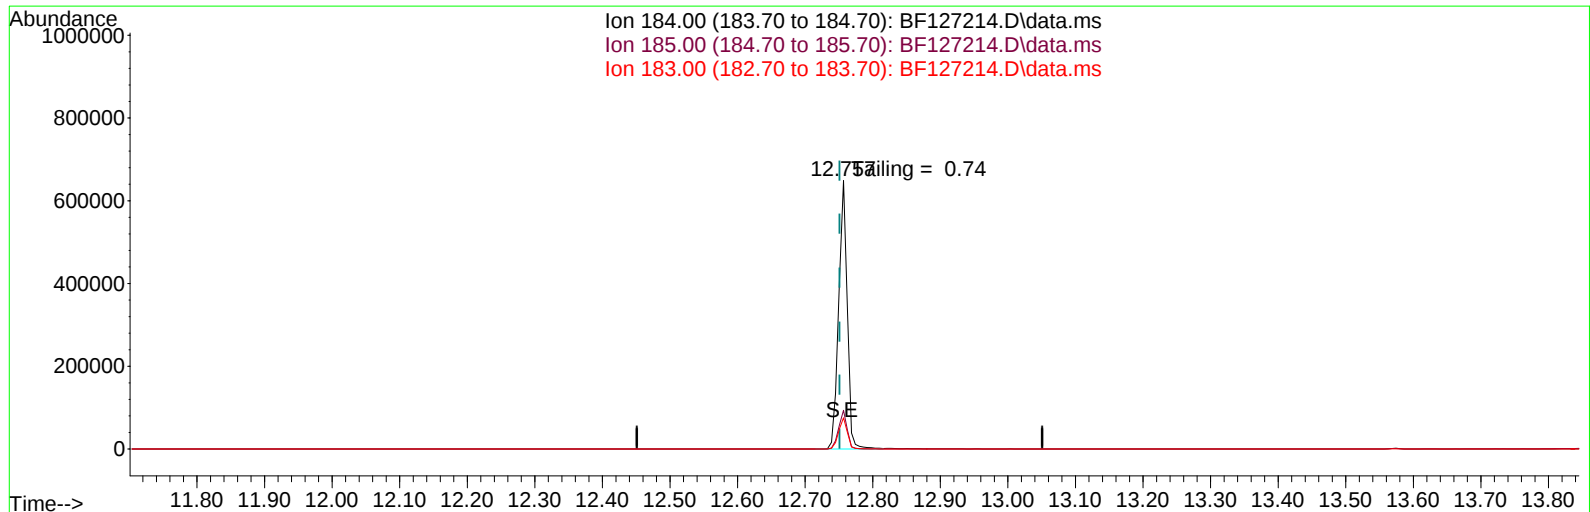

TIC: BF127214.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 572557

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.43
183.00	10.20	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2022	BNA_F	<u>BF127214.D</u>
Compound Name	Response	Retention Time
DDT	306617	13.57
DDD	5228	13.27
DDE	416	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5644	312261	1.81

Instrument :
BNA_F
ClientSampleId :
DFTPP