


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127225.D
 Acq On : 07 Mar 2022 17:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 02:16:58 2022

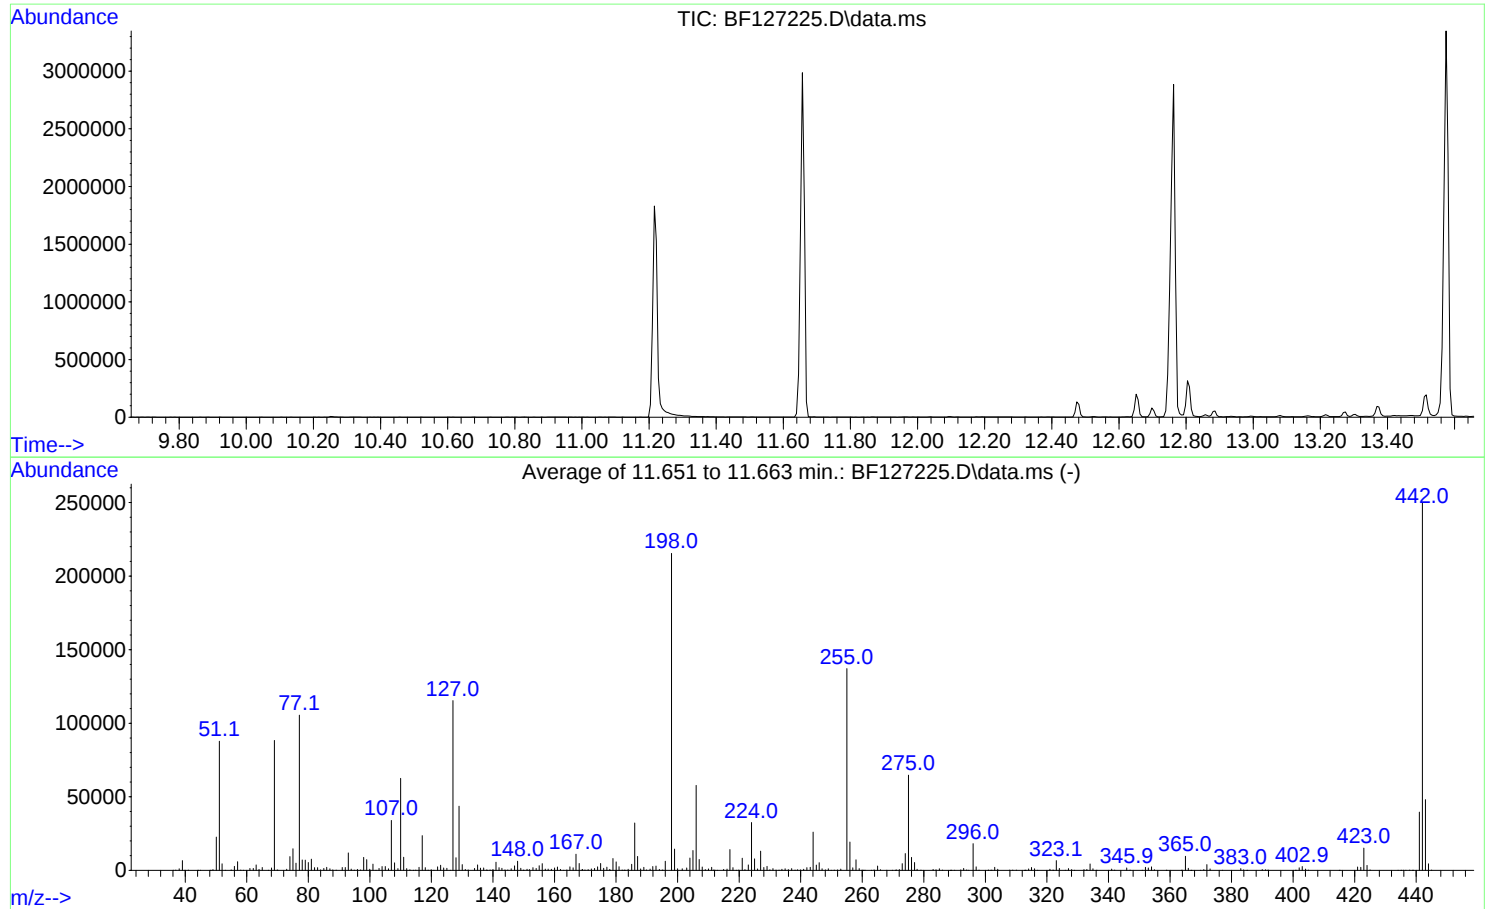


AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	87771	PASS
68	69	0.00	2	1.8	1618	PASS
69	198	0.00	100	41.0	88347	PASS
70	69	0.00	2	0.4	316	PASS
127	198	10	80	53.5	115352	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	215488	PASS
199	198	5	9	6.7	14475	PASS
275	198	10	60	30.0	64741	PASS
365	198	1	100	4.4	9560	PASS
441	198	0.01	100	18.4	39631	PASS
442	442	50	100	100.0	250043	PASS
443	442	15	24	19.2	48133	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
 Data File : BF127225.D
 Acq On : 07 Mar 2022 17:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 08 05:20:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 02:16:58 2022
 Response via : Initial Calibration

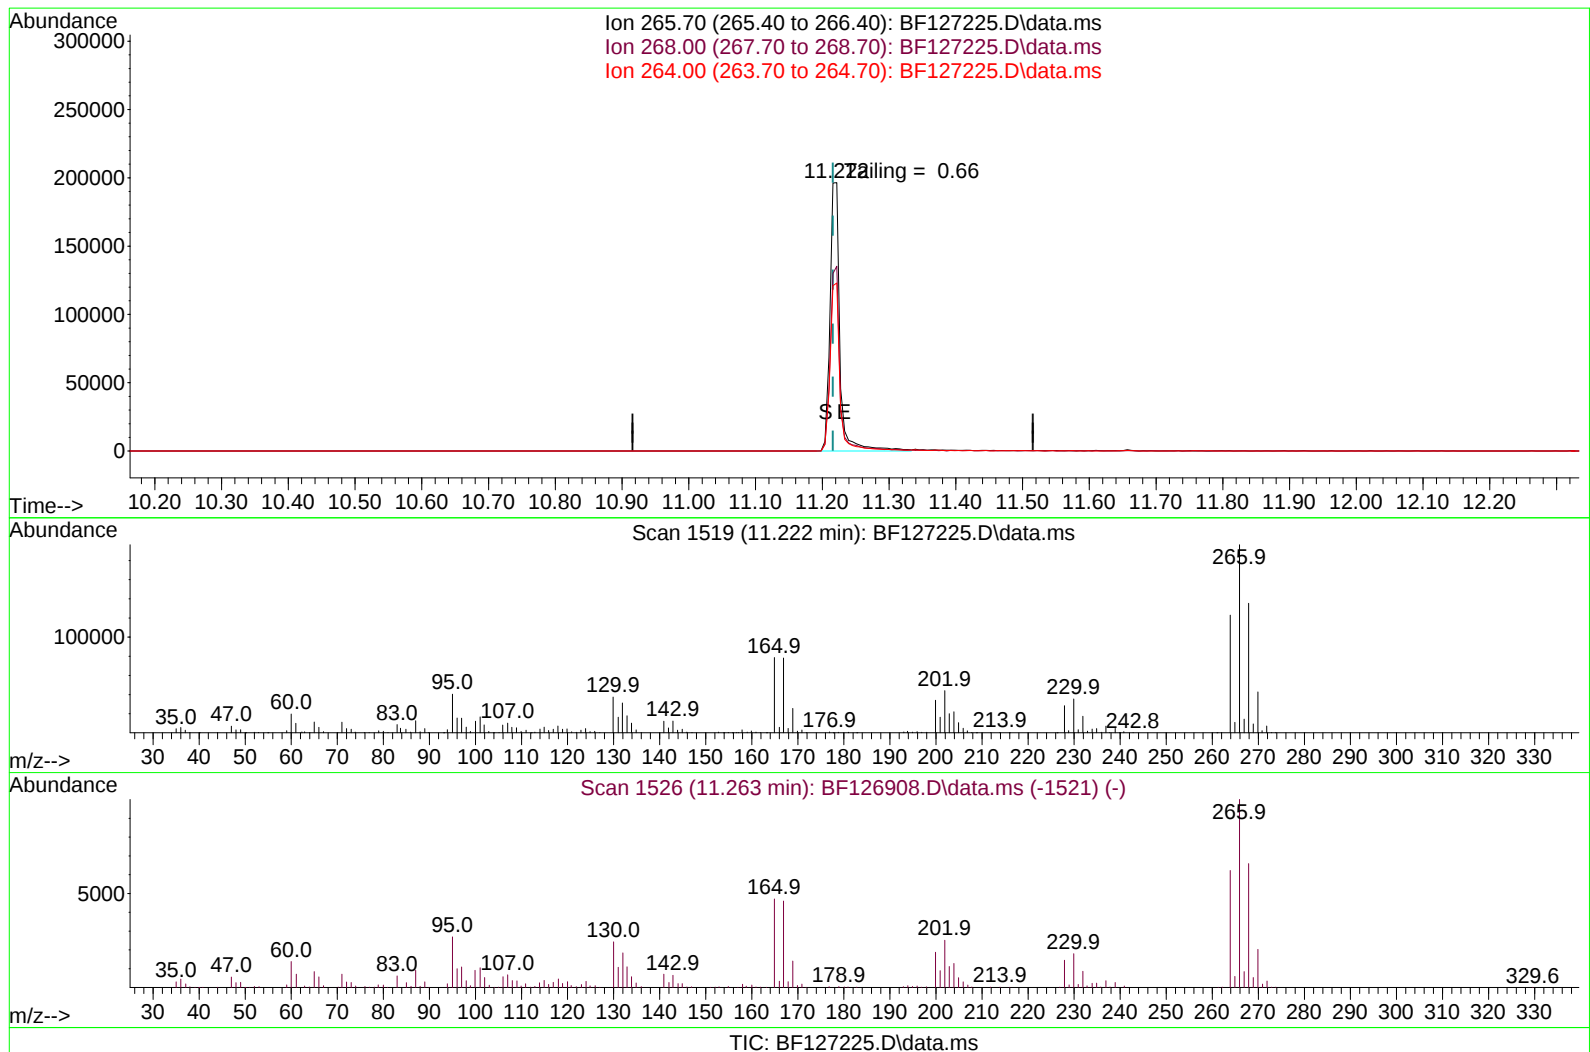

TIC: BF127225.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 26546.32 ng




response 204108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	68.89
264.00	63.00	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030722\
Data File : BF127225.D
Acq On : 07 Mar 2022 17:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 08 05:20:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 02:16:58 2022
Response via : Initial Calibration

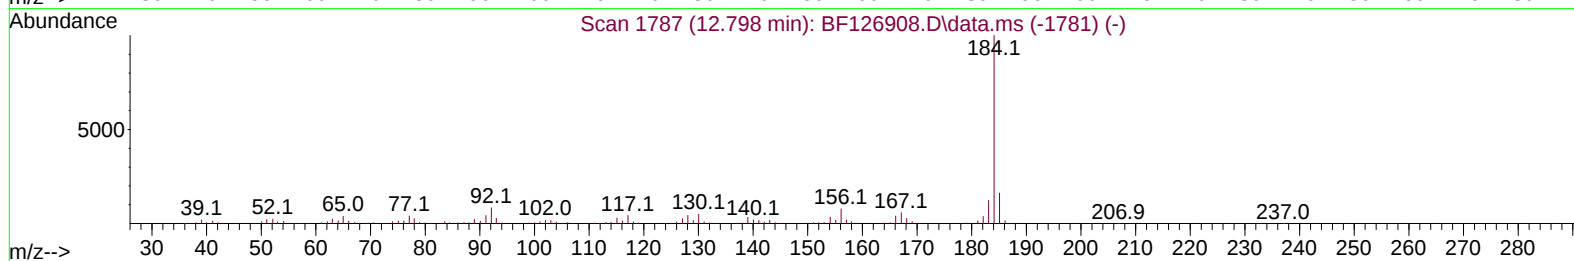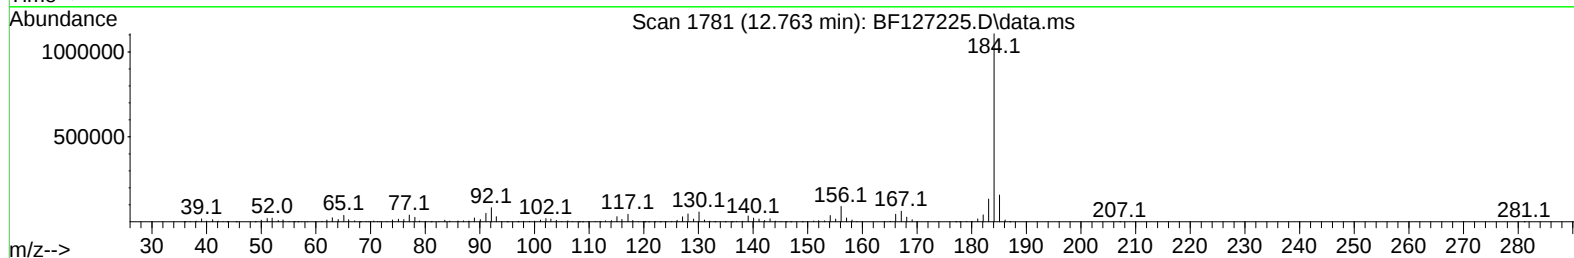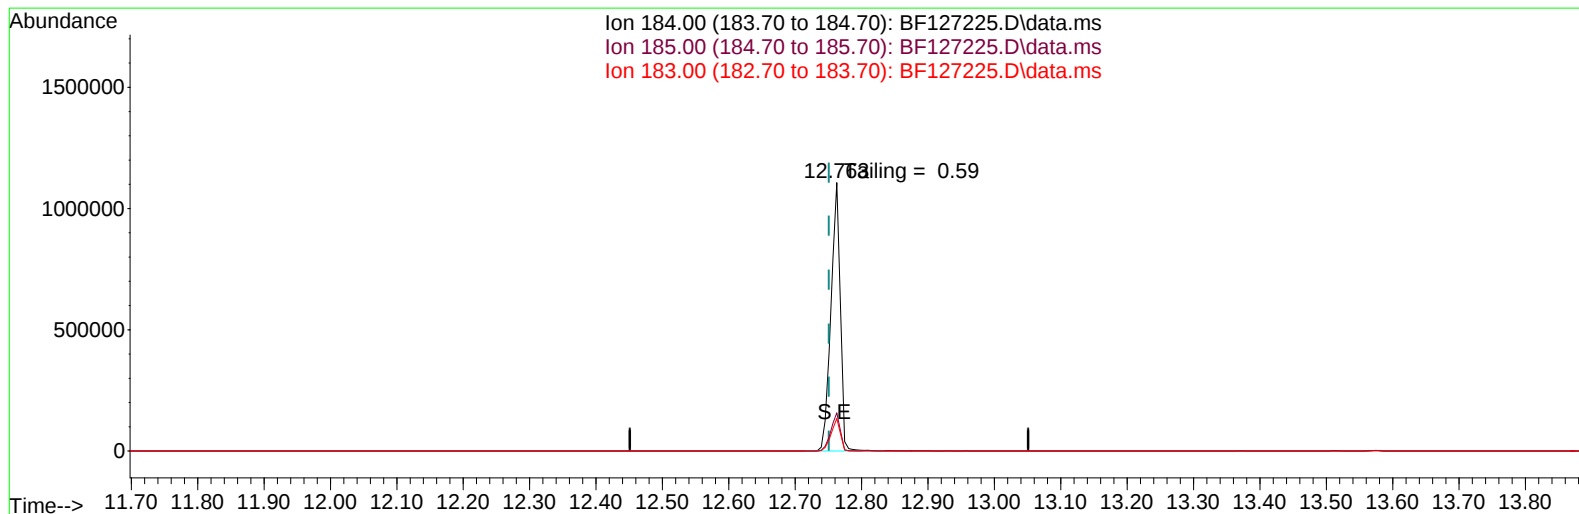

TIC: BF127225.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng

response 1091214

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.25
183.00	10.20	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2022	BNA_F	<u>BF127225.D</u>
Compound Name	Response	Retention Time
DDT	544452	13.574
DDD	10600	13.274
DDE	563	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11163	555615	2.01

Instrument :
BNA_F
ClientSampleId :
DFTPP