
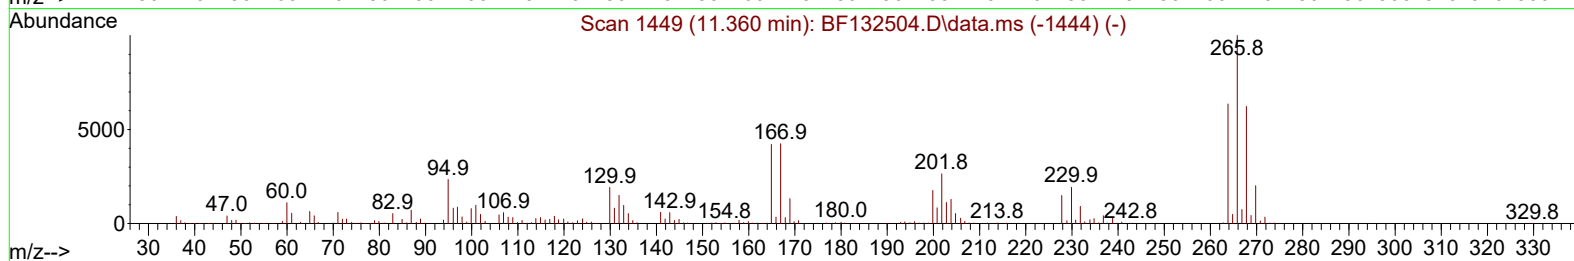
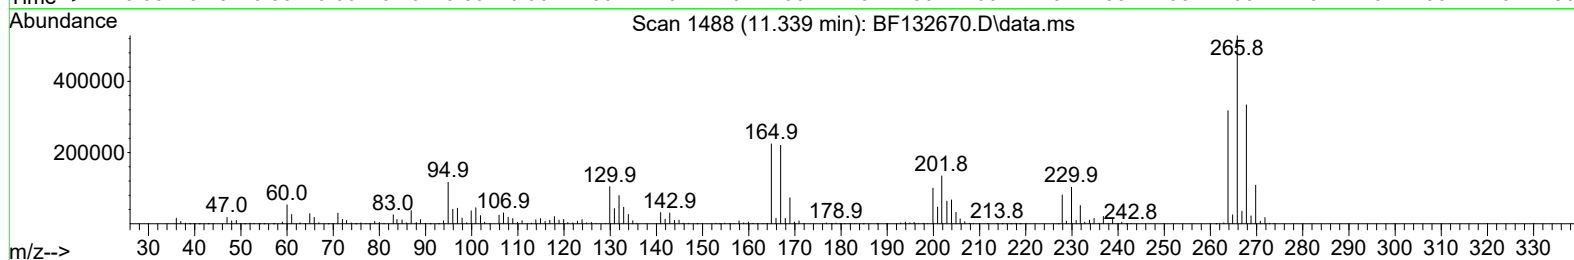


Quant Time: Mar 08 06:47:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 13:42:31 2023
Response via : Initial Calibration

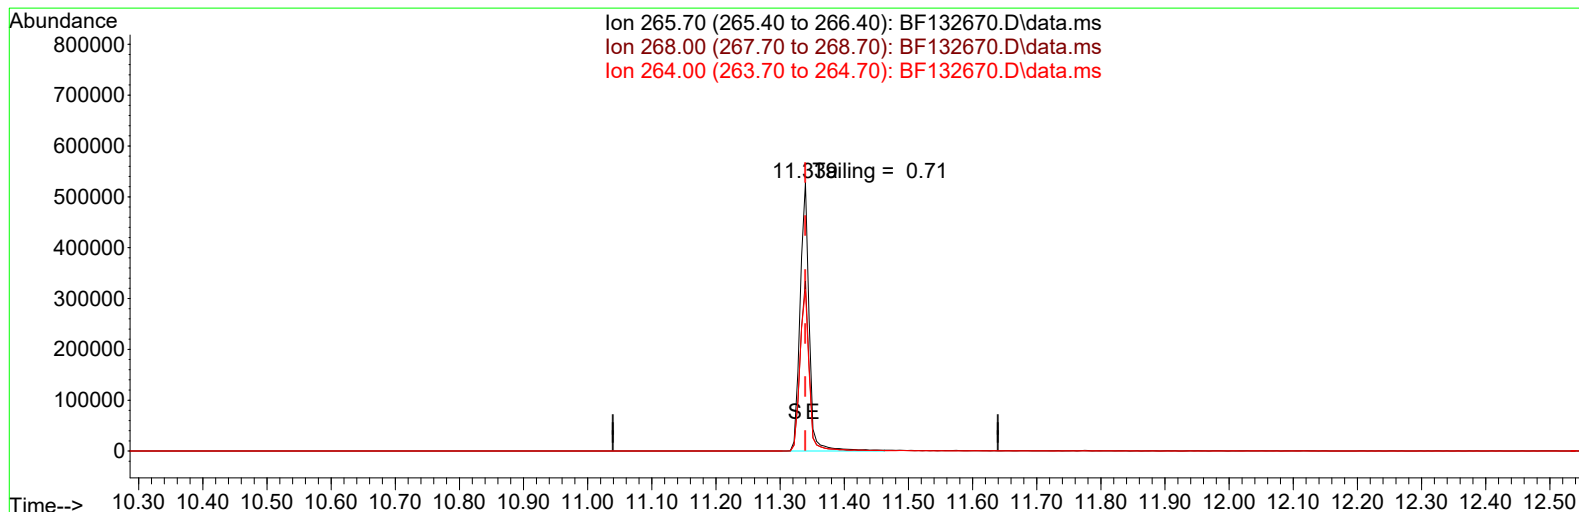

TIC: BF132670.D\data.ms

(70) Pentachlorophenol (C)




11.339min (0.000) 405503.65 ng

response **528370**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.28
264.00	63.60	60.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
Data File : BF132670.D
Acq On : 07 Mar 2023 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 06:47:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 13:42:31 2023
Response via : Initial Calibration

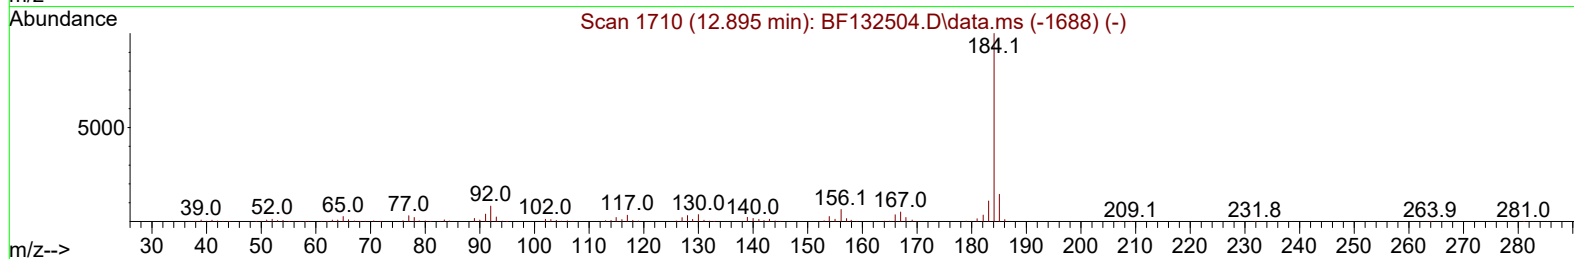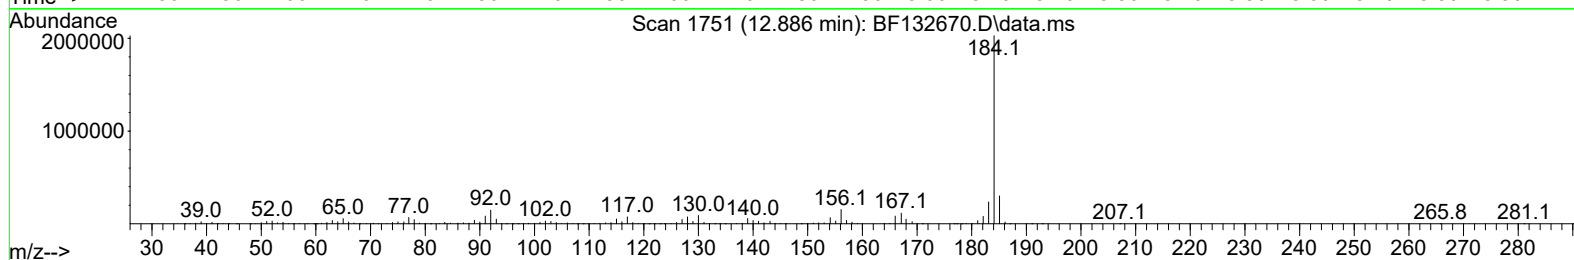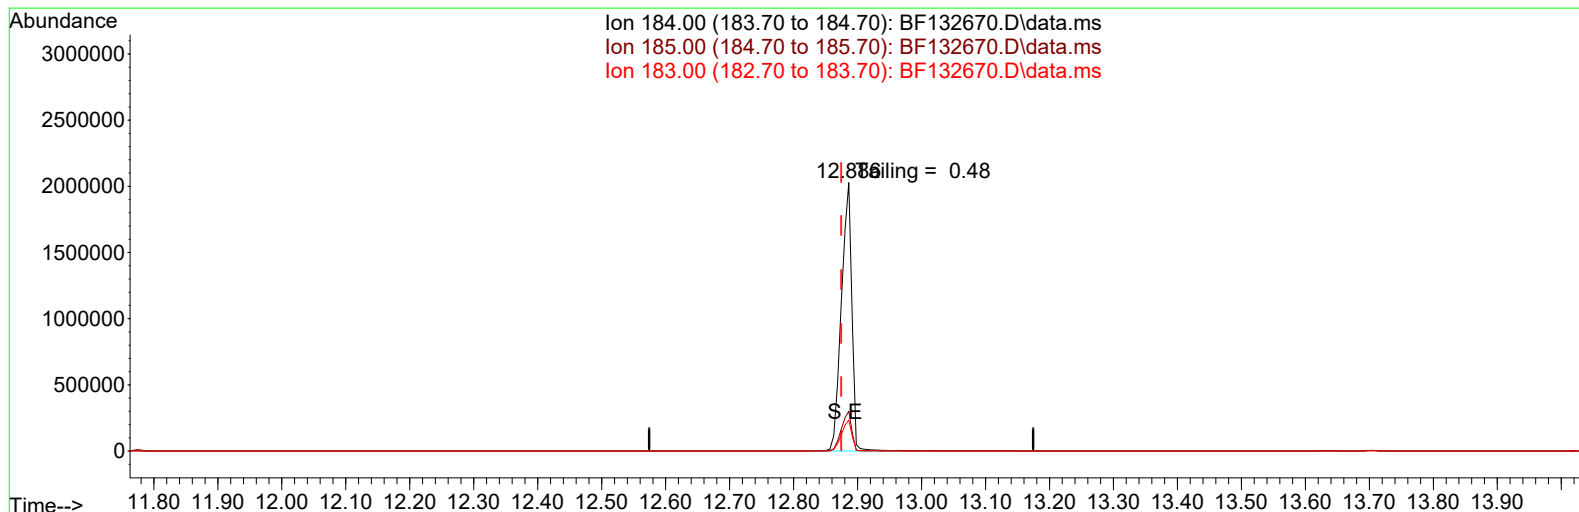

TIC: BF132670.D\data.ms

(77) Benzidine**12.886min (+ 0.012) 1463249.67 ng****response 2315279**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.79
183.00	10.90	11.58
0.00	0.00	0.00