

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
 Data File : BF132672.D
 Acq On : 07 Mar 2023 11:28
 Operator : CG\JU
 Sample : PB151052BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB151052BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	444	450	462	rBV	1557247	2524880	36.60%	5.928%
2	5.628	512	517	520	rBV	4684771	5012885	72.67%	11.769%
3	6.622	680	686	689	rBV	4283938	5040576	73.07%	11.834%
4	6.987	745	748	752	rBV	1425845	1184076	17.17%	2.780%
5	7.557	839	845	848	rBV	3377629	3435917	49.81%	8.066%
6	8.275	963	967	970	rBV	1934544	1568032	22.73%	3.681%
7	9.351	1144	1150	1153	rBV	6287559	5961629	86.42%	13.996%
8	10.033	1263	1266	1270	rVB	2200714	1892893	27.44%	4.444%
9	10.833	1397	1402	1405	rBV	4297145	4104389	59.50%	9.636%
10	11.533	1517	1521	1524	rBV	2319456	2050315	29.72%	4.813%
11	13.127	1787	1792	1795	rBV	6749745	6898102	100.00%	16.195%
12	13.633	1874	1878	1882	rBV2	76773	73228	1.06%	0.172%
13	14.192	1968	1973	1976	rBV	1620071	1605107	23.27%	3.768%
14	15.739	2230	2236	2246	rBV	917155	1243228	18.02%	2.919%




Sum of corrected areas: 42595257

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
Data File : BF132672.D
Acq On : 07 Mar 2023 11:28
Operator : CG\JU
Sample : PB151052BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151052BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

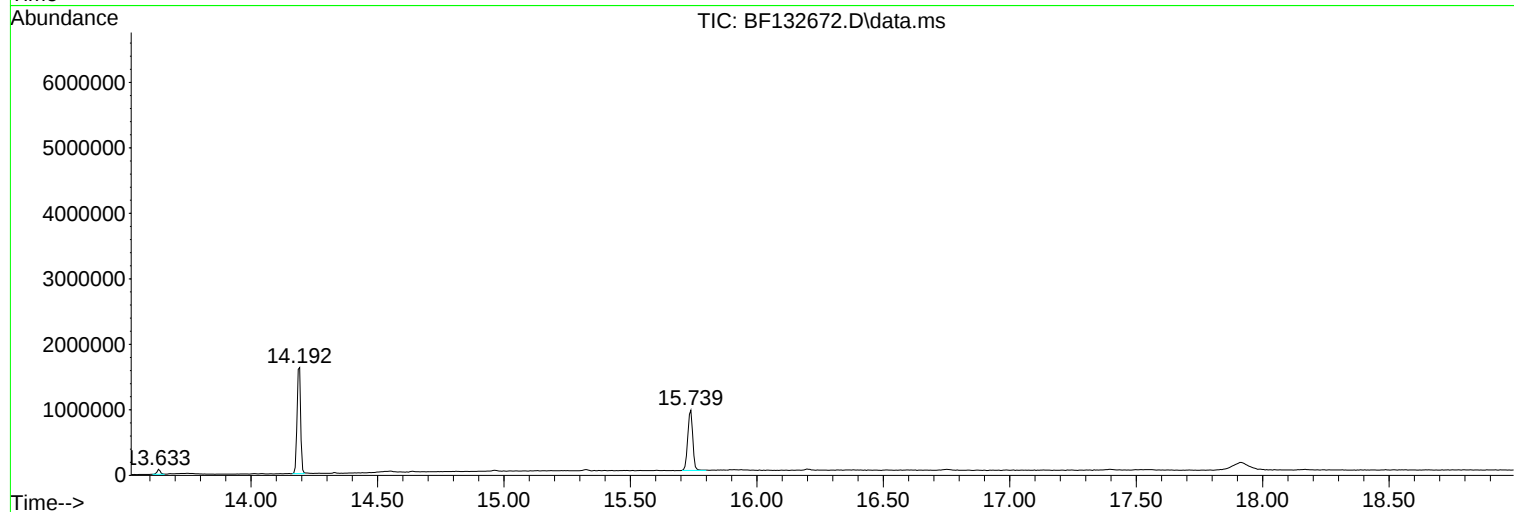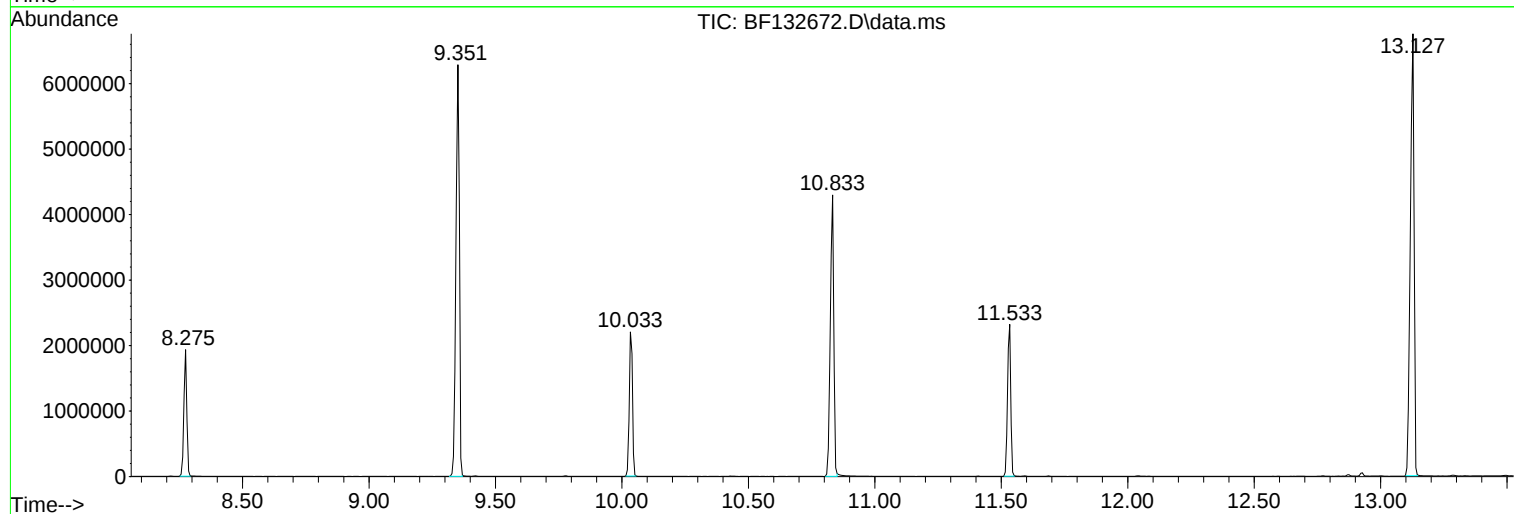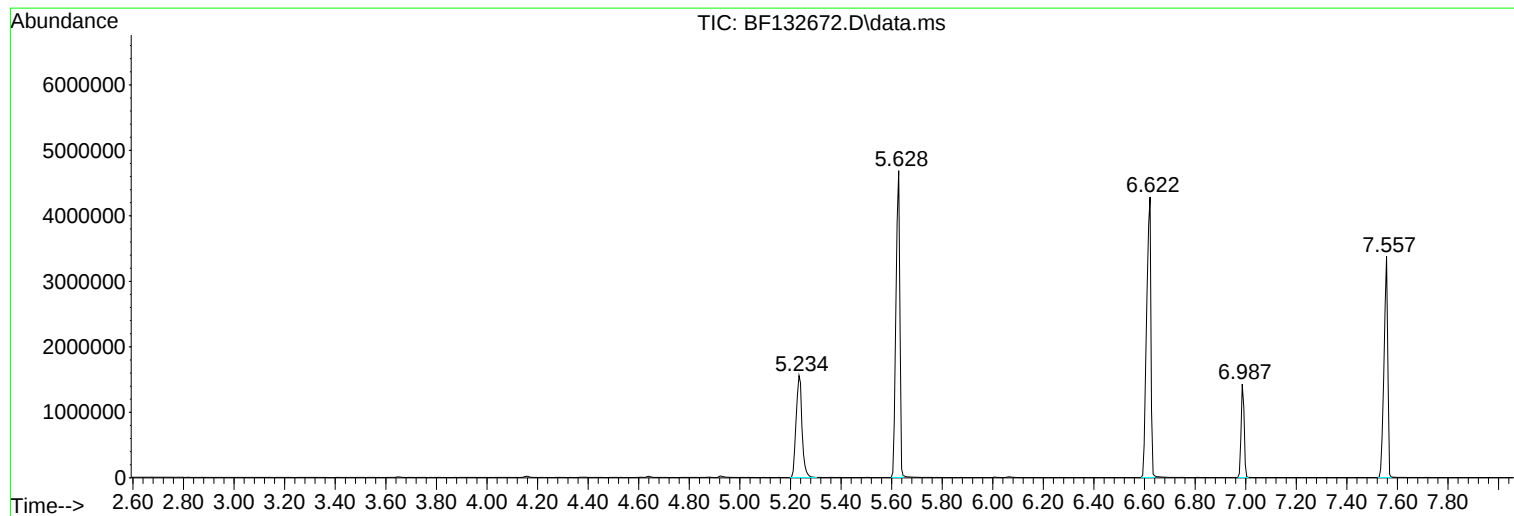

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
Data File : BF132672.D
Acq On : 07 Mar 2023 11:28
Operator : CG\JU
Sample : PB151052BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151052BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.234	42.65 ng	2524880	1,4-Dichlorobenzene-d4	6.987

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
4	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

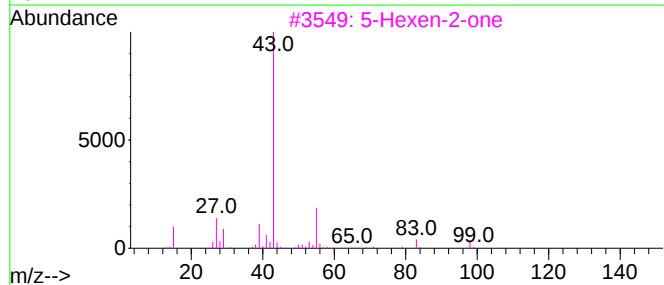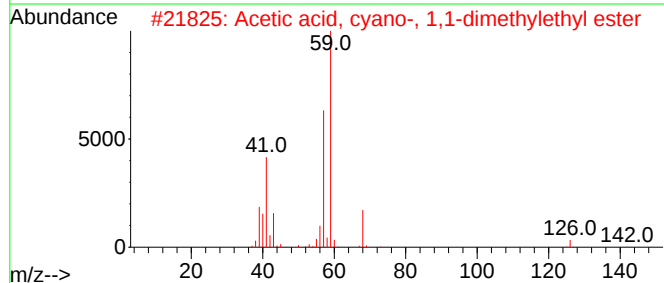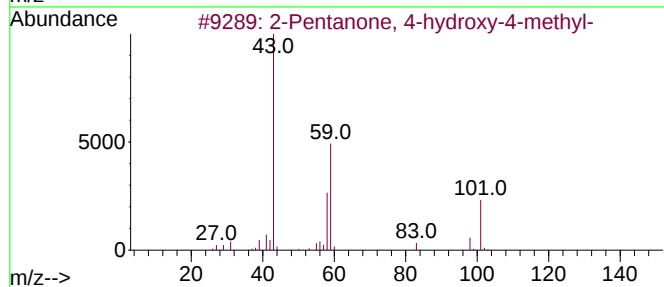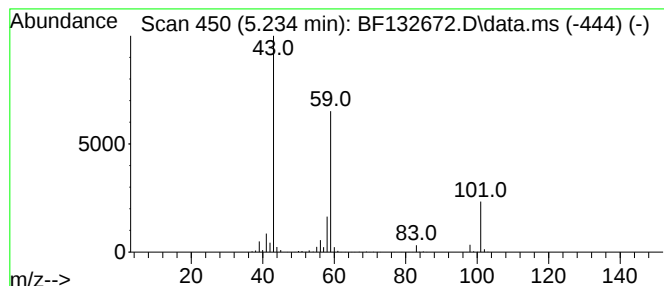

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
Data File : BF132672.D
Acq On : 07 Mar 2023 11:28
Operator : CG\JU
Sample : PB151052BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151052BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.234	42.6	ng	2524880	1	6.987	1184080	20.0