
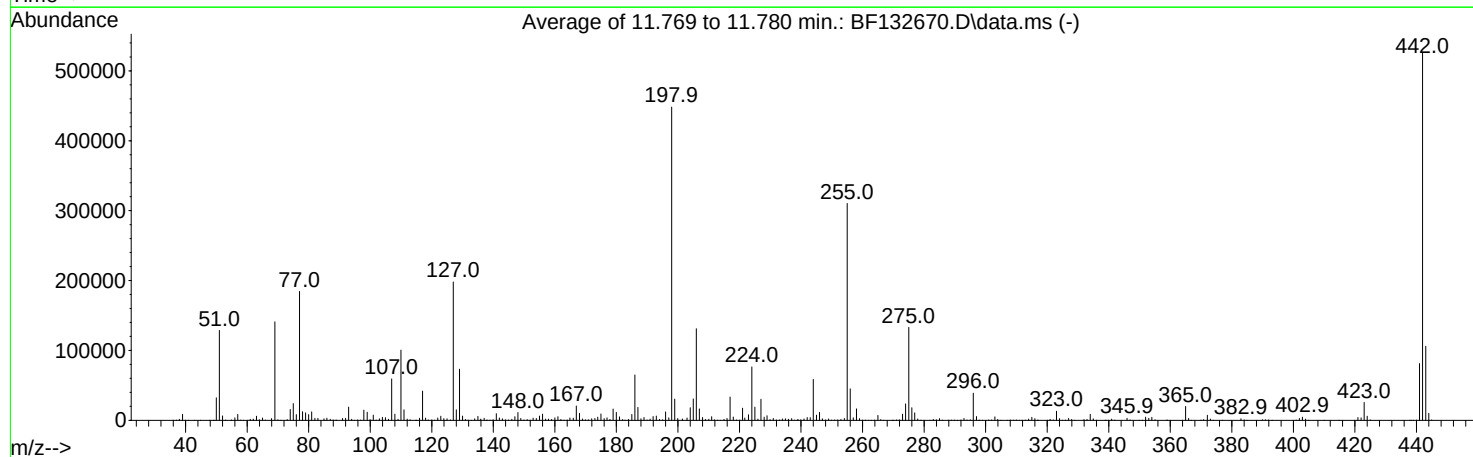


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
Data File : BF132670.D
Acq On : 07 Mar 2023 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 07 13:42:31 2023

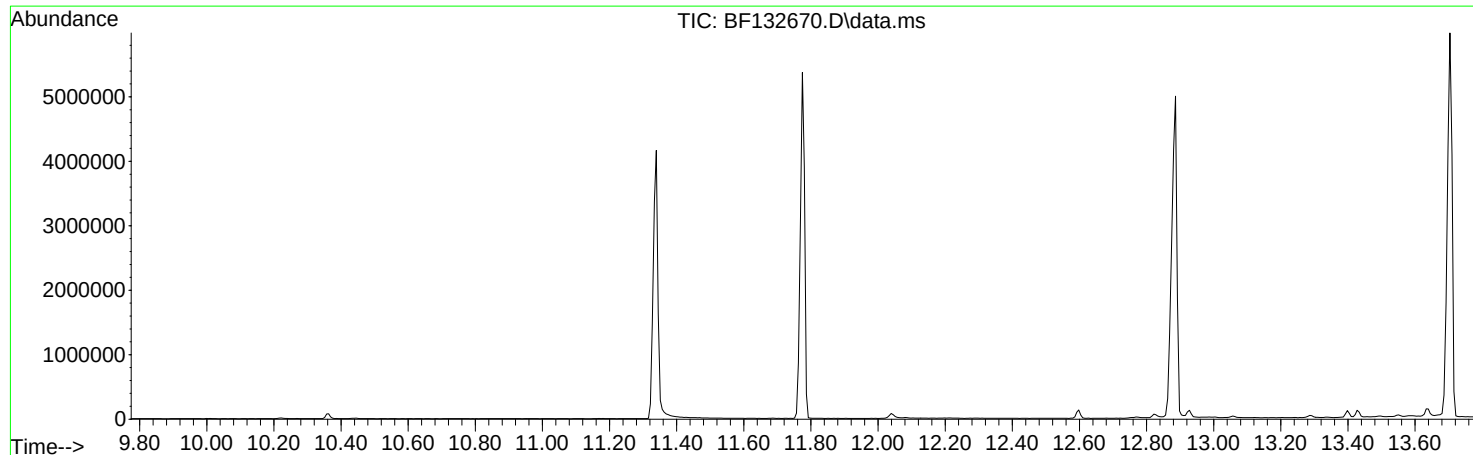




AutoFind: Scans 1561, 1562, 1563; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	128564	PASS
68	69	0.00	2	1.7	2463	PASS
69	198	0.00	100	31.4	140867	PASS
70	69	0.00	2	0.6	836	PASS
127	198	10	80	44.2	197995	PASS
197	198	0.00	2	0.8	3523	PASS
198	198	100	100	100.0	448128	PASS
199	198	5	9	6.8	30341	PASS
275	198	10	60	29.7	133011	PASS
365	198	1	100	4.4	19722	PASS
441	198	0.01	100	18.1	81104	PASS
442	442	50	100	100.0	526443	PASS
443	442	15	24	20.1	105920	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
 Data File : BF132670.D
 Acq On : 07 Mar 2023 10:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 08 06:47:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 13:42:31 2023
 Response via : Initial Calibration

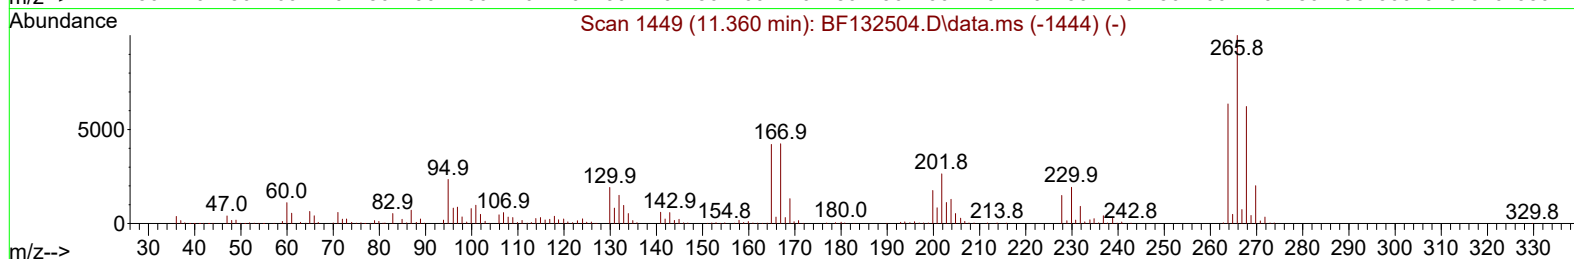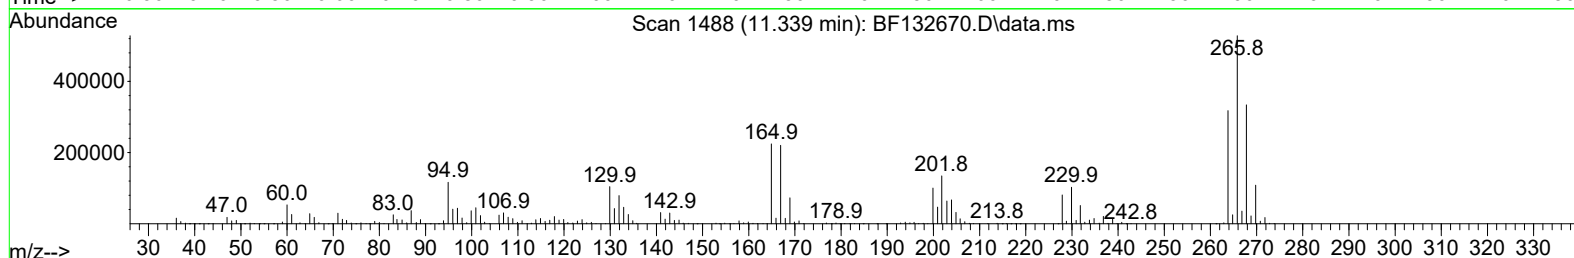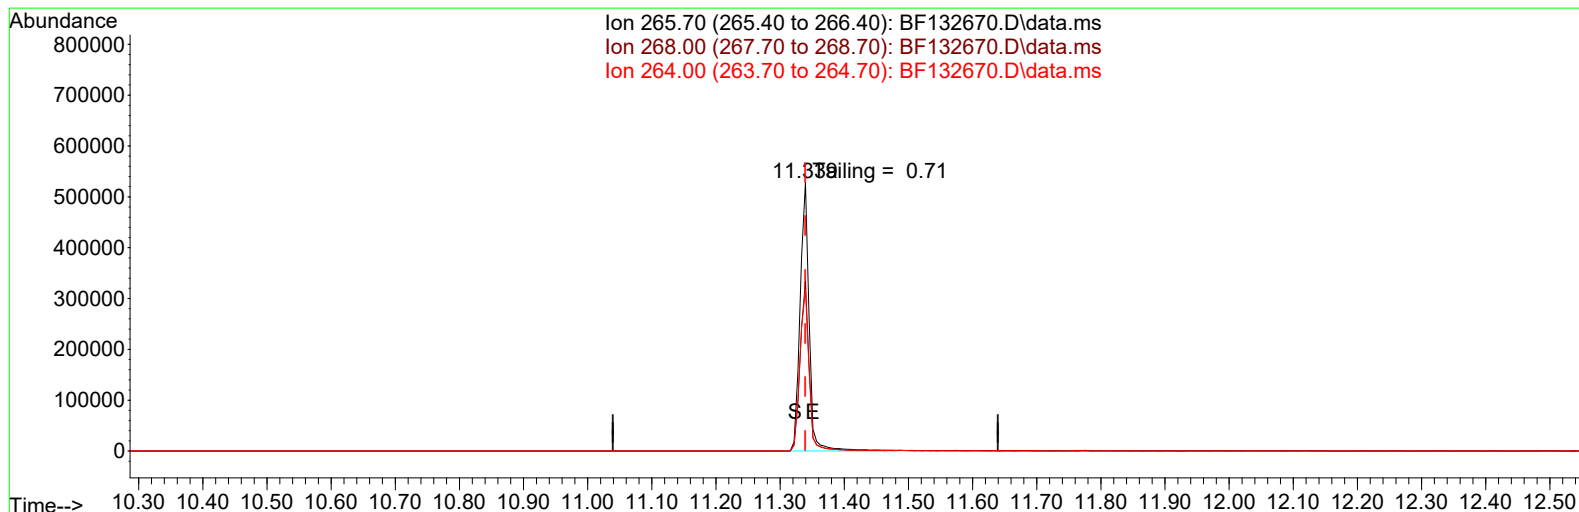

TIC: BF132670.D\data.ms

(70) Pentachlorophenol (C)

11.339min (0.000) 405503.65 ng




response 528370

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.28
264.00	63.60	60.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030723\
Data File : BF132670.D
Acq On : 07 Mar 2023 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 08 06:47:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 13:42:31 2023
Response via : Initial Calibration

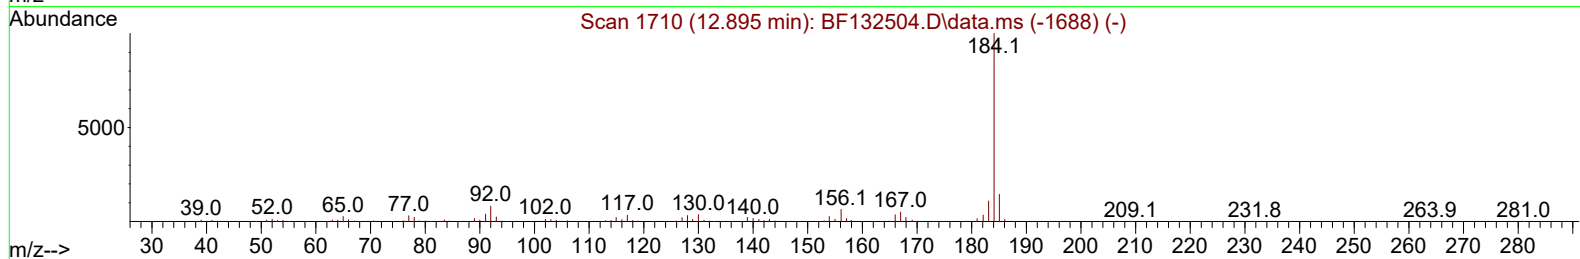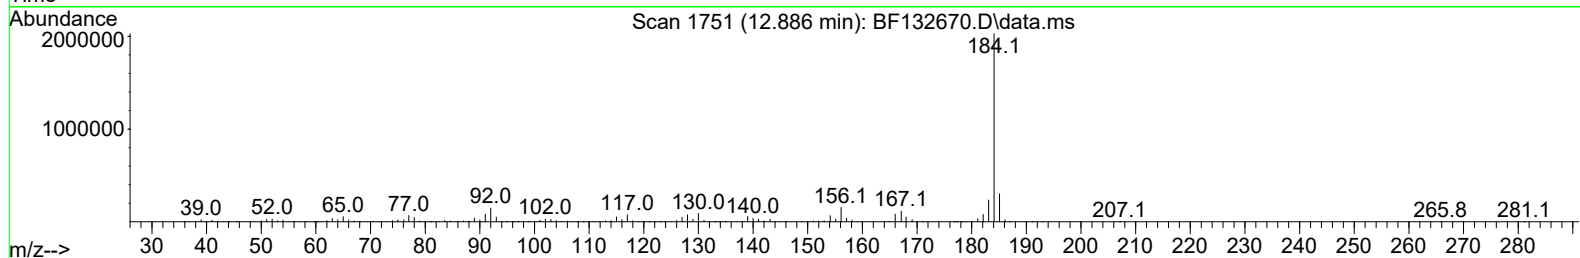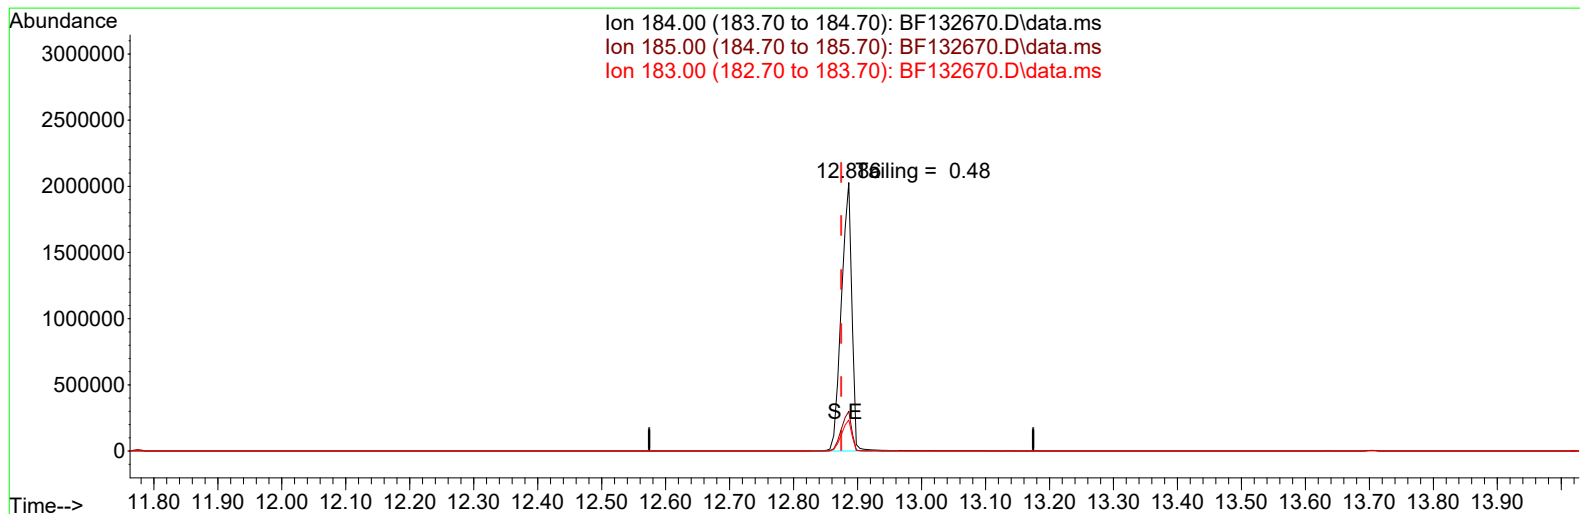

TIC: BF132670.D\data.ms

(77) Benzidine

12.886min (+ 0.012) 1463249.67 ng

response 2315279

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.79
183.00	10.90	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2023	BNA_F	<u>BF132670.D</u>
Compound Name	Response	Retention Time
DDT	1217188	13.704
DDD	35899	13.398
DDE	4207	13.057
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40106	1257294	3.19

Instrument :
BNA_F
ClientSampleId :
DFTPP