
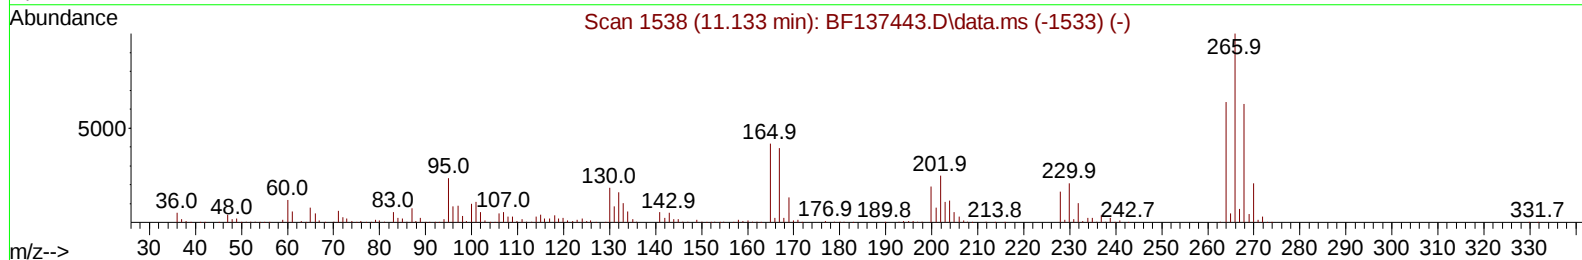
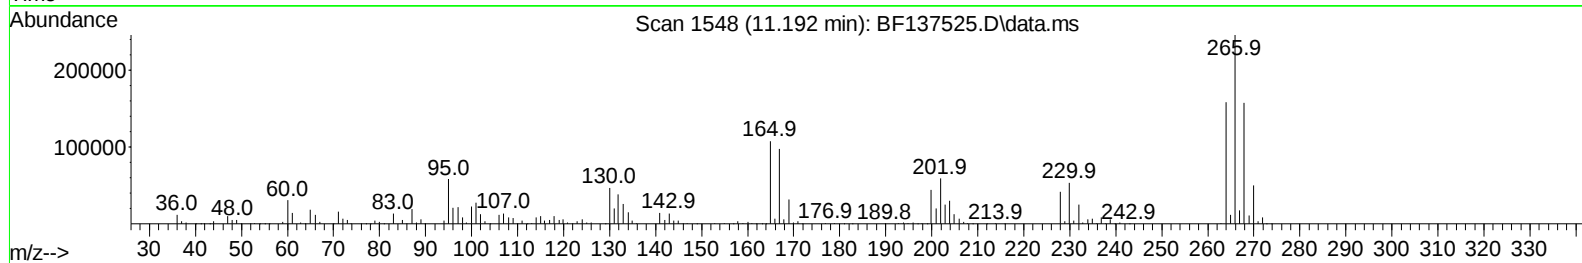


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030724\
Data File : BF137525.D
Acq On : 07 Mar 2024 12:40
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 18:25:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 00:07:28 2024
Response via : Initial Calibration

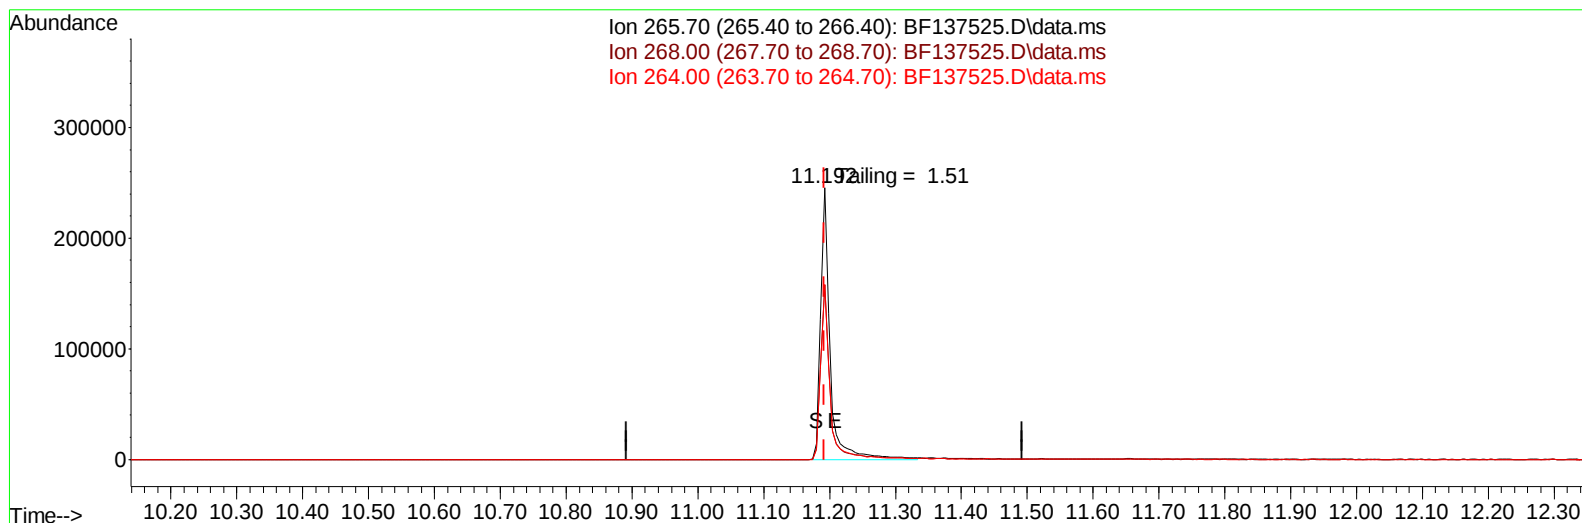




TIC: BF137525.D\data.ms

(70) Pentachlorophenol (C)**11.192min (+ 0.000) 27310.55 ng****response 239922**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	64.20
264.00	63.60	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030724\
Data File : BF137525.D
Acq On : 07 Mar 2024 12:40
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 18:25:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 00:07:28 2024
Response via : Initial Calibration

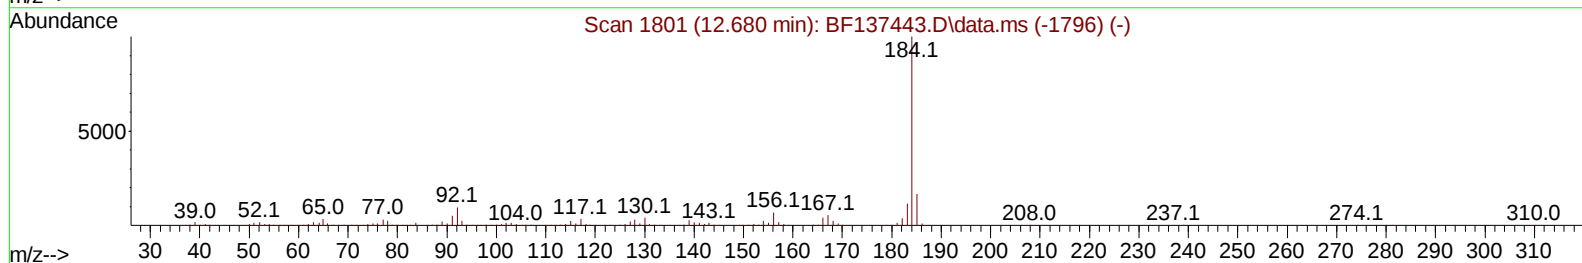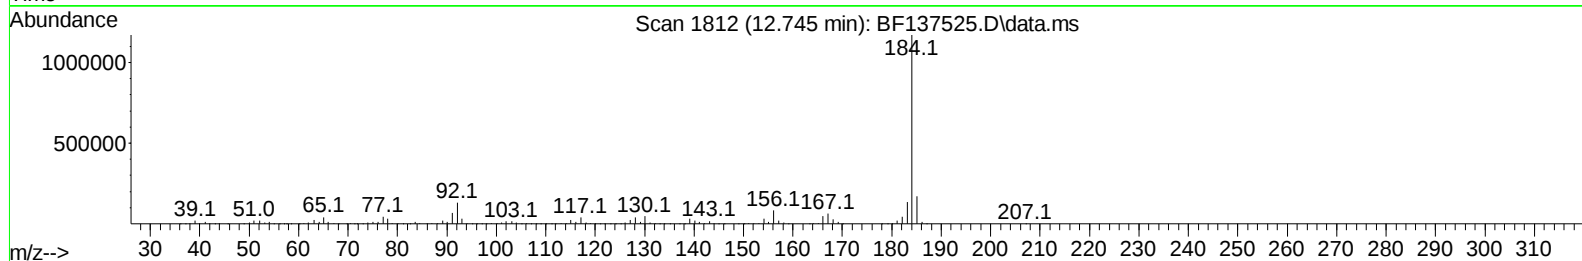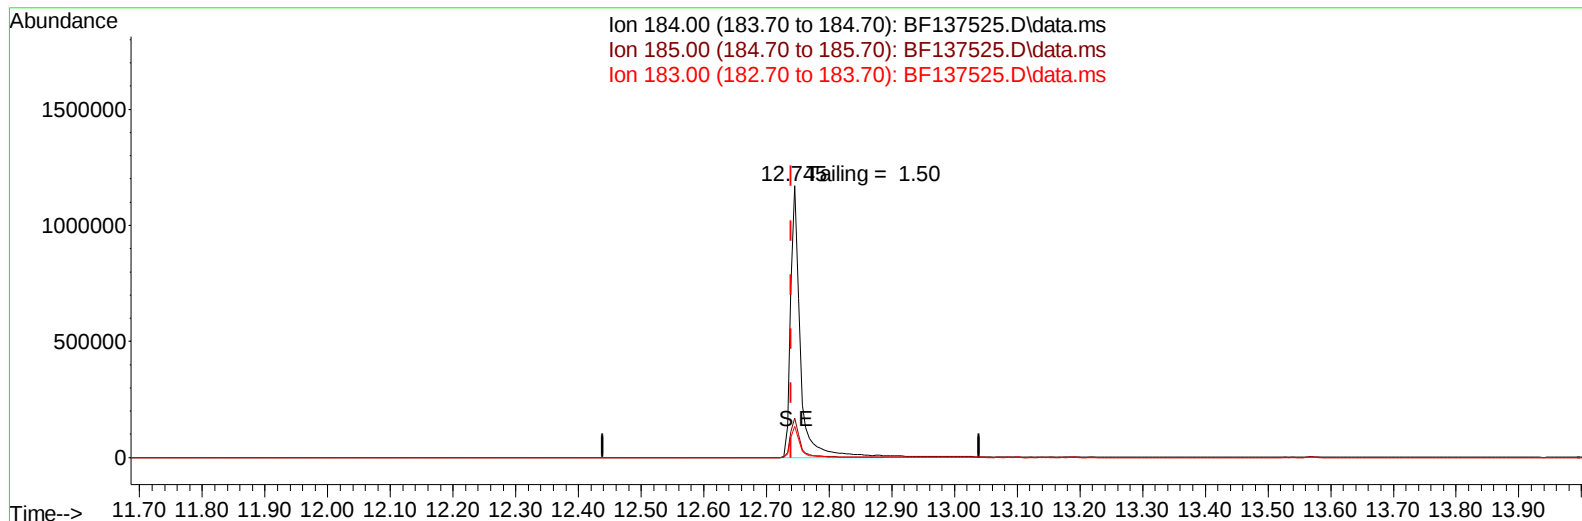

TIC: BF137525.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 0.00 ng

response 1300599

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.61
183.00	11.60	11.55
0.00	0.00	0.00