


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030724\
Data File : BF137525.D
Acq On : 07 Mar 2024 12:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p



Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 08 00:31:33 2024

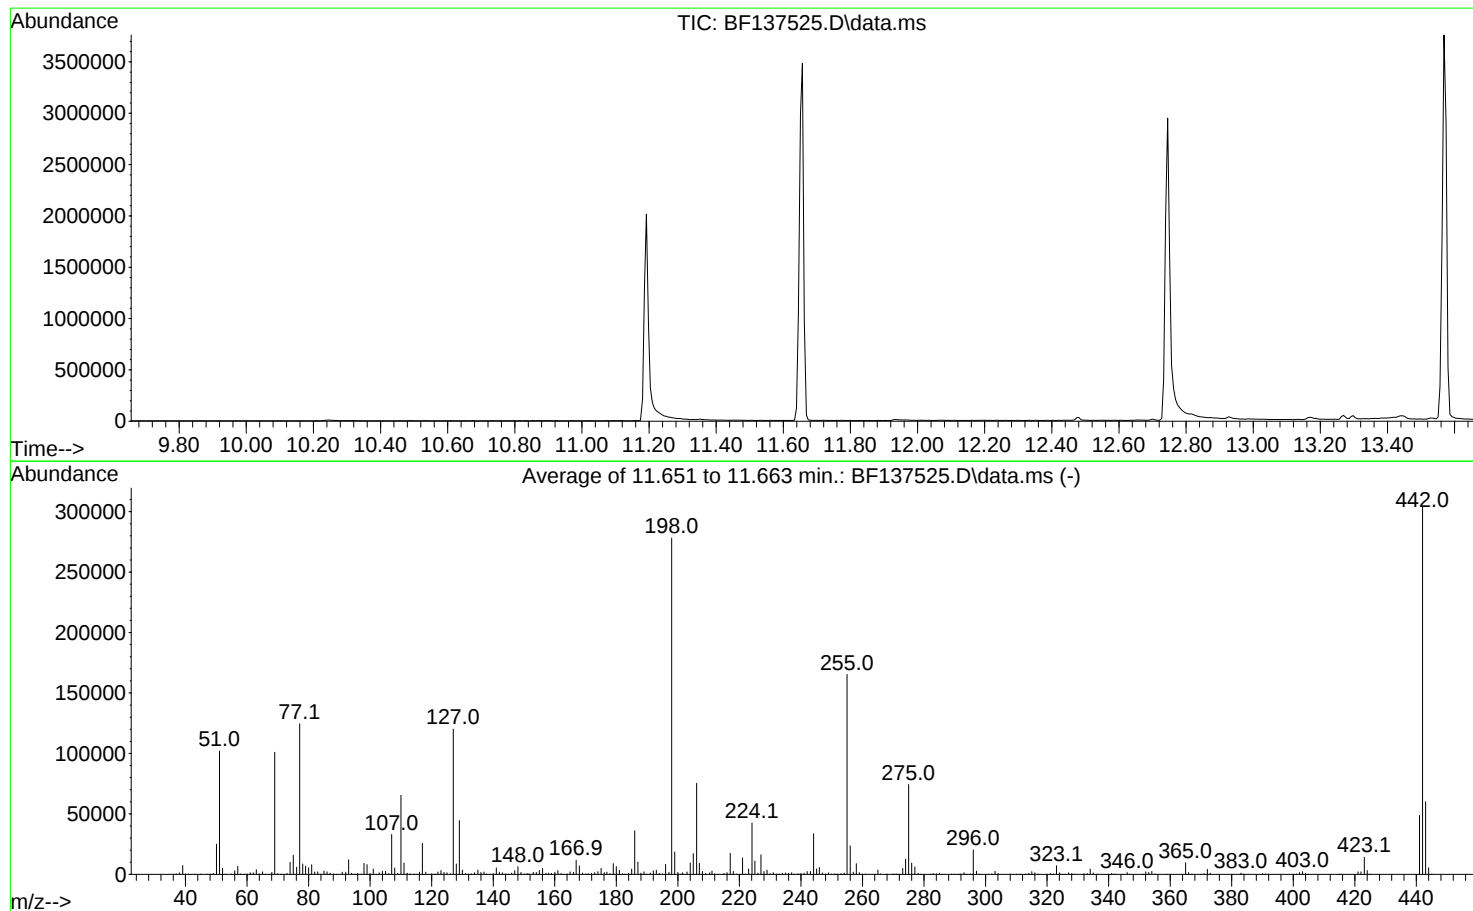

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	101964	PASS
68	69	0.00	2	1.7	1740	PASS
69	198	0.00	100	36.3	100923	PASS
70	69	0.00	2	0.7	671	PASS
127	198	10	80	43.2	120179	PASS
197	198	0.00	2	0.6	1674	PASS
198	198	100	100	100.0	278117	PASS
199	198	5	9	6.7	18597	PASS
275	198	10	60	26.7	74301	PASS
365	198	1	100	3.5	9630	PASS
441	198	0.01	100	17.5	48691	PASS
442	442	50	100	100.0	304235	PASS
443	442	15	24	19.8	60155	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP

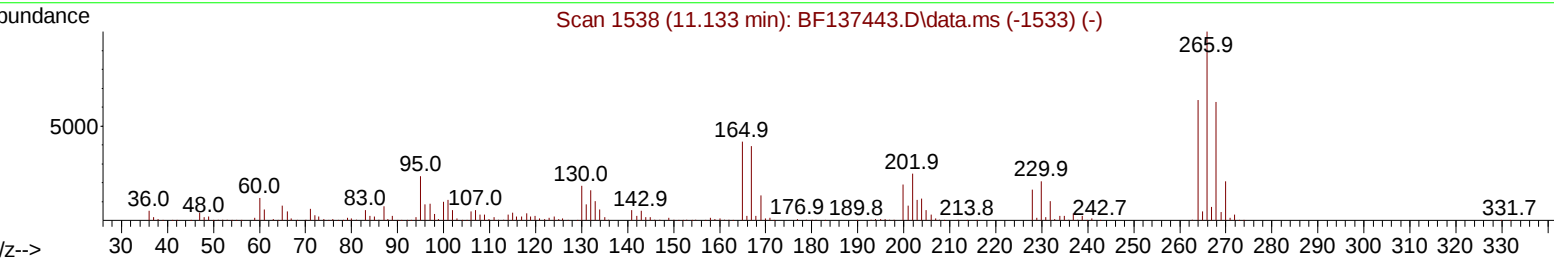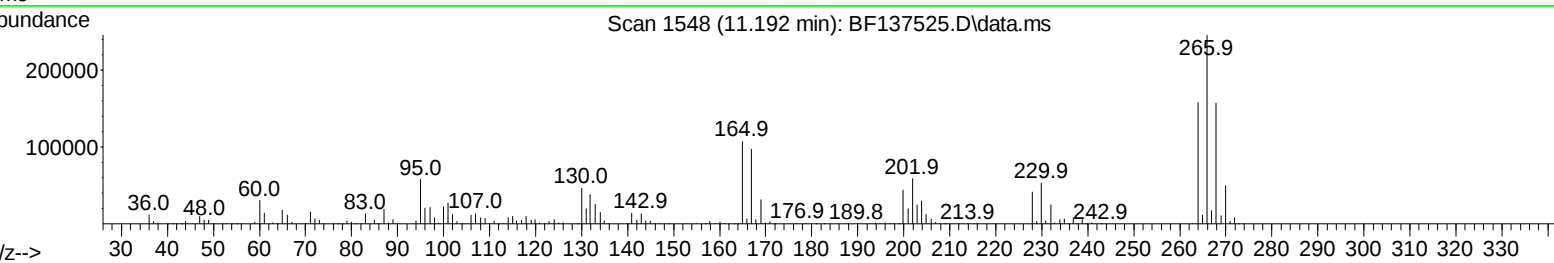

TIC: BF137525.D\data.ms




response **239922**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	64.20
264.00	63.60	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030724\
Data File : BF137525.D
Acq On : 07 Mar 2024 12:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 18:25:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 00:07:28 2024
Response via : Initial Calibration

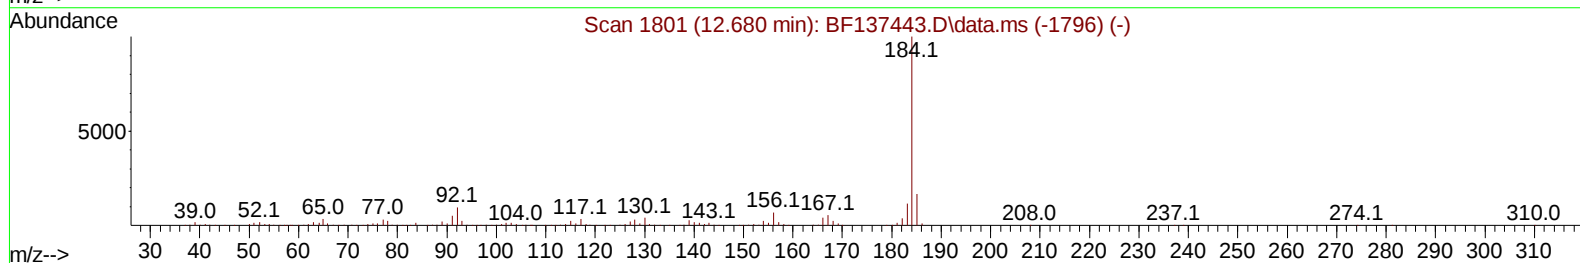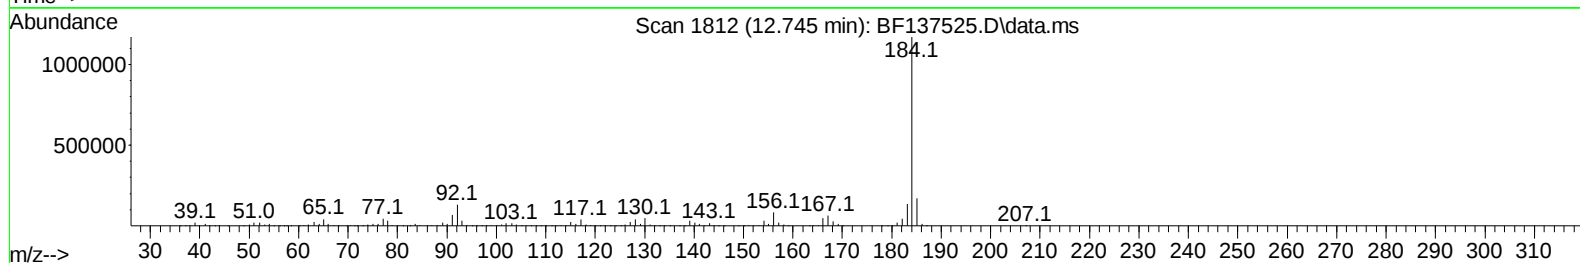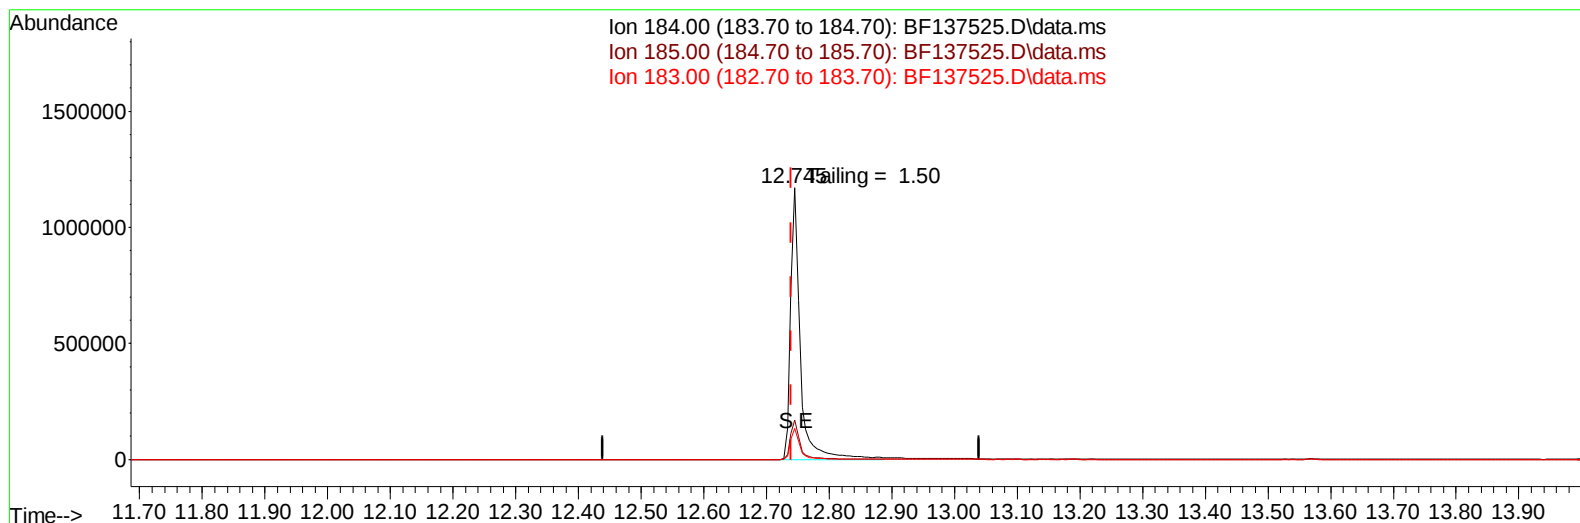

TIC: BF137525.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 0.00 ng

response 1300599

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.61
183.00	11.60	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2024	BNA_F	<u>BF137525.D</u>
Compound Name	Response	Retention Time
DDT	648484	13.568
DDD	12304	13.268
DDE	3414	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15718	664202	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP