
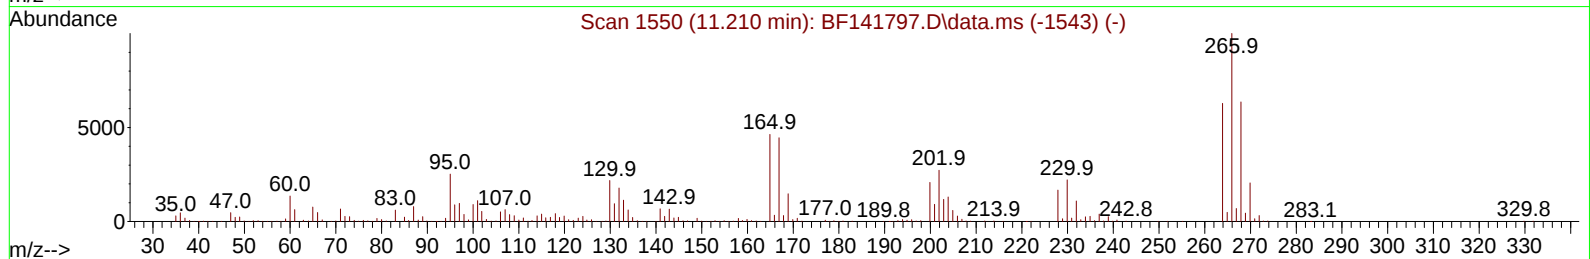
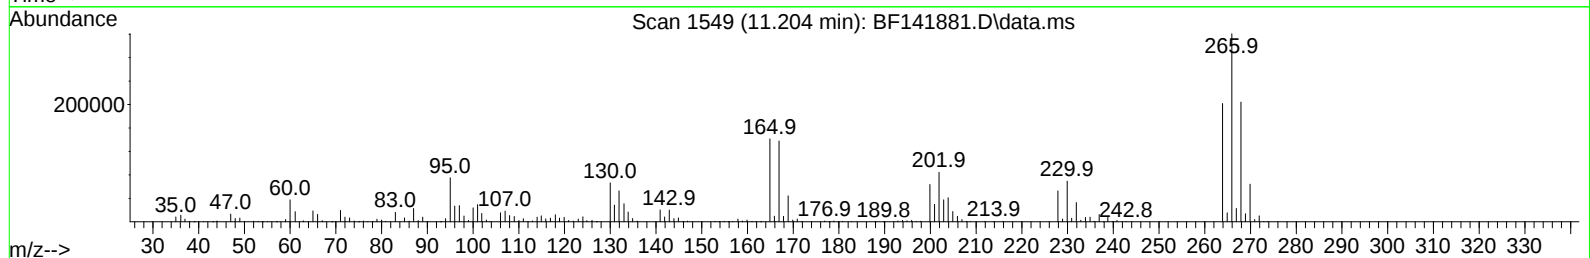


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
Data File : BF141881.D
Acq On : 07 Mar 2025 08:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 09:59:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

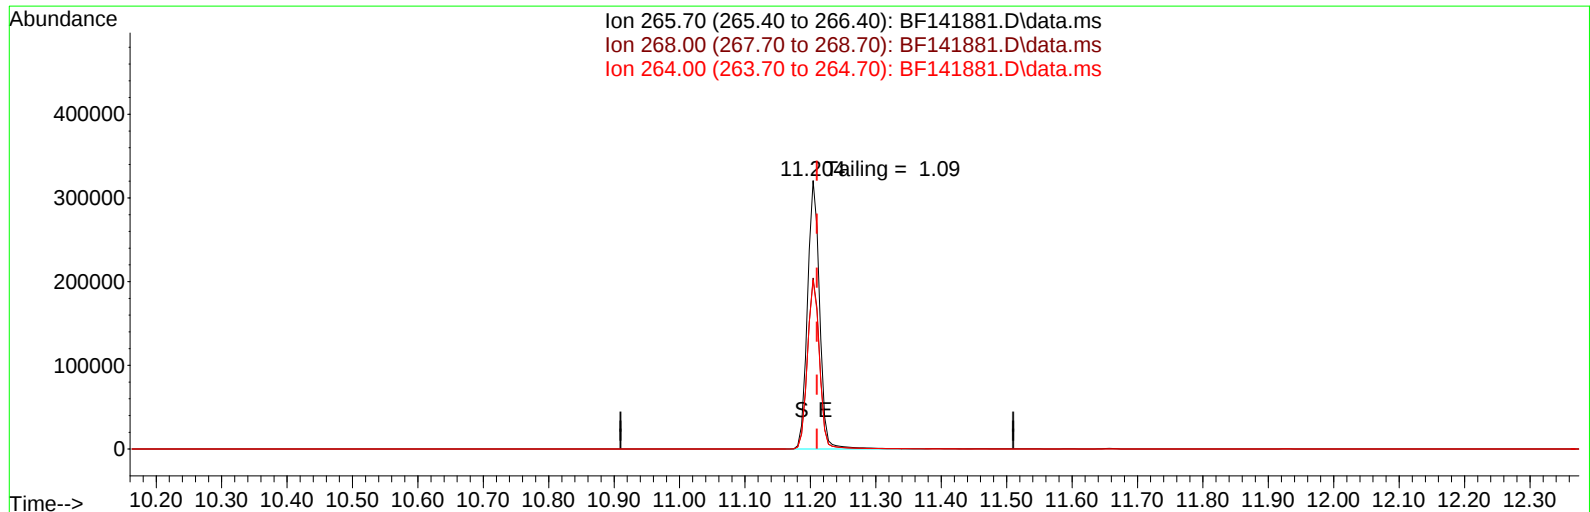

TIC: BF141881.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 136401.80 ng

response 416145

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.68
264.00	62.80	62.88
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\  
Data File : BF141881.D  
Acq On    : 07 Mar 2025  08:26  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 07 09:59:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

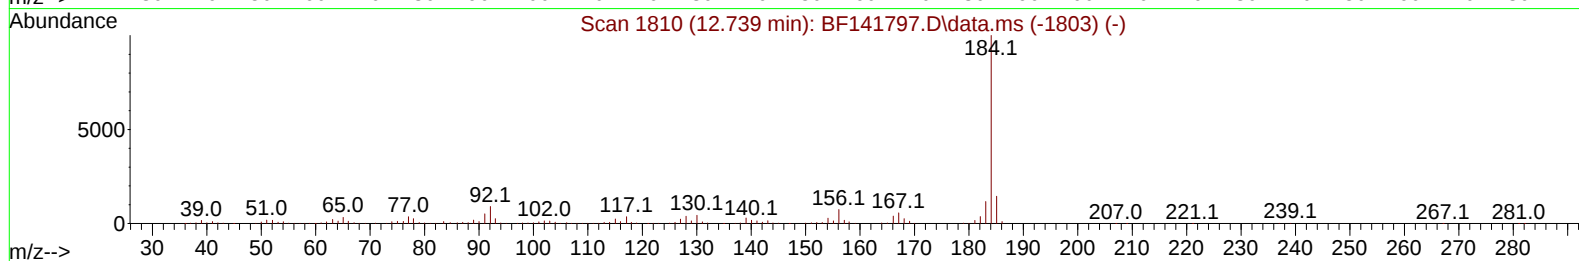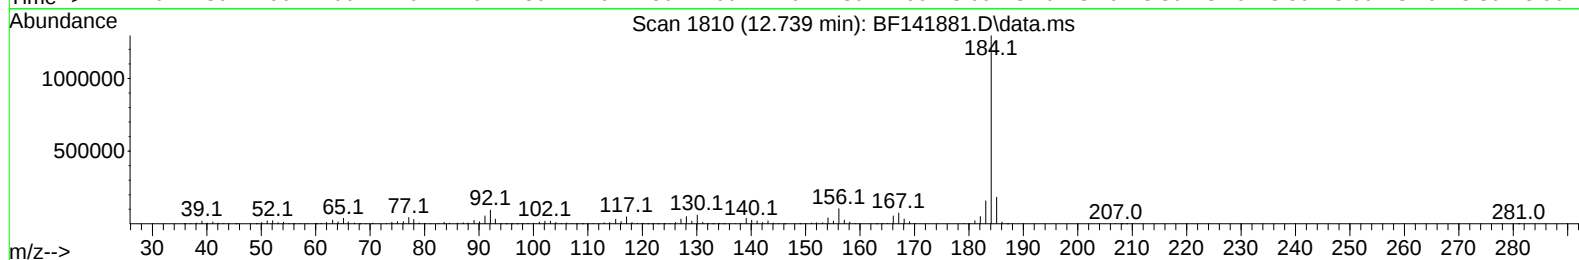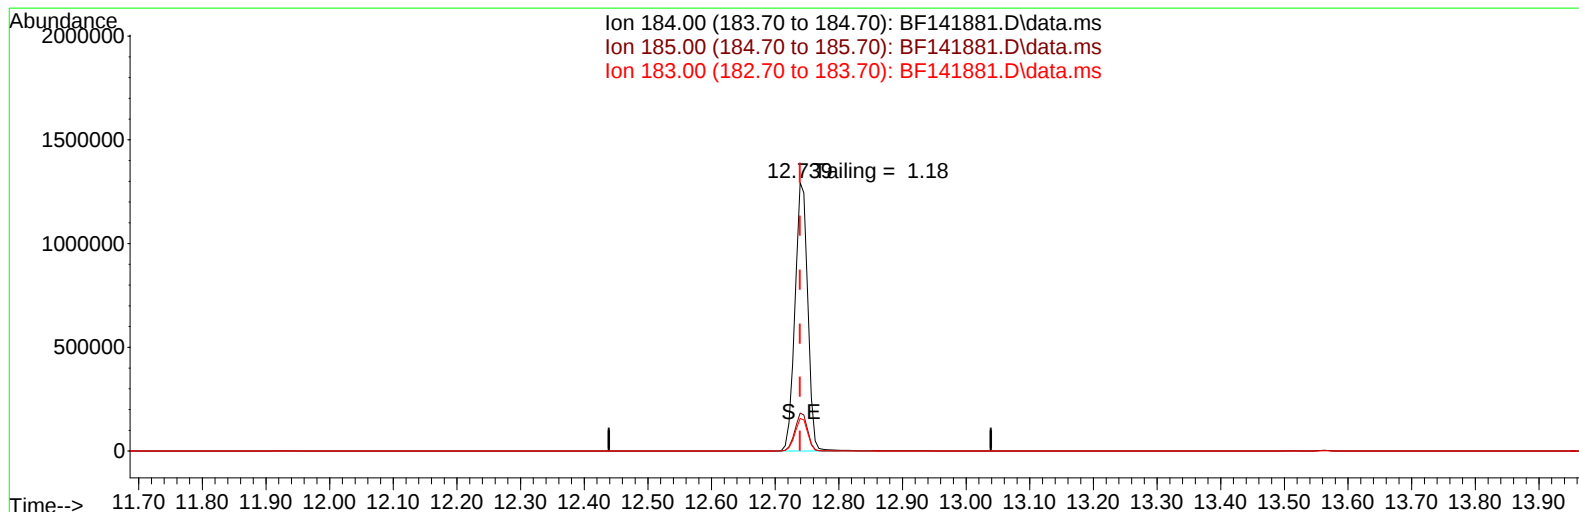

TIC: BF141881.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 161104.25 ng

response **1816840**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.17
183.00	11.70	12.15
0.00	0.00	0.00