

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
 Data File : BF141883.D
 Acq On : 07 Mar 2025 09:26
 Operator : RC/JU
 Sample : PB167016BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167016BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	19	30	38	rVB	52640	96108	1.15%	0.224%
2	5.510	574	581	587	rBV	3547766	5110574	61.11%	11.920%
3	6.504	743	750	755	rBV	3439120	5071609	60.64%	11.829%
4	6.881	809	814	820	rBV	834377	1068595	12.78%	2.492%
5	7.445	902	910	915	rBV	2322544	3436340	41.09%	8.015%
6	8.163	1026	1032	1052	rBV	1073978	1423191	17.02%	3.320%
7	9.239	1207	1215	1220	rBV	4988394	6803663	81.35%	15.869%
8	9.916	1321	1330	1346	rBV	1310313	1670756	19.98%	3.897%
9	10.704	1457	1464	1469	rBV	3658516	4797737	57.37%	11.190%
10	11.404	1577	1583	1588	rBV	1401569	1779090	21.27%	4.150%
11	12.992	1846	1853	1858	rBV	6235602	8363236	100.00%	19.507%
12	14.039	2025	2031	2040	rVB	1258959	1646229	19.68%	3.840%
13	15.510	2275	2281	2296	rVB	814195	1272610	15.22%	2.968%
14	17.133	2548	2557	2579	rVB3	71808	333584	3.99%	0.778%




Sum of corrected areas: 42873322

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
Data File : BF141883.D
Acq On : 07 Mar 2025 09:26
Operator : RC/JU
Sample : PB167016BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167016BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

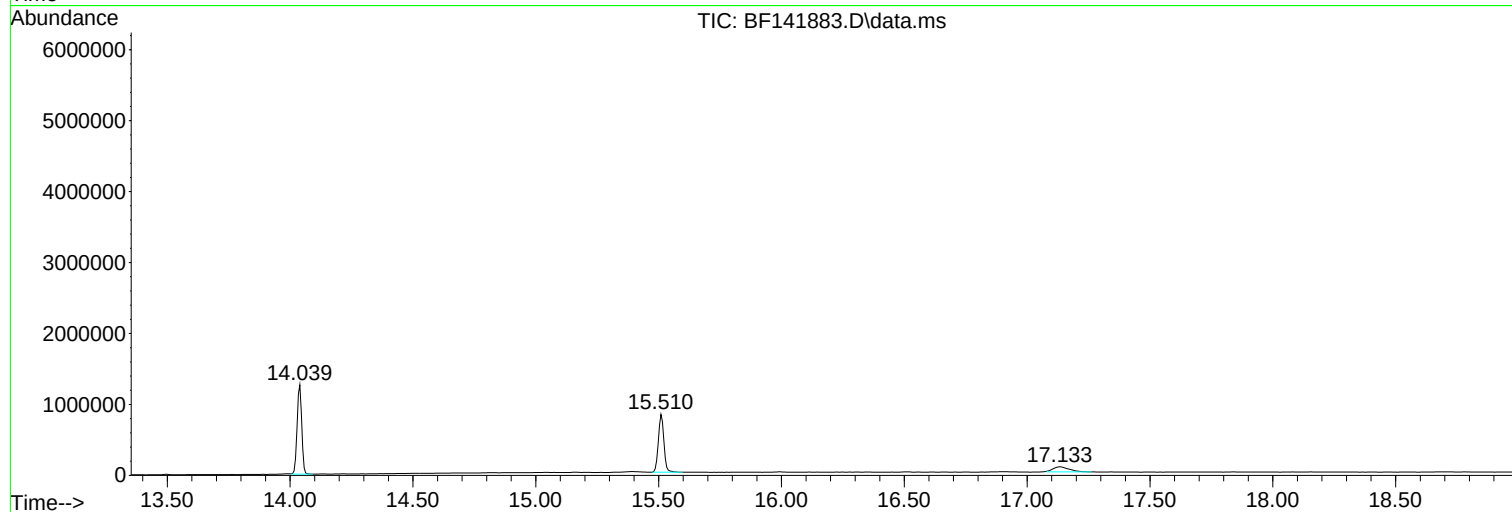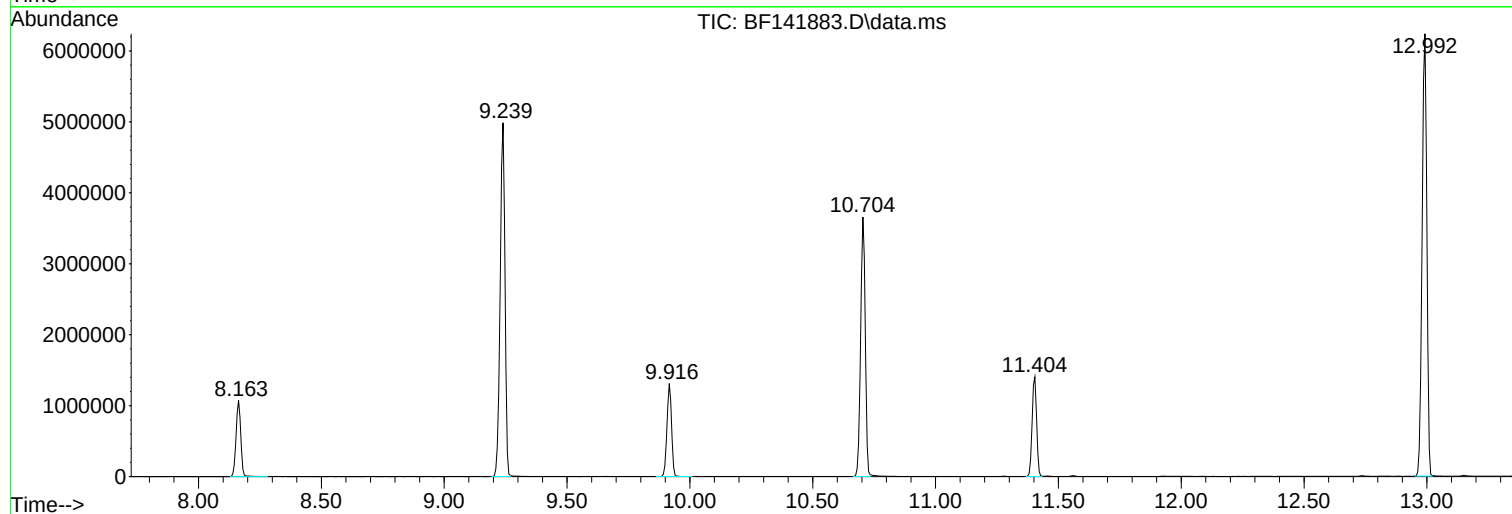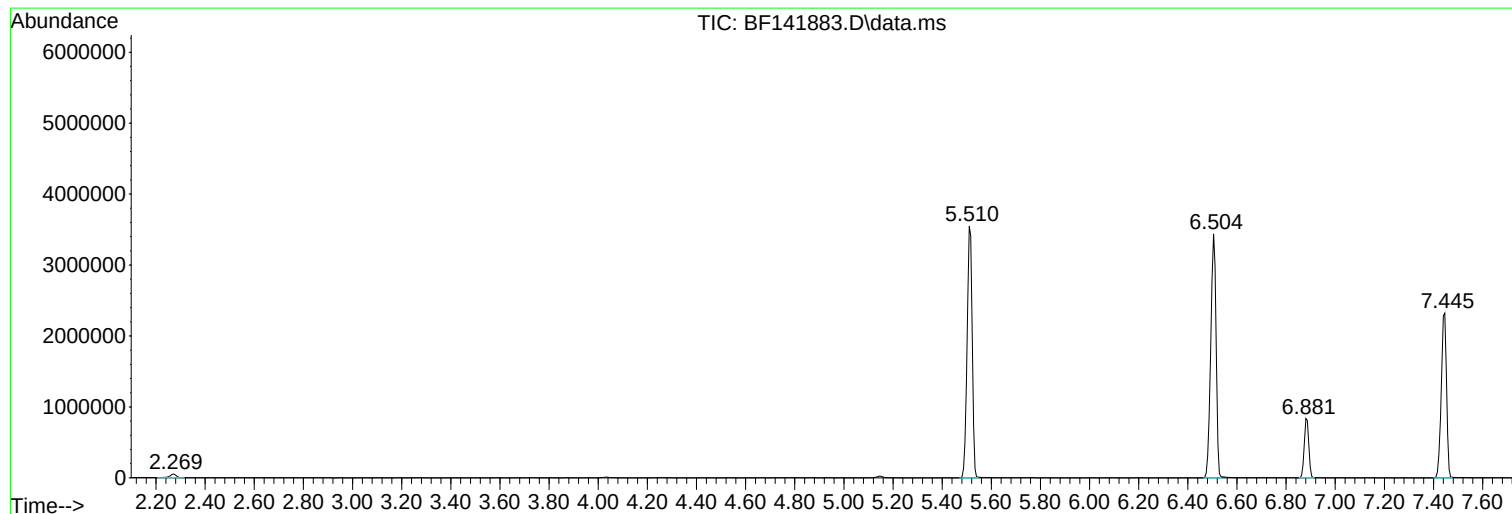

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
Data File : BF141883.D
Acq On : 07 Mar 2025 09:26
Operator : RC/JU
Sample : PB167016BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167016BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
Data File : BF141883.D
Acq On : 07 Mar 2025 09:26
Operator : RC/JU
Sample : PB167016BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167016BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------