
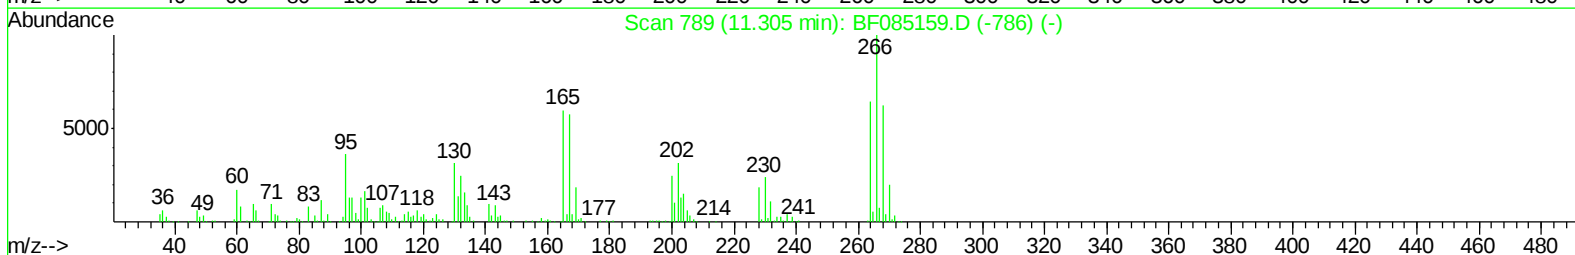
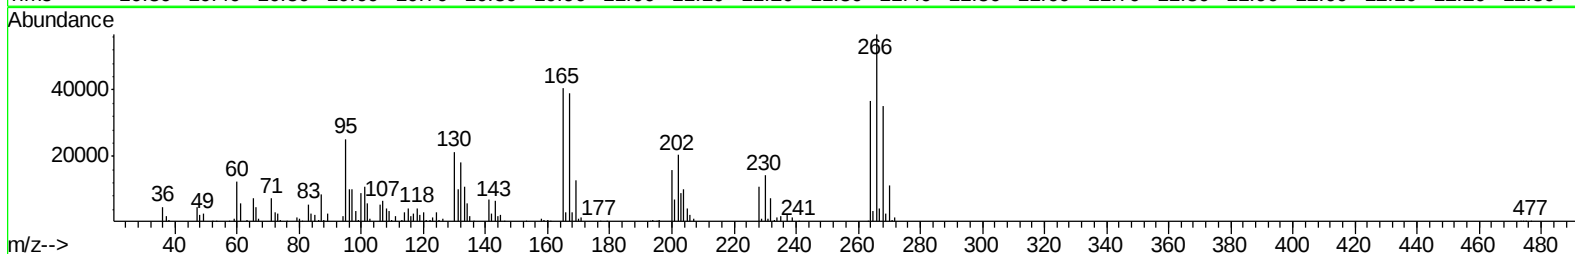


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030816\
Data File : BF085253.D
Acq On : 8 Mar 2016 13:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 02:32:17 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

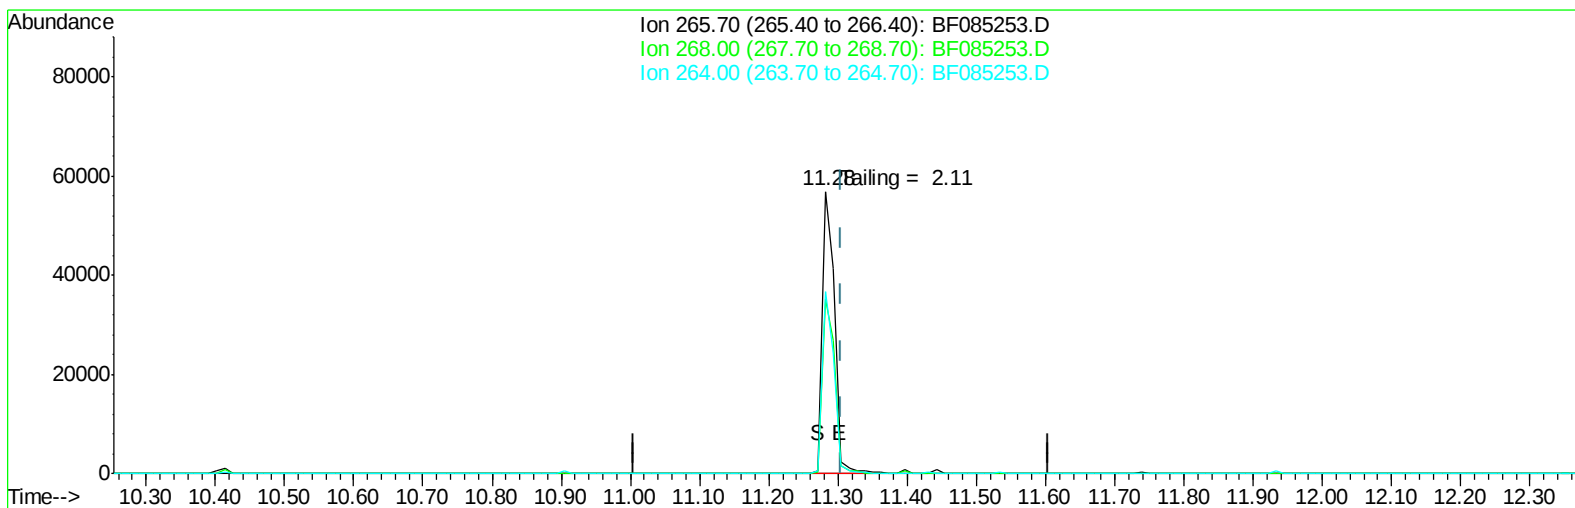

TIC: BF085253.D

(69) Pentachlorophenol (C)




11.282min (-0.023) 58773.19ng

response 71305

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	61.79
264.00	64.30	64.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030816\
Data File : BF085253.D
Acq On : 8 Mar 2016 13:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 02:32:17 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

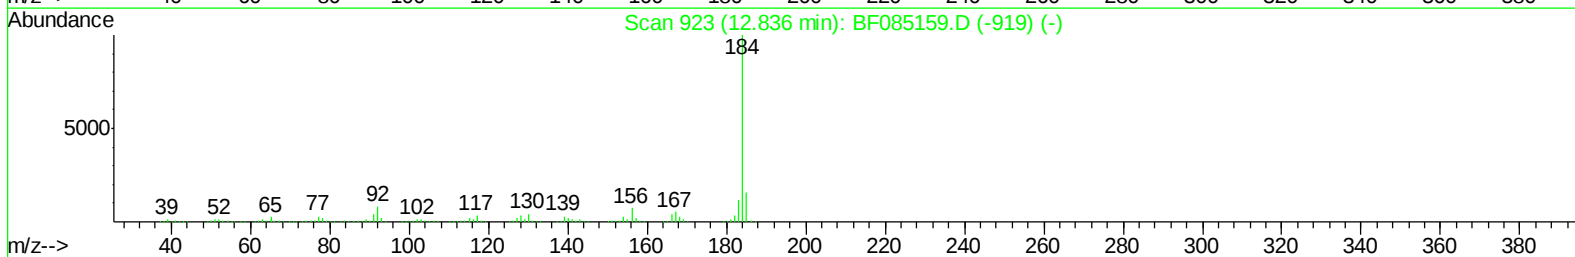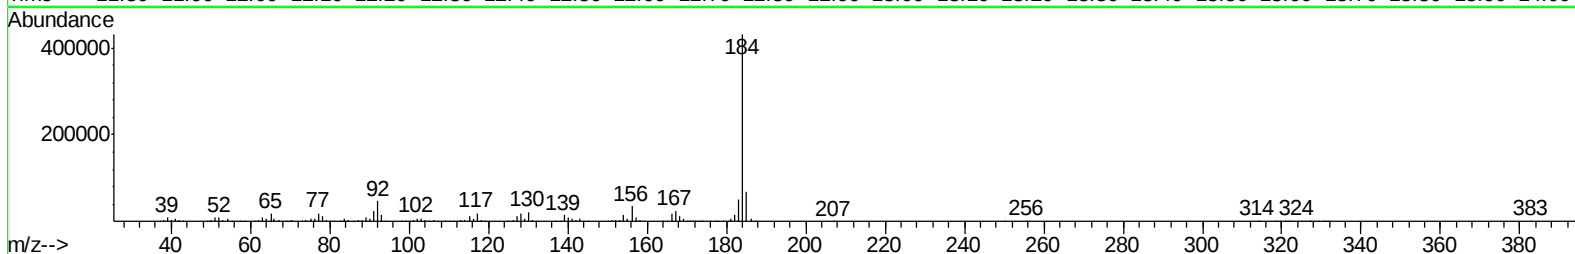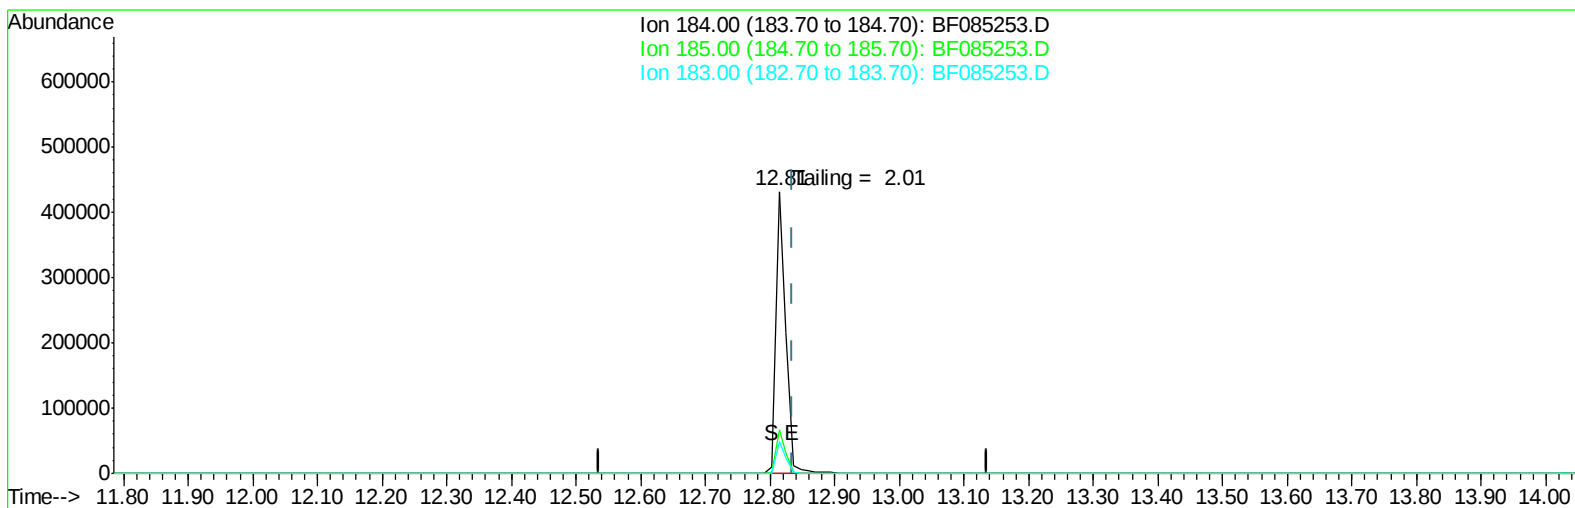

TIC: BF085253.D

(76) Benzidine

12.814min (-0.023) 46330.02ng

response 472954

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.65
183.00	11.80	11.59
0.00	0.00	0.00