


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030816\
 Data File : BF085277.D
 Acq On : 9 Mar 2016 1:24
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

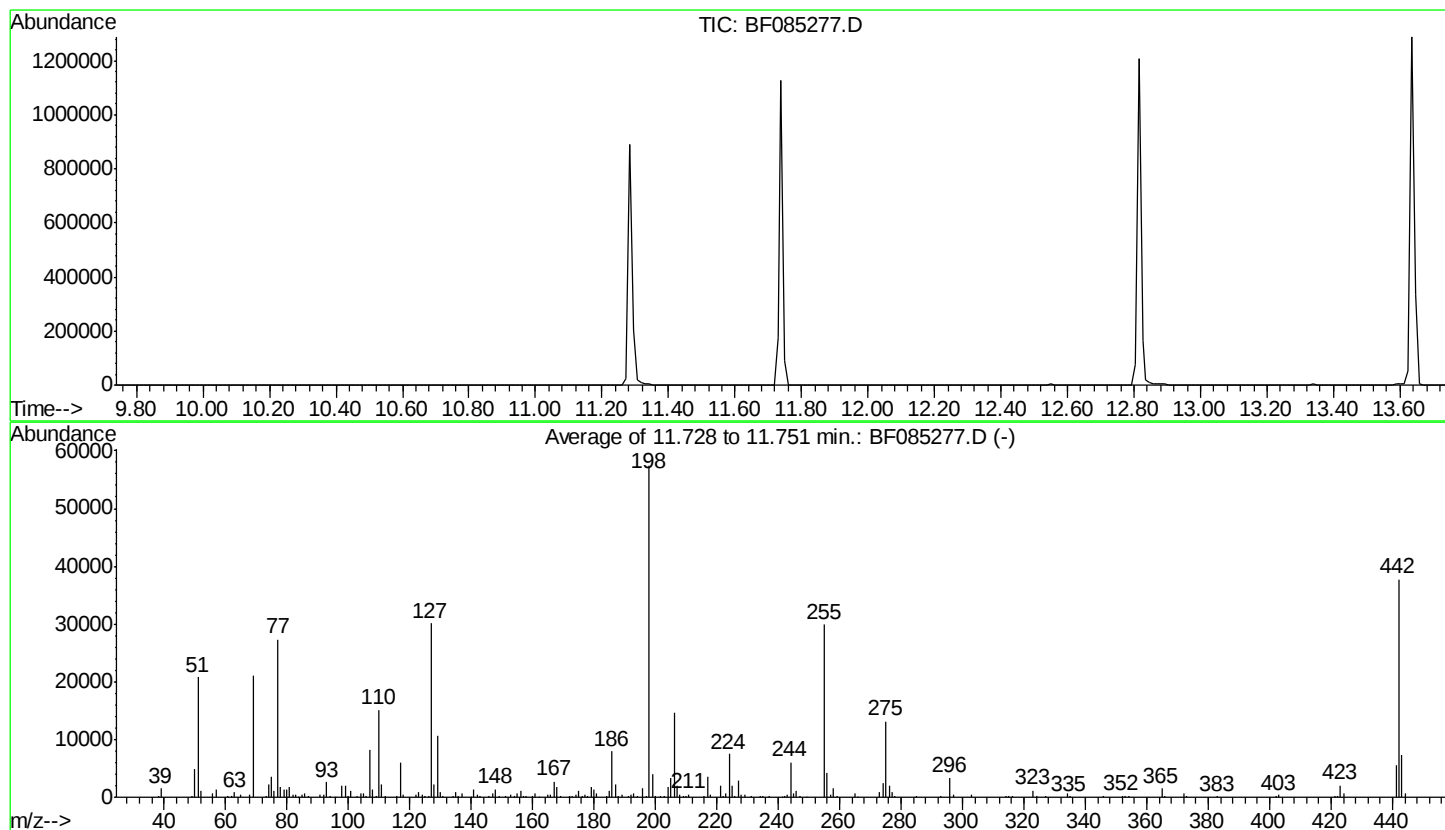

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	20755	PASS
68	69	0.00	2	1.7	363	PASS
69	198	0.00	100	36.7	21065	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	30067	PASS
197	198	0.00	2	0.6	333	PASS
198	198	100	100	100.0	57435	PASS
199	198	5	9	6.8	3924	PASS
275	198	10	60	22.8	13122	PASS
365	198	1	100	2.6	1496	PASS
441	442	0.01	24	14.9	5632	PASS
442	198	50	100	65.7	37714	PASS
443	442	15	24	19.3	7267	PASS