
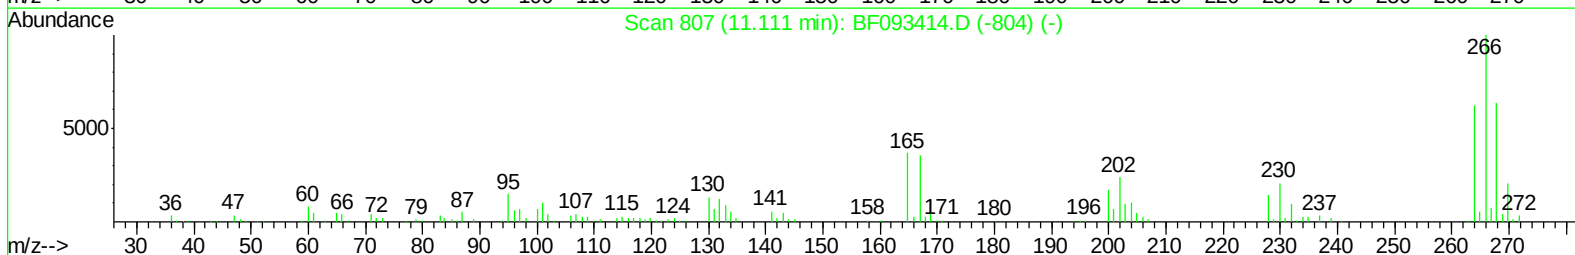
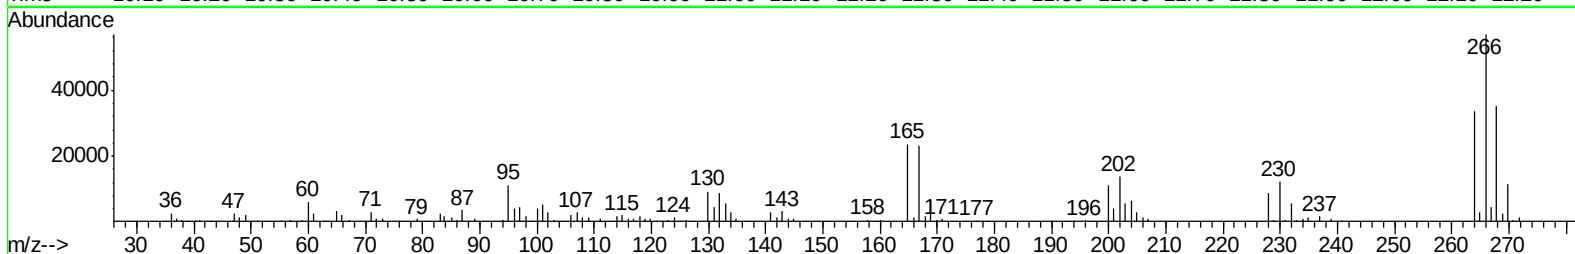


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030817\
Data File : BF093455.D
Acq On : 9 Mar 2017 4:51
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 06:59:28 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

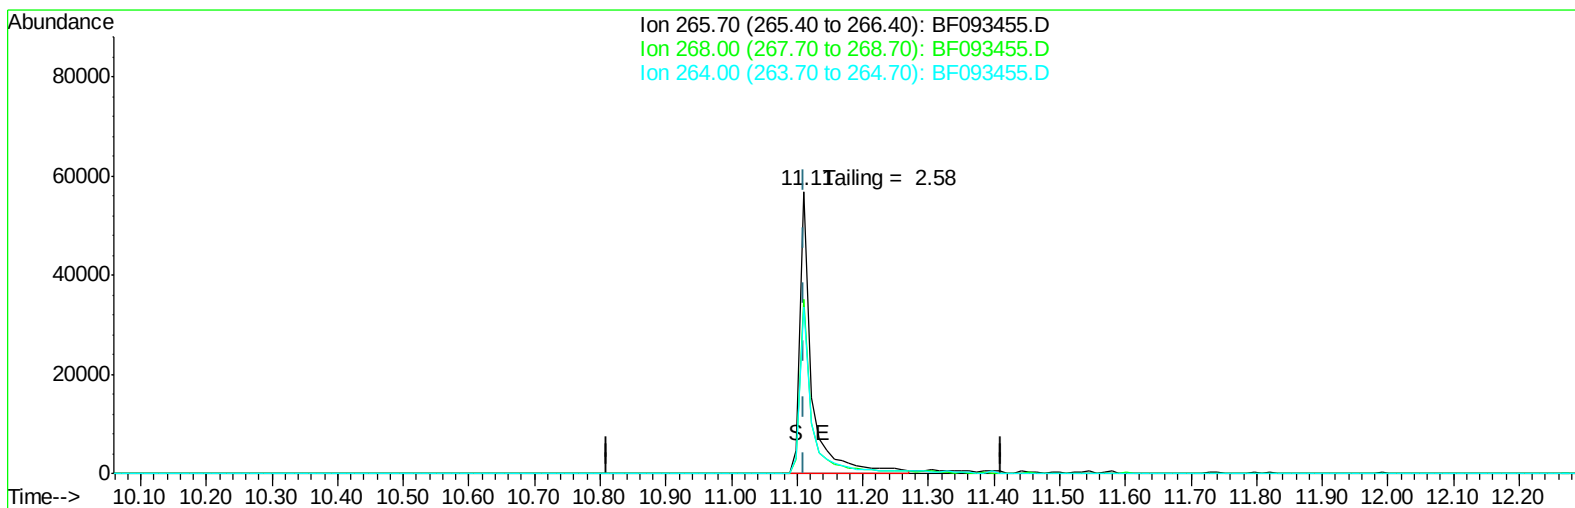

TIC: BF093455.D

(69) Pentachlorophenol (C)




11.111min (-0.000) 0.00ng

response 72153

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	61.68
264.00	62.90	59.02
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030817\  
Data File : BF093455.D  
Acq On    : 9 Mar 2017    4:51  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 09 06:59:28 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

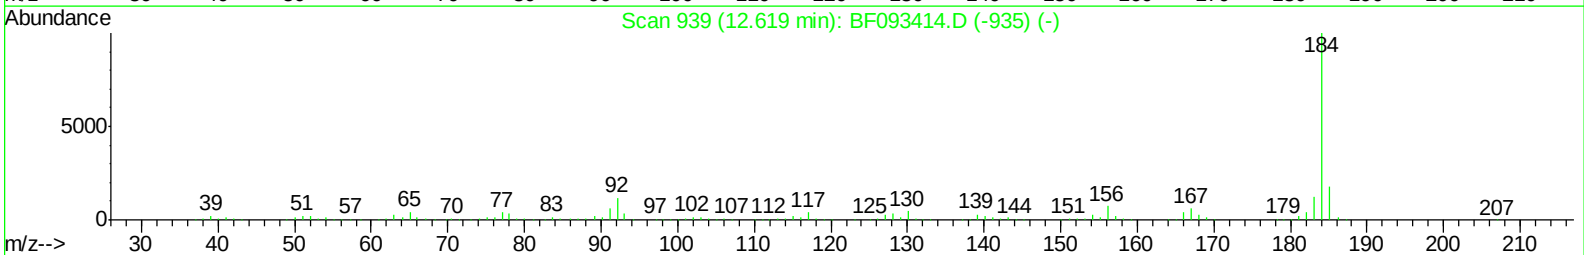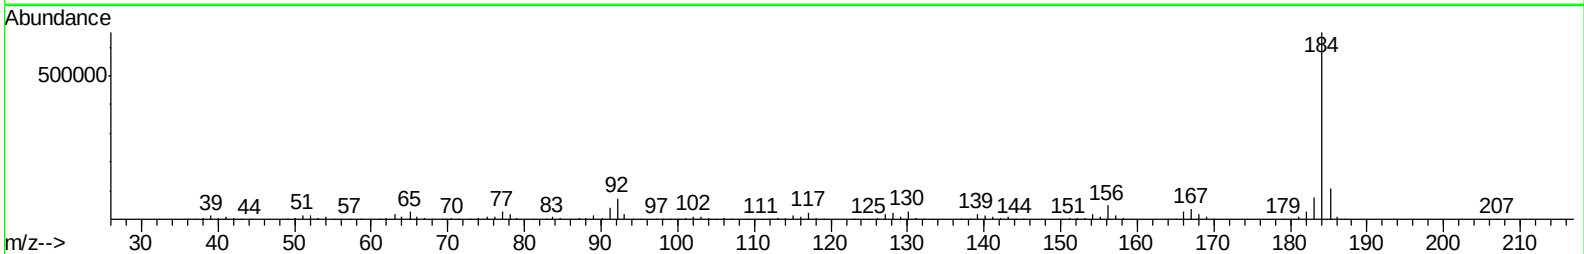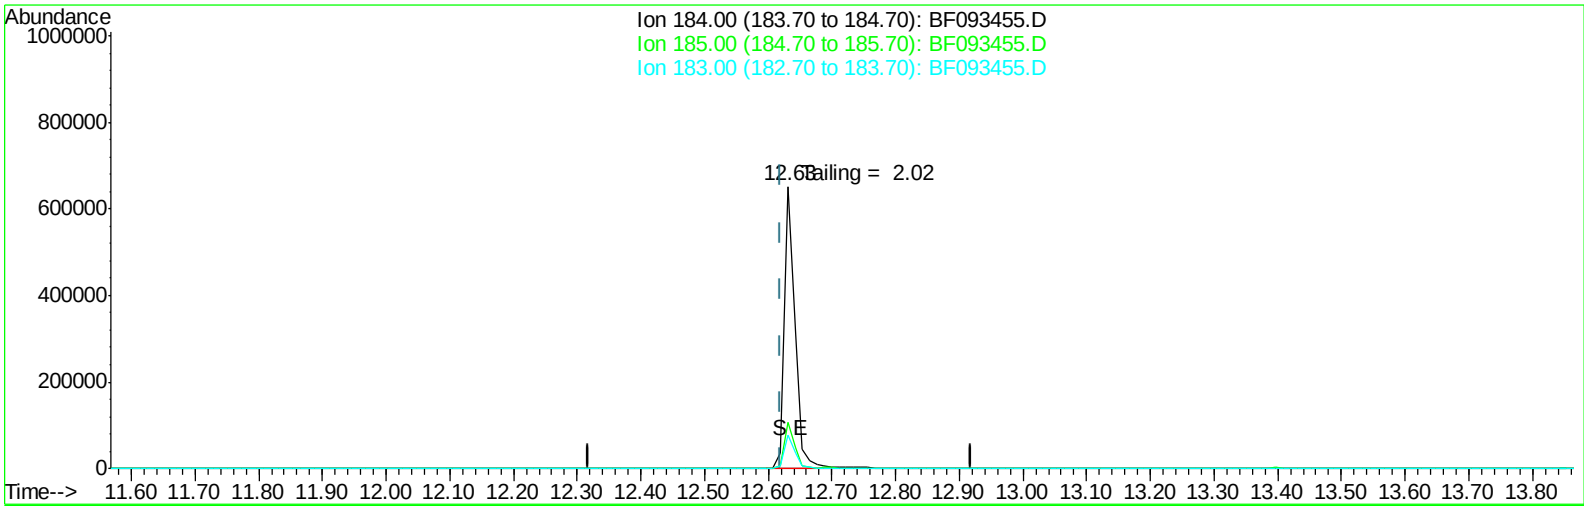

TIC: BF093455.D

(76) Benzidine

12.631min (+0.011) 0.00ng

response 756811

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	16.23
183.00	11.50	11.78
0.00	0.00	0.00