

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030817\
 Data File : BF093464.D
 Acq On : 9 Mar 2017 9:00
 Operator : SJ/MA
 Sample : I2127-25
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D-14

Quant Time: Mar 09 10:20:06 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 15:55:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.77	152	173253	20.00	ng	0.00
21) Naphthalene-d8	8.06	136	647084	20.00	ng	0.00
38) Acenaphthene-d10	9.81	164	284482	20.00	ng	0.00
63) Phenanthrene-d10	11.29	188	418757	20.00	ng	0.01
75) Chrysene-d12	13.93	240	366012	20.00	ng	0.01
86) Perylene-d12	15.34	264	286605	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	1386414	133.18	ng	0.02
7) Phenol-d6	6.42	99	1709037	130.19	ng	0.01
23) Nitrobenzene-d5	7.34	82	1092918	93.71	ng	0.00
41) 2,4,6-Tribromophenol	10.60	330	232416	125.40	ng	0.00
44) 2-Fluorobiphenyl	9.13	172	1753626	114.66	ng	0.00
78) Terphenyl-d14	12.87	244	1068489	75.90	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030817\
Data File : BF093464.D
Acq On : 9 Mar 2017 9:00
Operator : SJ/MA
Sample : I2127-25
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D-14

Quant Time: Mar 09 10:20:06 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

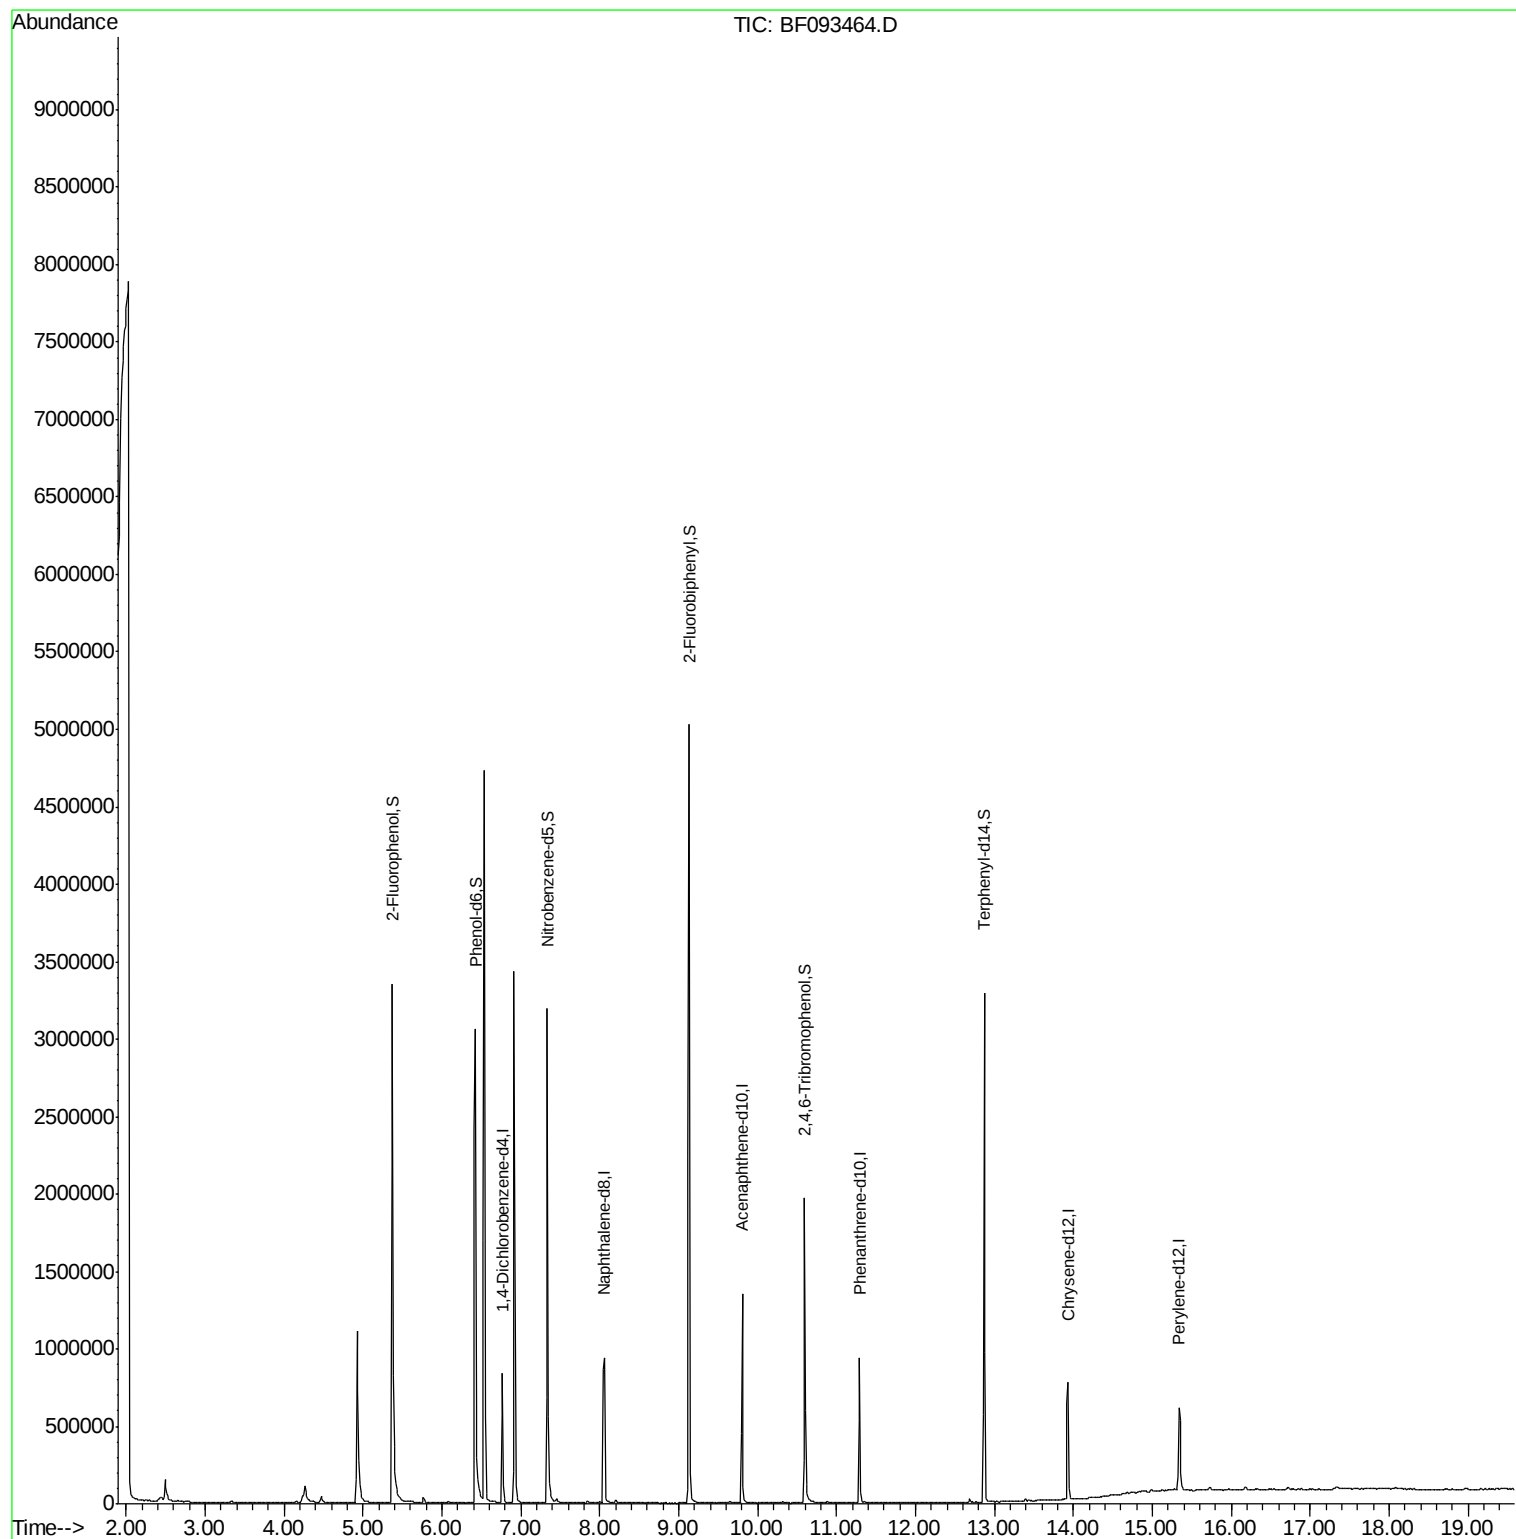



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.77 min Scan# 427

Delta R.T. -0.00 min

Lab File: BF093464.D

Acq: 9 Mar 2017 9:00

Instrument :

BNA_F

ClientSampled :

D-14


Tot Ion:152 Resp: 173253

Ion Ratio Lower Upper

152 100

150 154.6 124.9 187.3




115 54.1 46.0 69.0

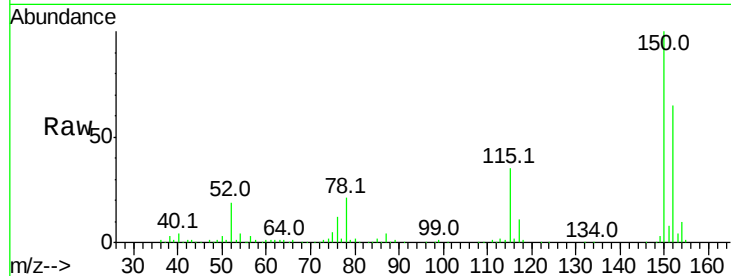

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

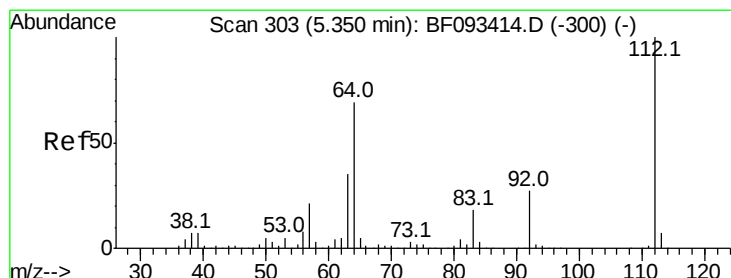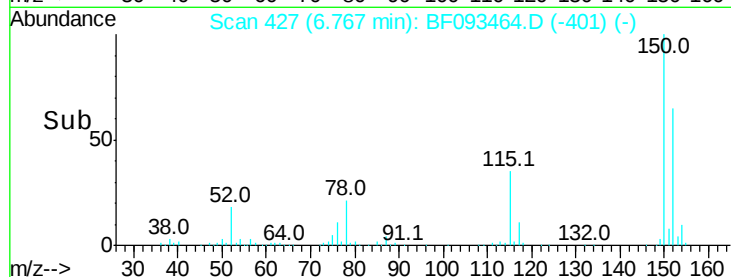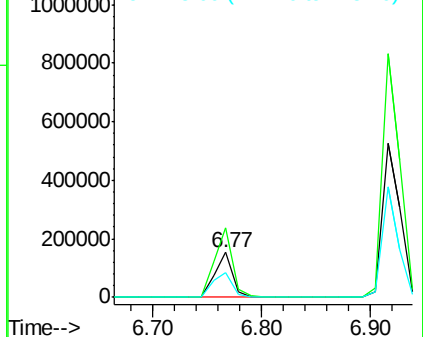

#5

2-Fluorophenol

Concen: 133.18 ng

RT: 5.37 min Scan# 305

Delta R.T. 0.02 min

Lab File: BF093464.D

Acq: 9 Mar 2017 9:00


Tgt Ion:112 Resp: 1386414

Ion Ratio Lower Upper

112 100

64 59.2 46.1 69.1



63 29.8 23.8 35.6

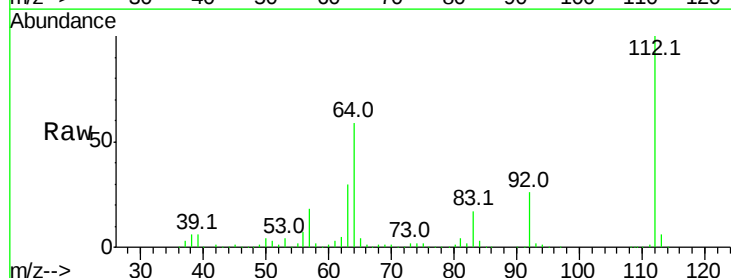


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

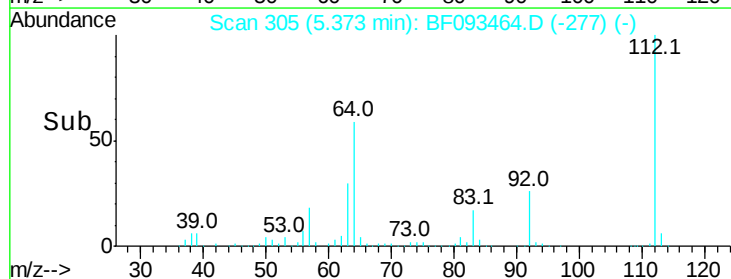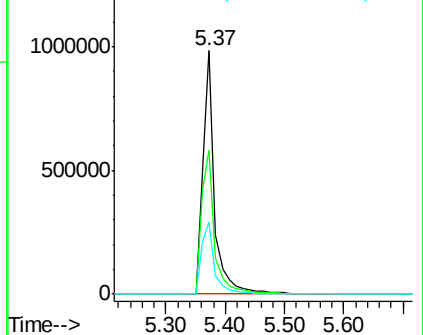

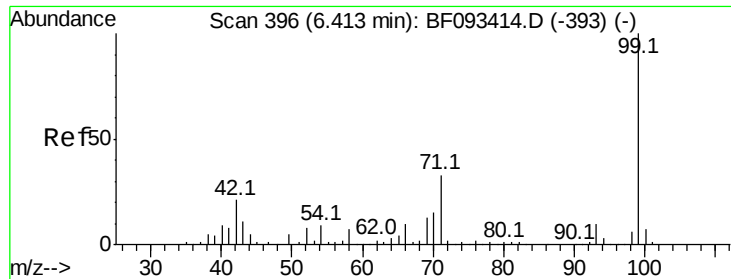

#7

Phenol-d6

Concen: 130.19 ng

RT: 6.42 min Scan# 397

Delta R.T. 0.01 min

Lab File: BF093464.D

Acq: 9 Mar 2017 9:00

Instrument :


BNA_F

ClientSampleId :

D-14

Tot Ion: 99 Resp: 1709037

Ion	Ratio	Lower	Upper
99	100		
42	16.8	15.6	23.4
71	29.1	27.5	41.3



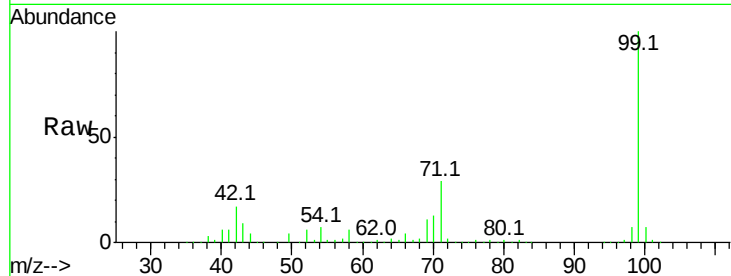


Abundance

Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

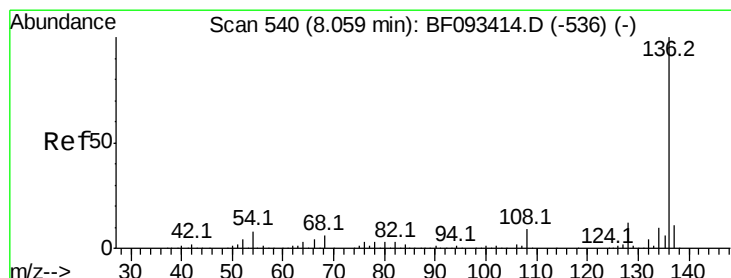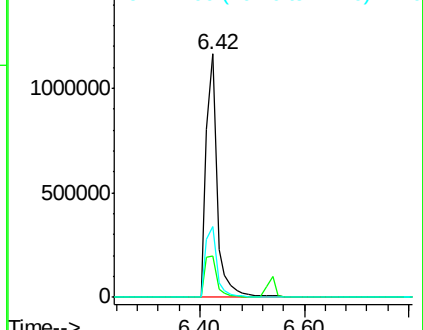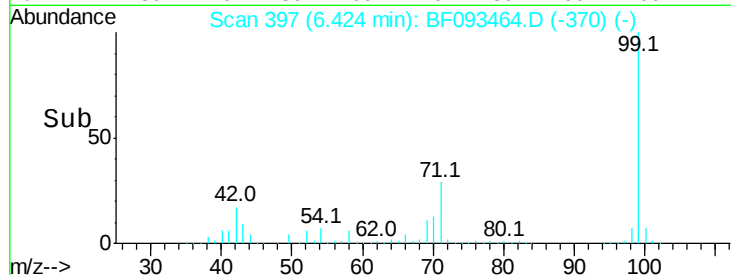

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.06 min Scan# 540


Delta R.T. -0.00 min

Lab File: BF093464.D

Acq: 9 Mar 2017 9:00

Tgt Ion: 136 Resp: 647084

Ion	Ratio	Lower	Upper
136	100		
137	10.4	8.4	12.6
54	7.5	4.5	6.7#
68	5.4	3.6	5.4

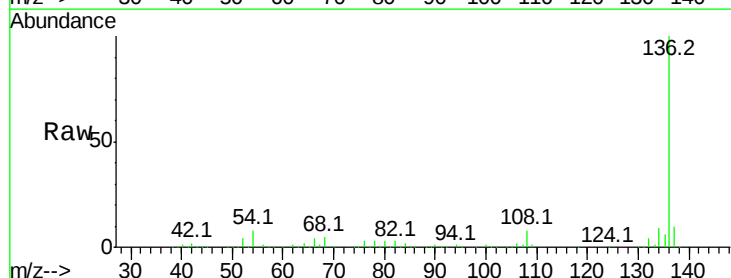



Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

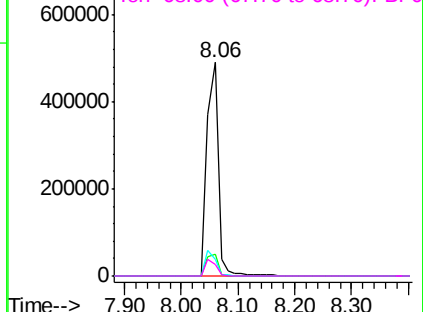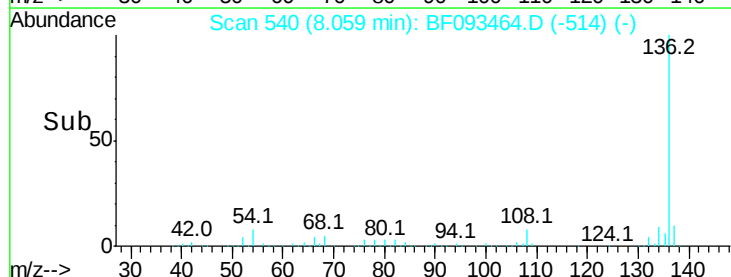




#23
 Nitrobenzene-d5
 Concen: 93.71 ng
 RT: 7.34 min Scan# 477
 Delta R.T. -0.00 min
 Lab File: BF093464.D
 Acq: 9 Mar 2017 9:00



Instrument :
 BNA_F
 ClientSampleID :
 D-14

Tot Ion: 82 Resp: 1092918

Ion	Ratio	Lower	Upper
82	100		
128	40.9	34.6	52.0
54	58.2	39.5	59.3

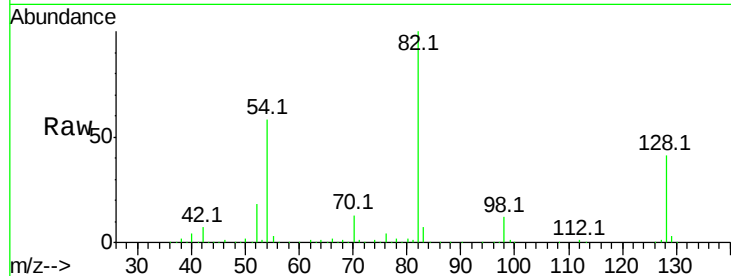


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

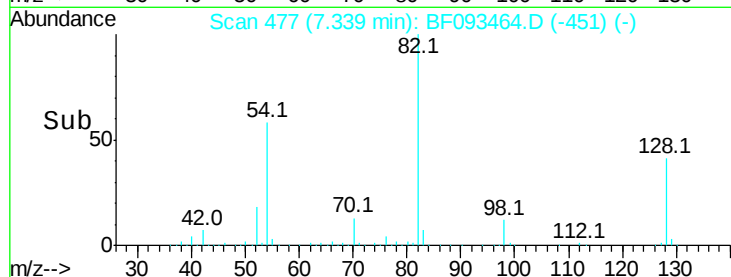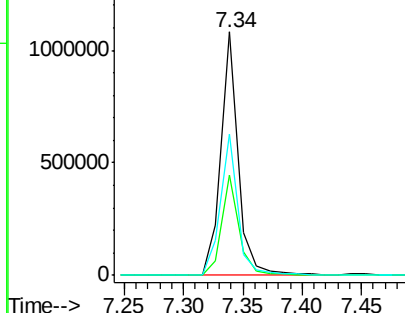



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.81 min Scan# 693
 Delta R.T. -0.00 min
 Lab File: BF093464.D
 Acq: 9 Mar 2017 9:00


Tgt Ion: 164 Resp: 284482

Ion	Ratio	Lower	Upper
164	100		
162	103.0	80.2	120.2
160	45.7	36.9	55.3

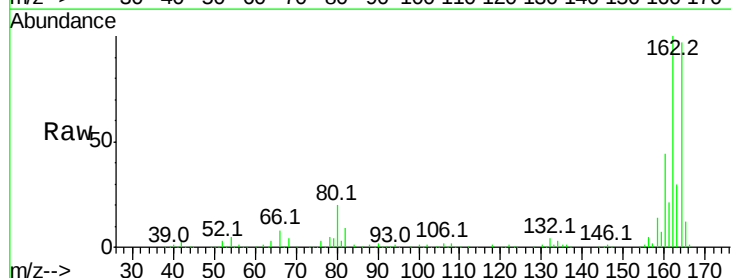

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

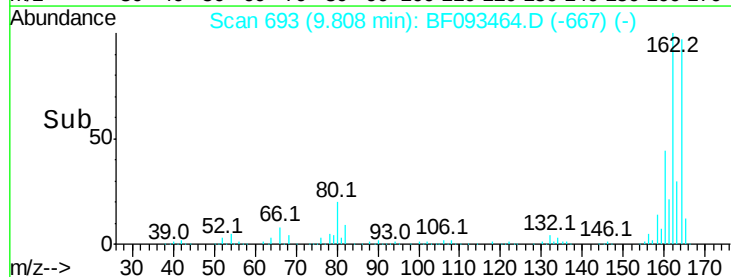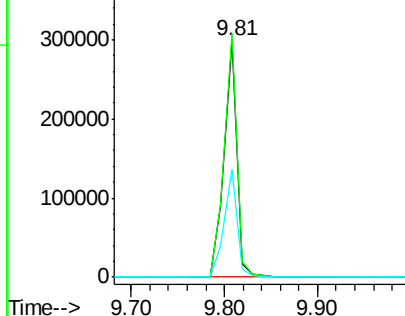


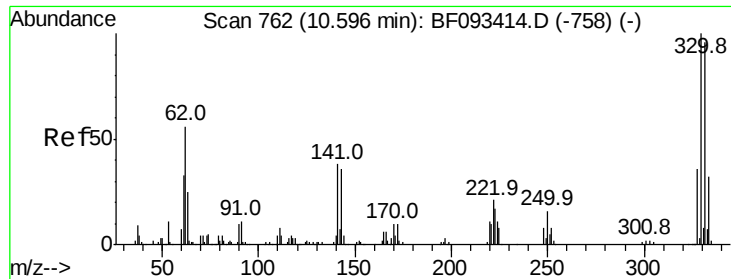




#41
 2,4,6-Tribromophenol
 Concen: 125.40 ng
 RT: 10.60 min Scan# 762
 Delta R.T. -0.00 min
 Lab File: BF093464.D
 Acq: 9 Mar 2017 9:00

Instrument :
 BNA_F
 ClientSampled :
 D-14

Tot Ion:330 Resp: 232416
 Ion Ratio Lower Upper
 330 100
 332 96.0 77.4 116.2
 141 41.6 34.1 51.1

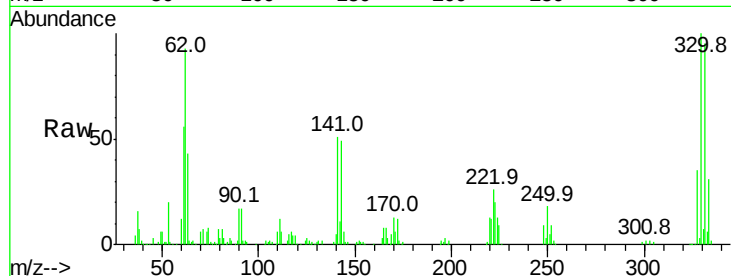


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

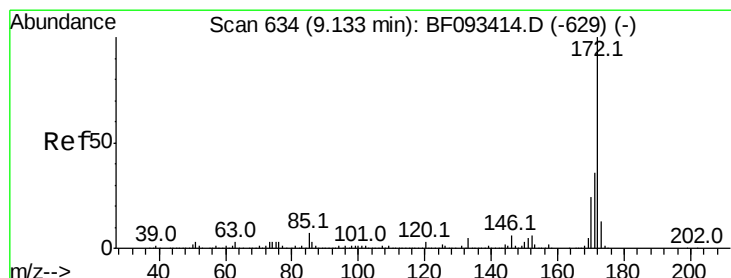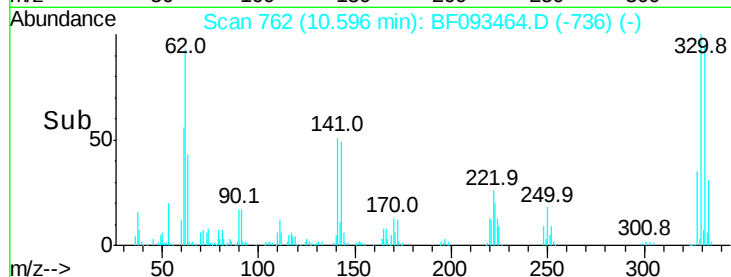
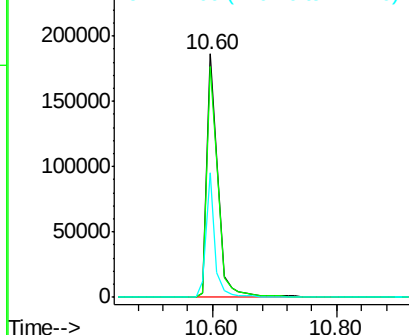



#44
 2-Fluorobiphenyl
 Concen: 114.66 ng
 RT: 9.13 min Scan# 634
 Delta R.T. -0.00 min
 Lab File: BF093464.D
 Acq: 9 Mar 2017 9:00

Tgt Ion:172 Resp: 1753626
 Ion Ratio Lower Upper
 172 100
 171 37.0 29.4 44.0
 170 25.0 20.2 30.4

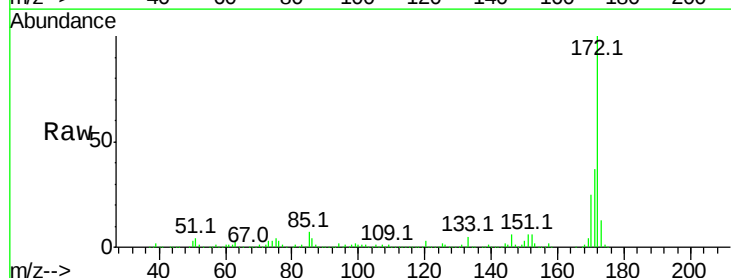

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

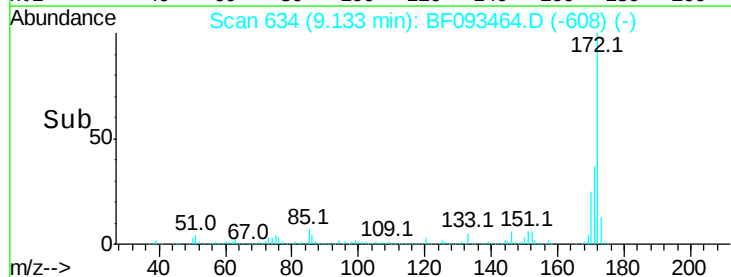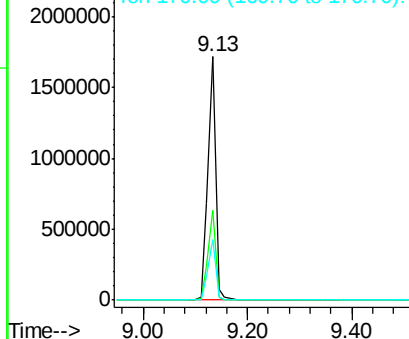


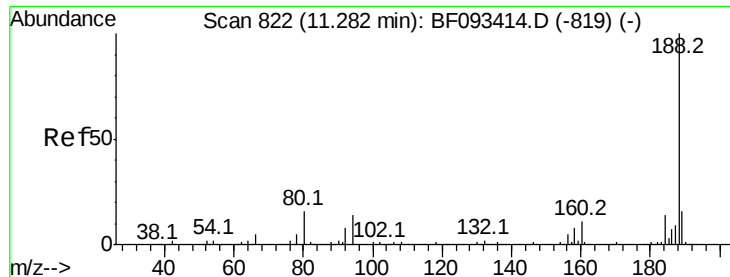




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.29 min Scan# 823
Delta R.T. 0.01 min
Lab File: BF093464.D
Acq: 9 Mar 2017 9:00

Instrument :
BNA_F
ClientSampled :
D-14

Tot Ion:188 Resp: 418757
Ion Ratio Lower Upper
188 100
94 9.1 10.0 15.0#
80 9.7 11.2 16.8#

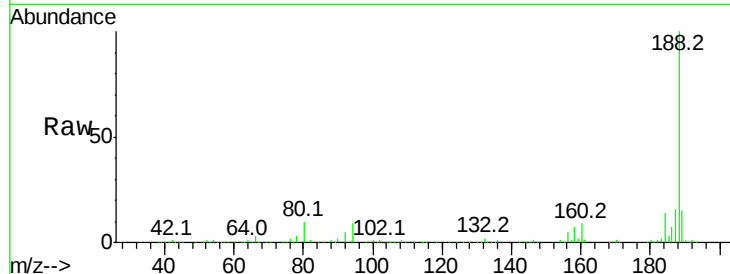


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

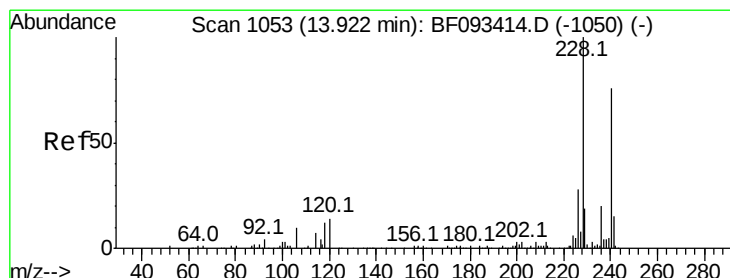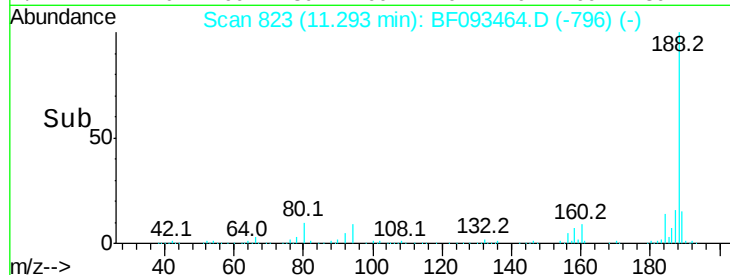
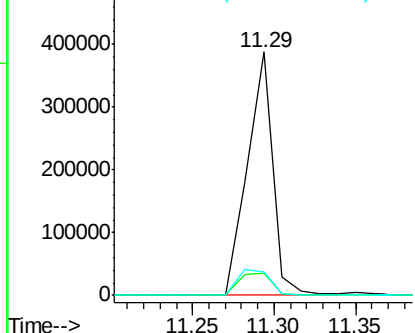


#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.93 min Scan# 1054
Delta R.T. 0.01 min
Lab File: BF093464.D
Acq: 9 Mar 2017 9:00

Tgt Ion:240 Resp: 366012
Ion Ratio Lower Upper
240 100
120 9.6 12.9 19.3#
236 26.0 20.9 31.3

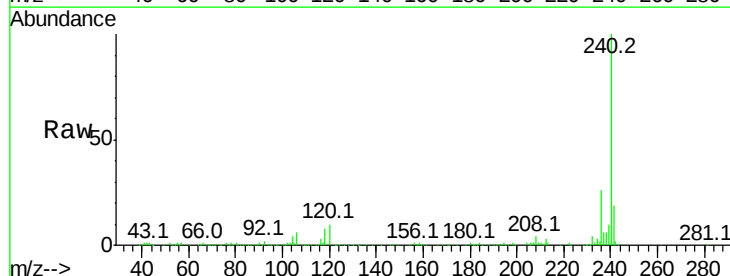

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

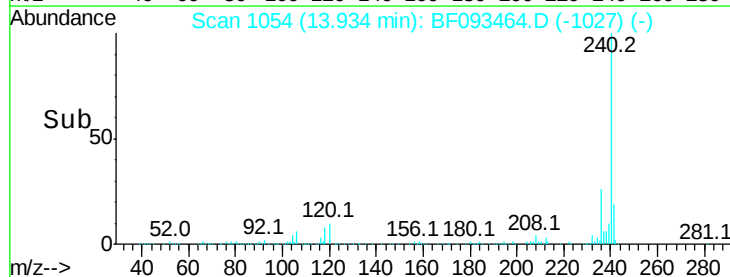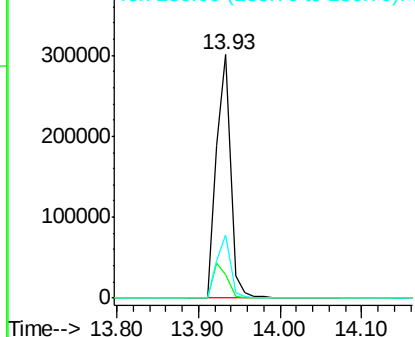



#78

Terphenyl-d14

Concen: 75.90 ng

RT: 12.87 min Scan# 961

Delta R.T. -0.00 min

Lab File: BF093464.D

Acq: 9 Mar 2017 9:00

Instrument :

BNA_F

ClientSampled :

D-14


Tot Ion:244 Resp: 1068489

Ion Ratio Lower Upper

244 100

212 7.7 6.2 9.2




122 15.1 11.4 17.2

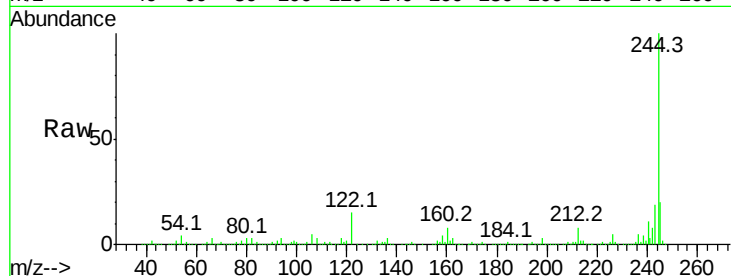

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

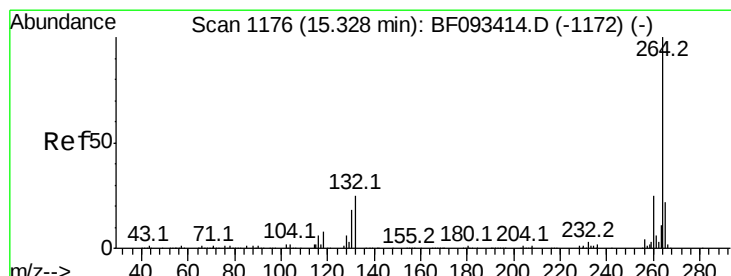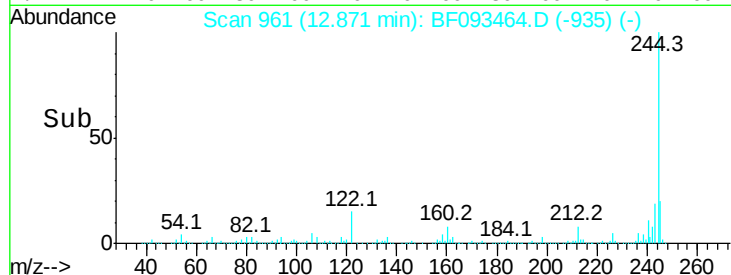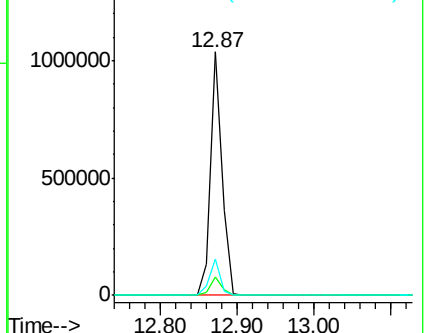

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.34 min Scan# 1177

Delta R.T. 0.01 min

Lab File: BF093464.D

Acq: 9 Mar 2017 9:00


Tgt Ion:264 Resp: 286605

Ion Ratio Lower Upper

264 100

260 23.5 19.2 28.8

265 20.8 17.4 26.0

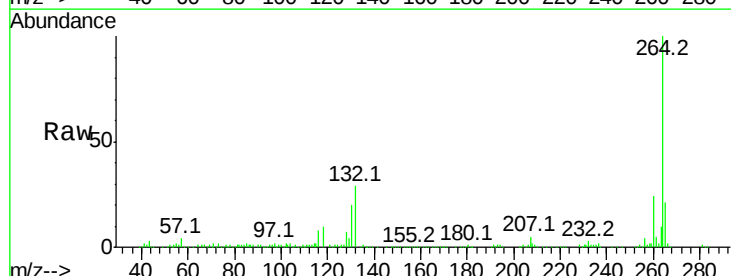

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

